

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073024\
 Data File : FB030850.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jul 2024 23:41
 Operator : YP/AJ
 Sample : P3390-07
 Misc : 1 PPB WATER LOD
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 31 06:36:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB073024.M
 Quant Title :
 QLast Update : Tue Jul 30 12:33:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	212082	18.011 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	23851	1.132 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	11232	0.527 ng/ml
3) t n-Heptane	7.747	8123	0.366 ng/ml
4) t Benzene	7.879	9241	0.350 ng/ml
6) t Toluene	10.614	27879	1.097 ng/ml
7) t Ethylbenzene	13.053	8618	0.365 ng/ml
8) t m-Xylene	13.187	16239	0.688 ng/ml
9) t O-Xylene	13.914	16793	0.729 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	19879	0.867 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073024\
Data File : FB030850.D
Signal(s) : FID2B.CH
Acq On : 30 Jul 2024 23:41
Operator : YP/AJ
Sample : P3390-07
Misc : 1 PPB WATER LOD
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 31 06:36:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB073024.M
Quant Title :
QLast Update : Tue Jul 30 12:33:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

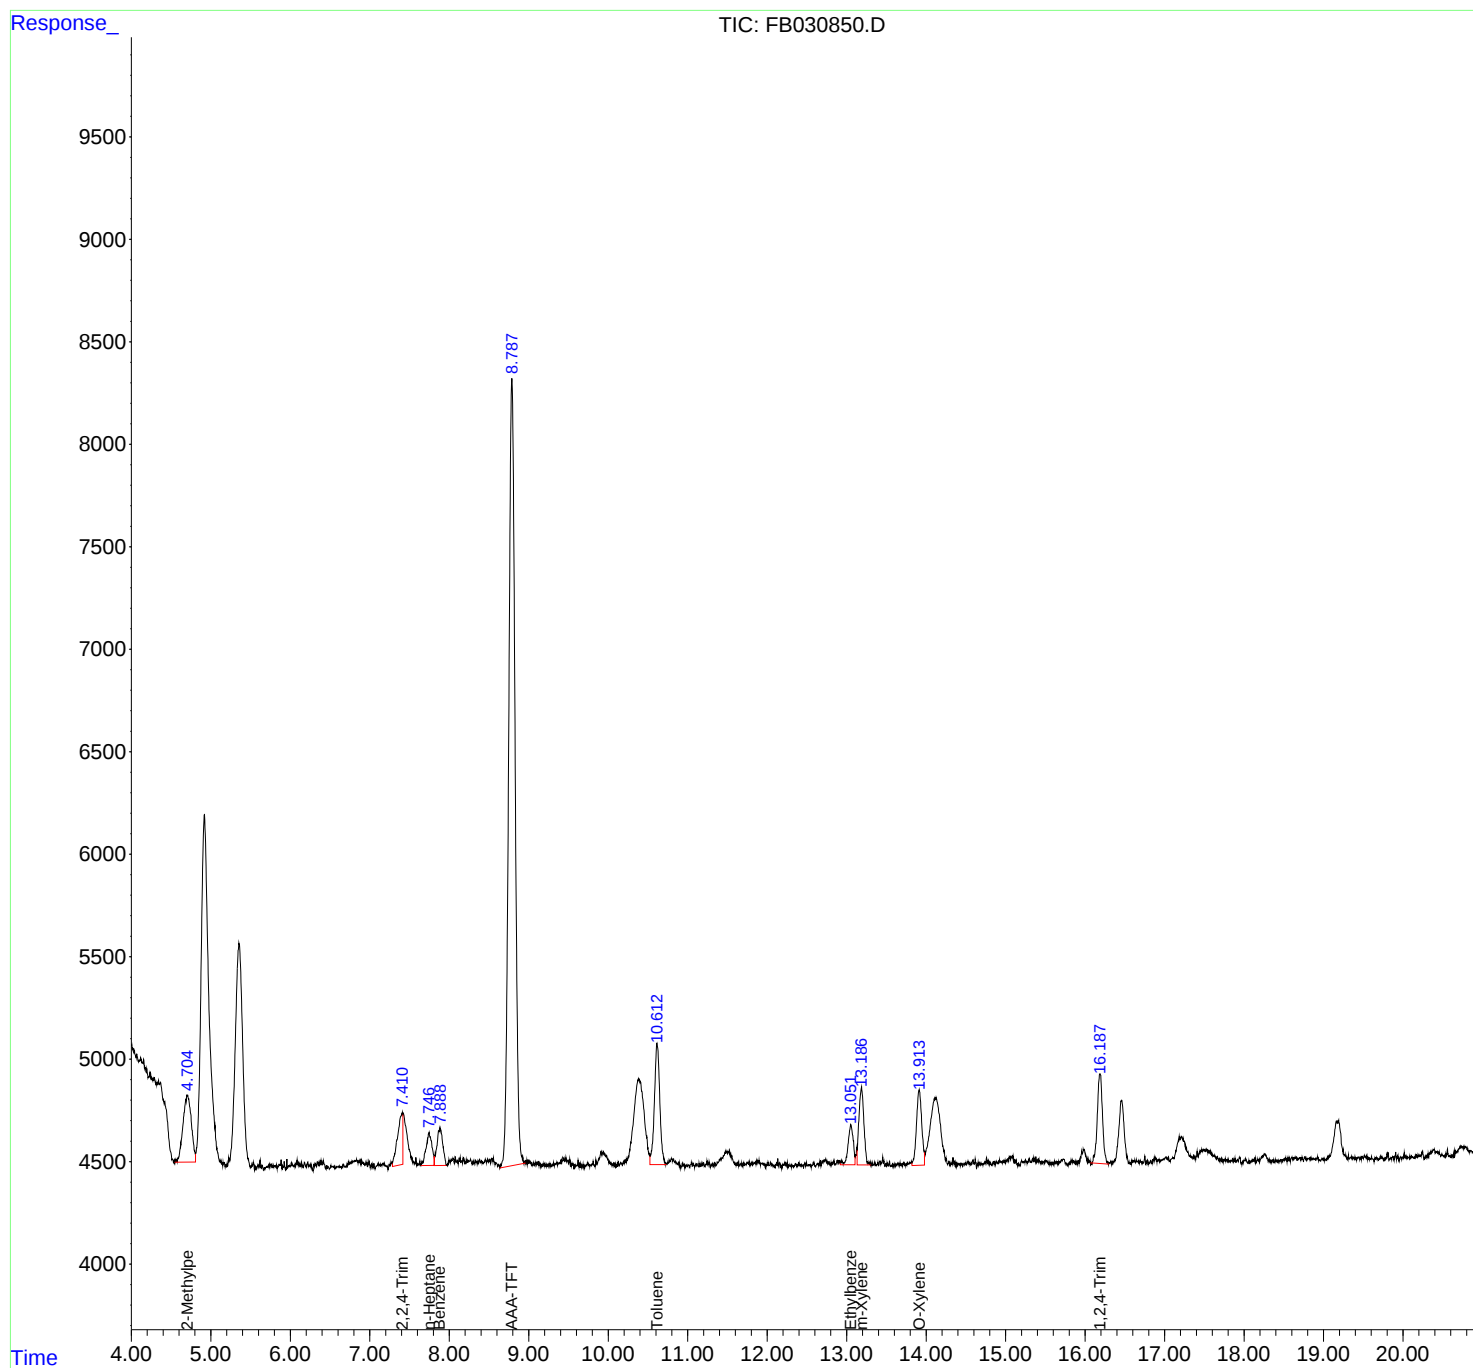


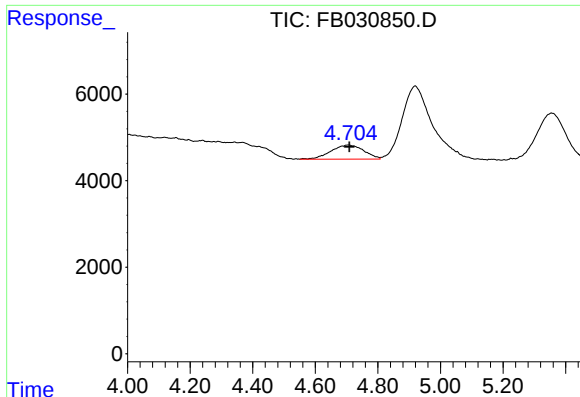

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 23851
Conc: 1.13 ng/ml

Instrument :
FID_B
ClientSampleId :

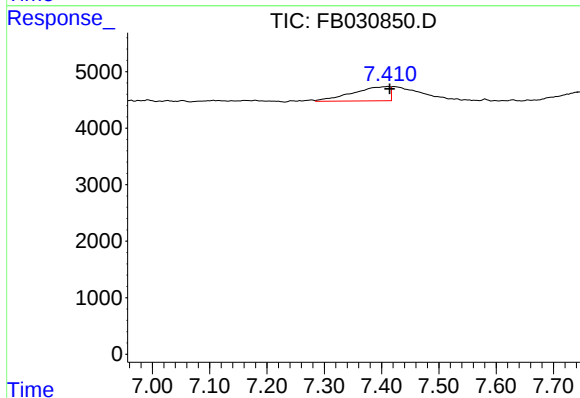


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.003 min
Response: 11232
Conc: 0.53 ng/ml

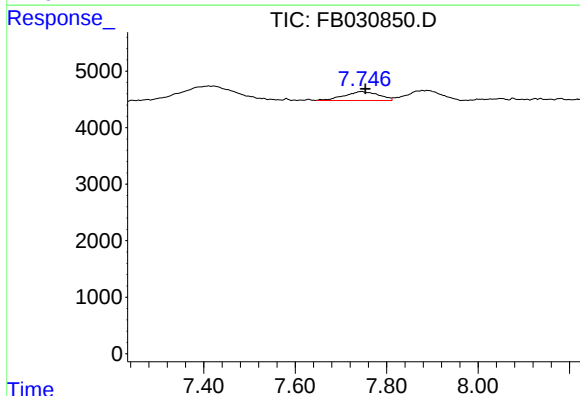


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.007 min
Response: 8123
Conc: 0.37 ng/ml

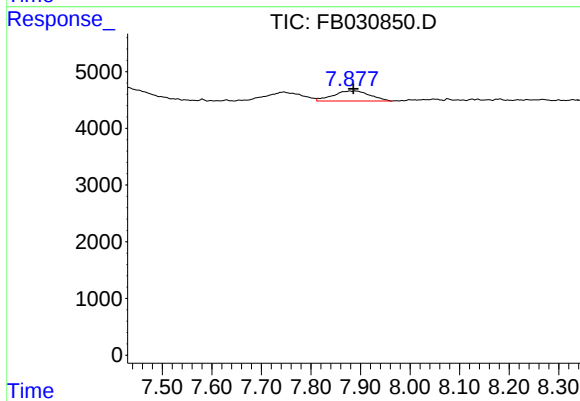

#4 Benzene


R.T.: 7.879 min
Delta R.T.: -0.006 min
Response: 9241
Conc: 0.35 ng/ml

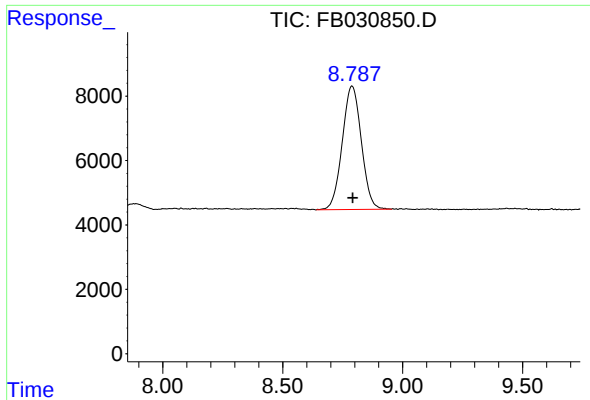

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 212082
Conc: 18.01 ng/ml

Instrument :
FID_B
ClientSampleId :

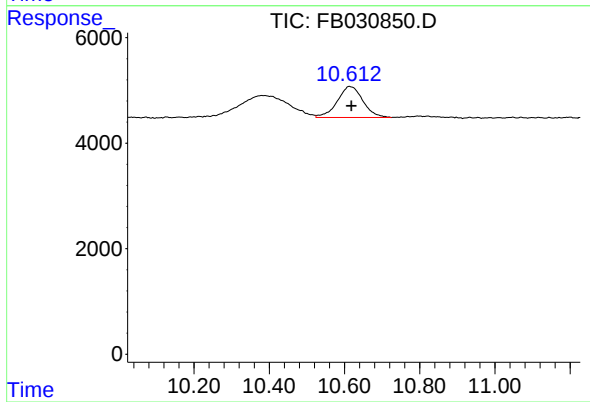


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.005 min
Response: 27879
Conc: 1.10 ng/ml

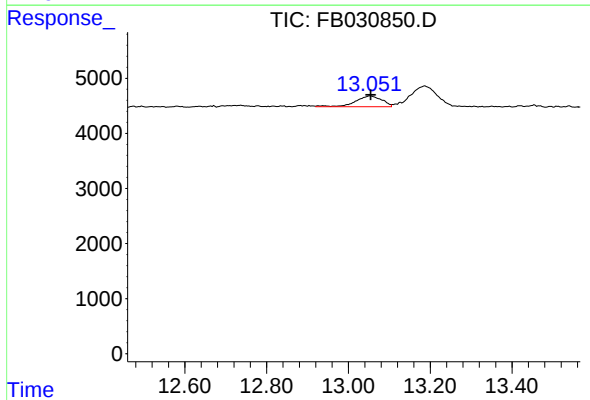


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.002 min
Response: 8618
Conc: 0.36 ng/ml

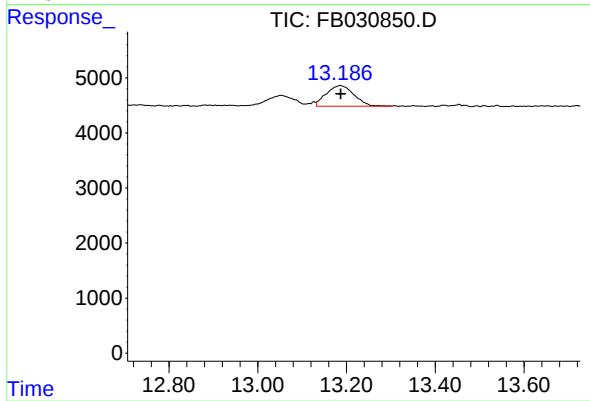

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.000 min
Response: 16239
Conc: 0.69 ng/ml

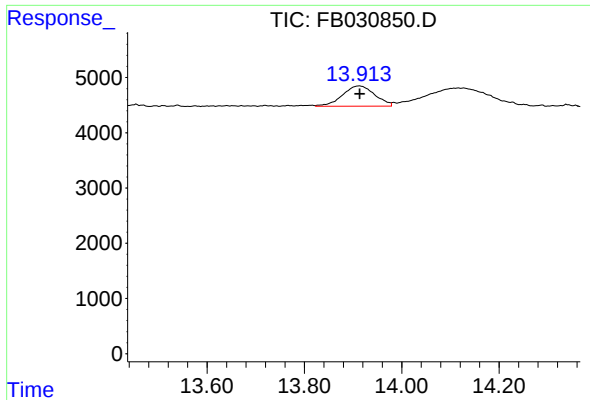

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.000 min
Response: 16793
Conc: 0.73 ng/ml

Instrument :
FID_B
ClientSampleId :

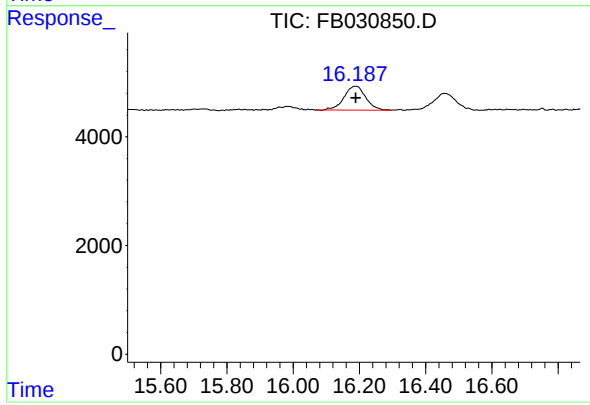

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.000 min
Response: 19879
Conc: 0.87 ng/ml