

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB073118\  
 Data File : FB017022.D  
 Signal(s) : FID2B.CH  
 Acq On : 31 Jul 2018 14:02  
 Operator : MJ/SJ  
 Sample : J4231-15 50X  
 Misc : 5.00g/5.00ml DI water  
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e  
 Quant Time: Jul 31 15:50:27 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072718.M  
 Quant Title :  
 QLast Update : Fri Jul 27 13:23:50 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 9.112  | 183924   | 23.118 ng/ml |
| Target Compounds             |        |          |              |
| 7) t Ethylbenzene            | 13.412 | 70772    | 5.157 ng/ml  |
| 8) t m-Xylene                | 13.542 | 22768    | 1.569 ng/ml  |
| 9) t O-Xylene                | 14.281 | 17626    | 1.146 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.560 | 88724    | 4.757 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB073118\  
Data File : FB017022.D  
Signal(s) : FID2B.CH  
Acq On : 31 Jul 2018 14:02  
Operator : MJ/SJ  
Sample : J4231-15 50X  
Misc : 5.00g/5.00ml DI water  
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jul 31 15:50:27 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072718.M  
Quant Title :  
QLast Update : Fri Jul 27 13:23:50 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

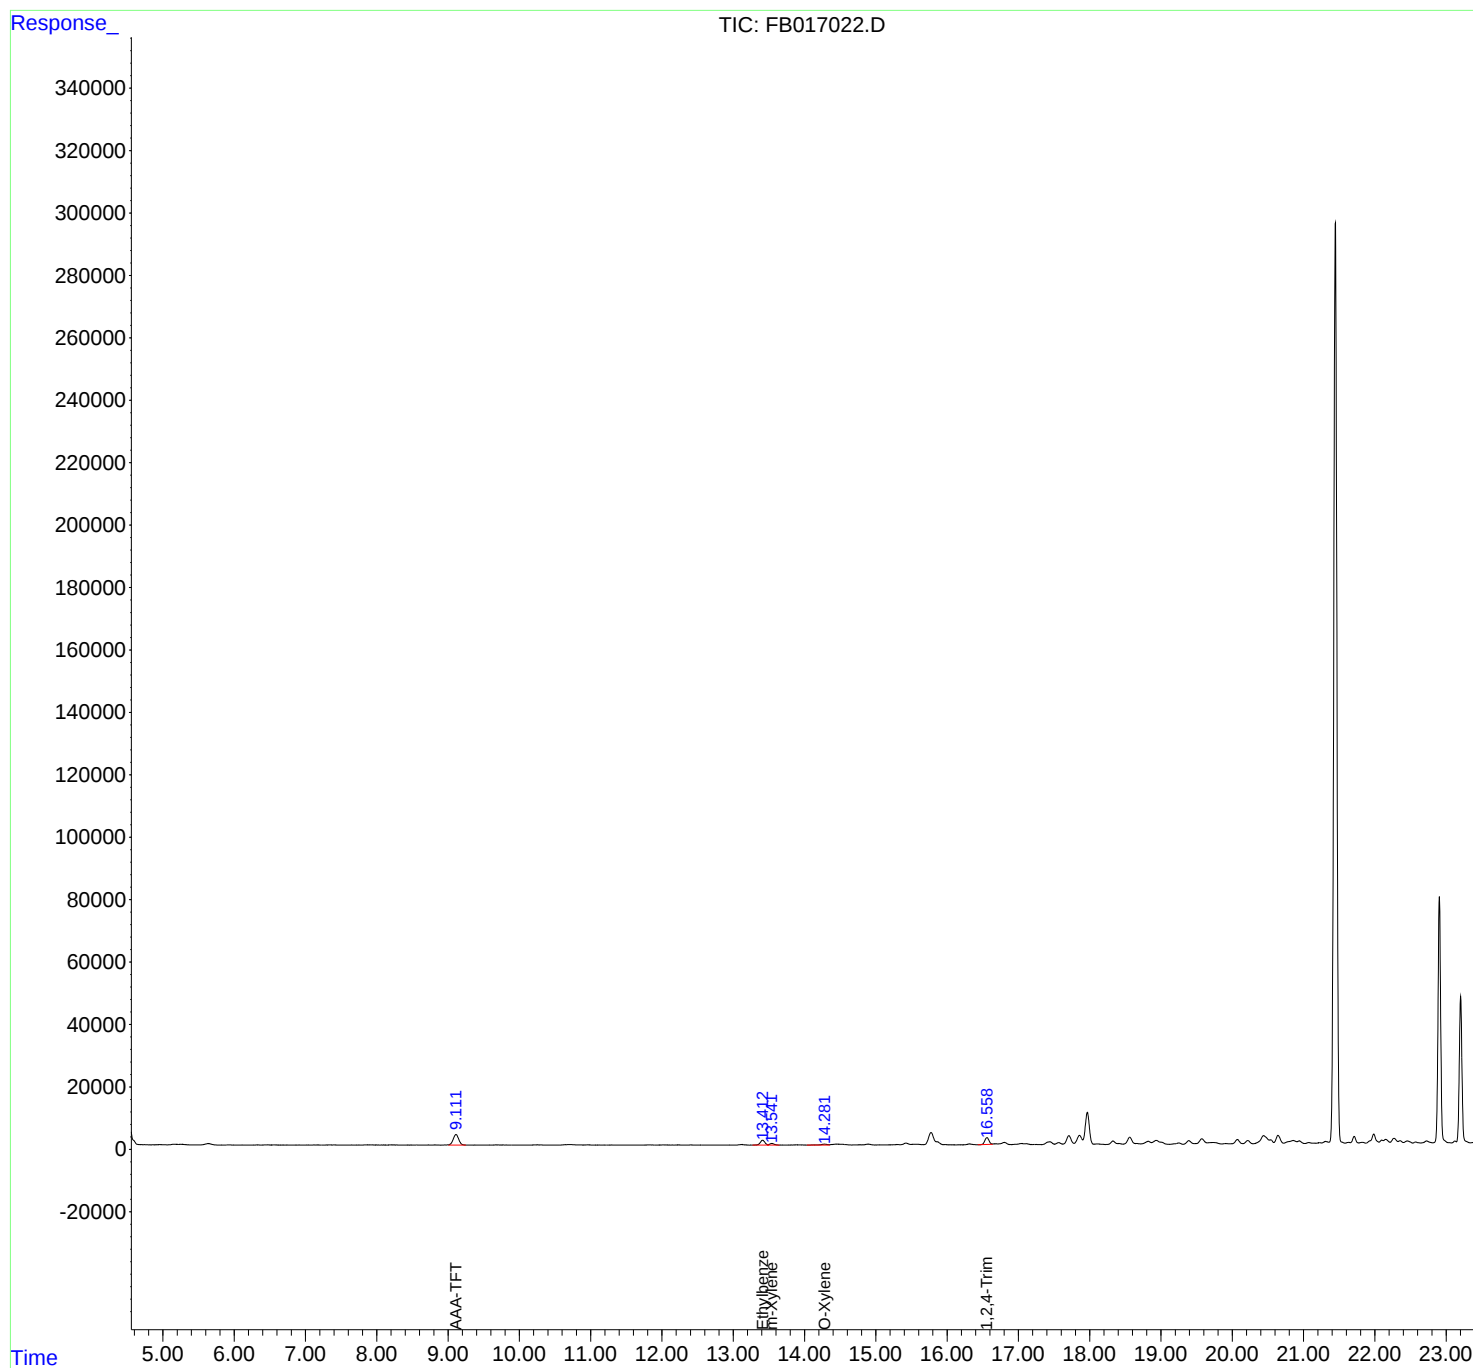

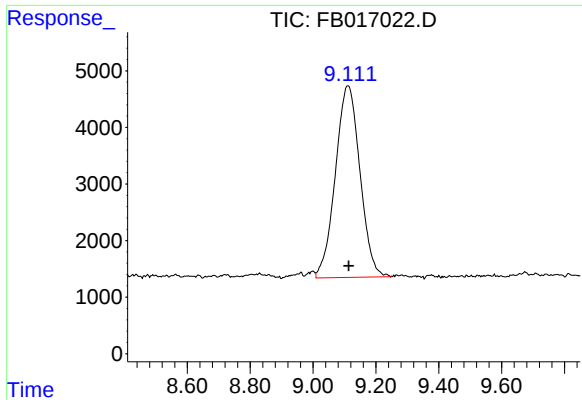


#5 AAA-TFT

R.T.: 9.112 min  
Delta R.T.: -0.002 min  
Response: 183924  
Conc: 23.12 ng/ml

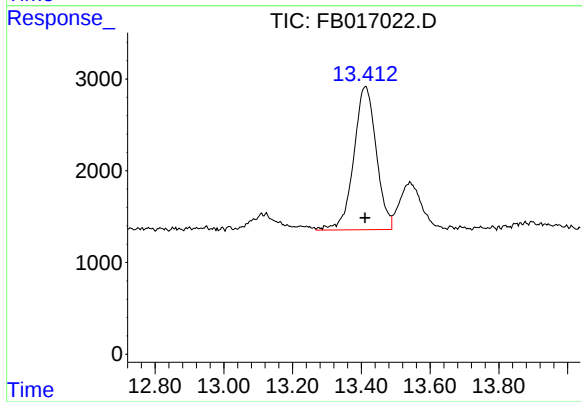


#7 Ethylbenzene

R.T.: 13.412 min  
Delta R.T.: 0.000 min  
Response: 70772  
Conc: 5.16 ng/ml

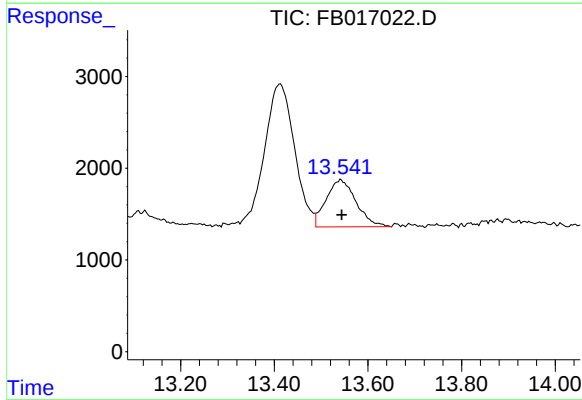


#8 m-Xylene

R.T.: 13.542 min  
Delta R.T.: -0.002 min  
Response: 22768  
Conc: 1.57 ng/ml

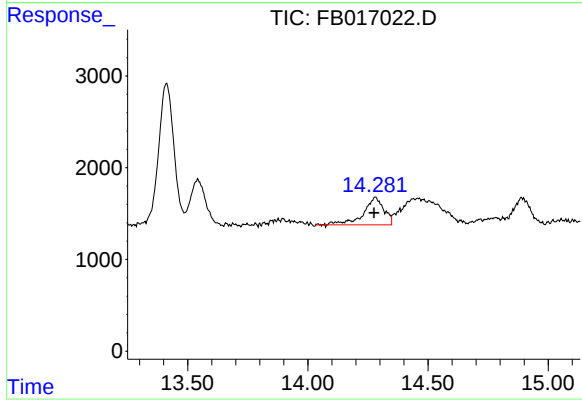

#9 O-Xylene

R.T.: 14.281 min  
Delta R.T.: 0.005 min  
Response: 17626  
Conc: 1.15 ng/ml

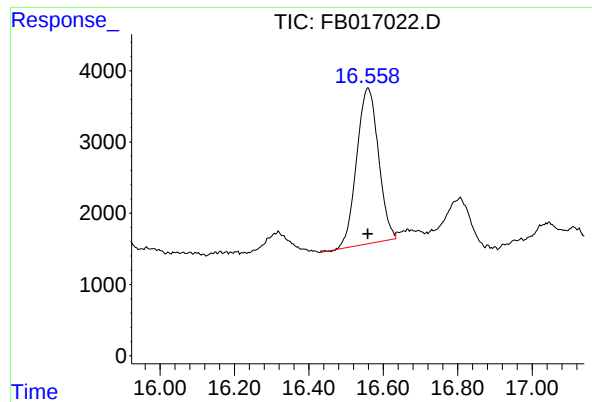

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min  
Delta R.T.: 0.001 min  
Response: 88724  
Conc: 4.76 ng/ml