

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073118\
Data File : FB017020.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 13:00
Operator : MJ/SJ
Sample : J4189-02 MSD
Misc : 5.03g/5.00ml DI water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 31 15:50:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	162637	20.442 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	382604	26.895 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	383570	27.962 ng/ml
3) t n-Heptane	8.067	122352	8.761 ng/ml
4) t Benzene	8.208	161862	9.241 ng/ml
6) t Toluene	10.962	403768	29.763 ng/ml
7) t Ethylbenzene	13.411	131648	9.593 ng/ml
8) t m-Xylene	13.544	278525	19.200 ng/ml
9) t O-Xylene	14.276	295809	19.227 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	352861	18.919 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073118\
Data File : FB017020.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2018 13:00
Operator : MJ/SJ
Sample : J4189-02 MSD
Misc : 5.03g/5.00ml DI water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 31 15:50:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

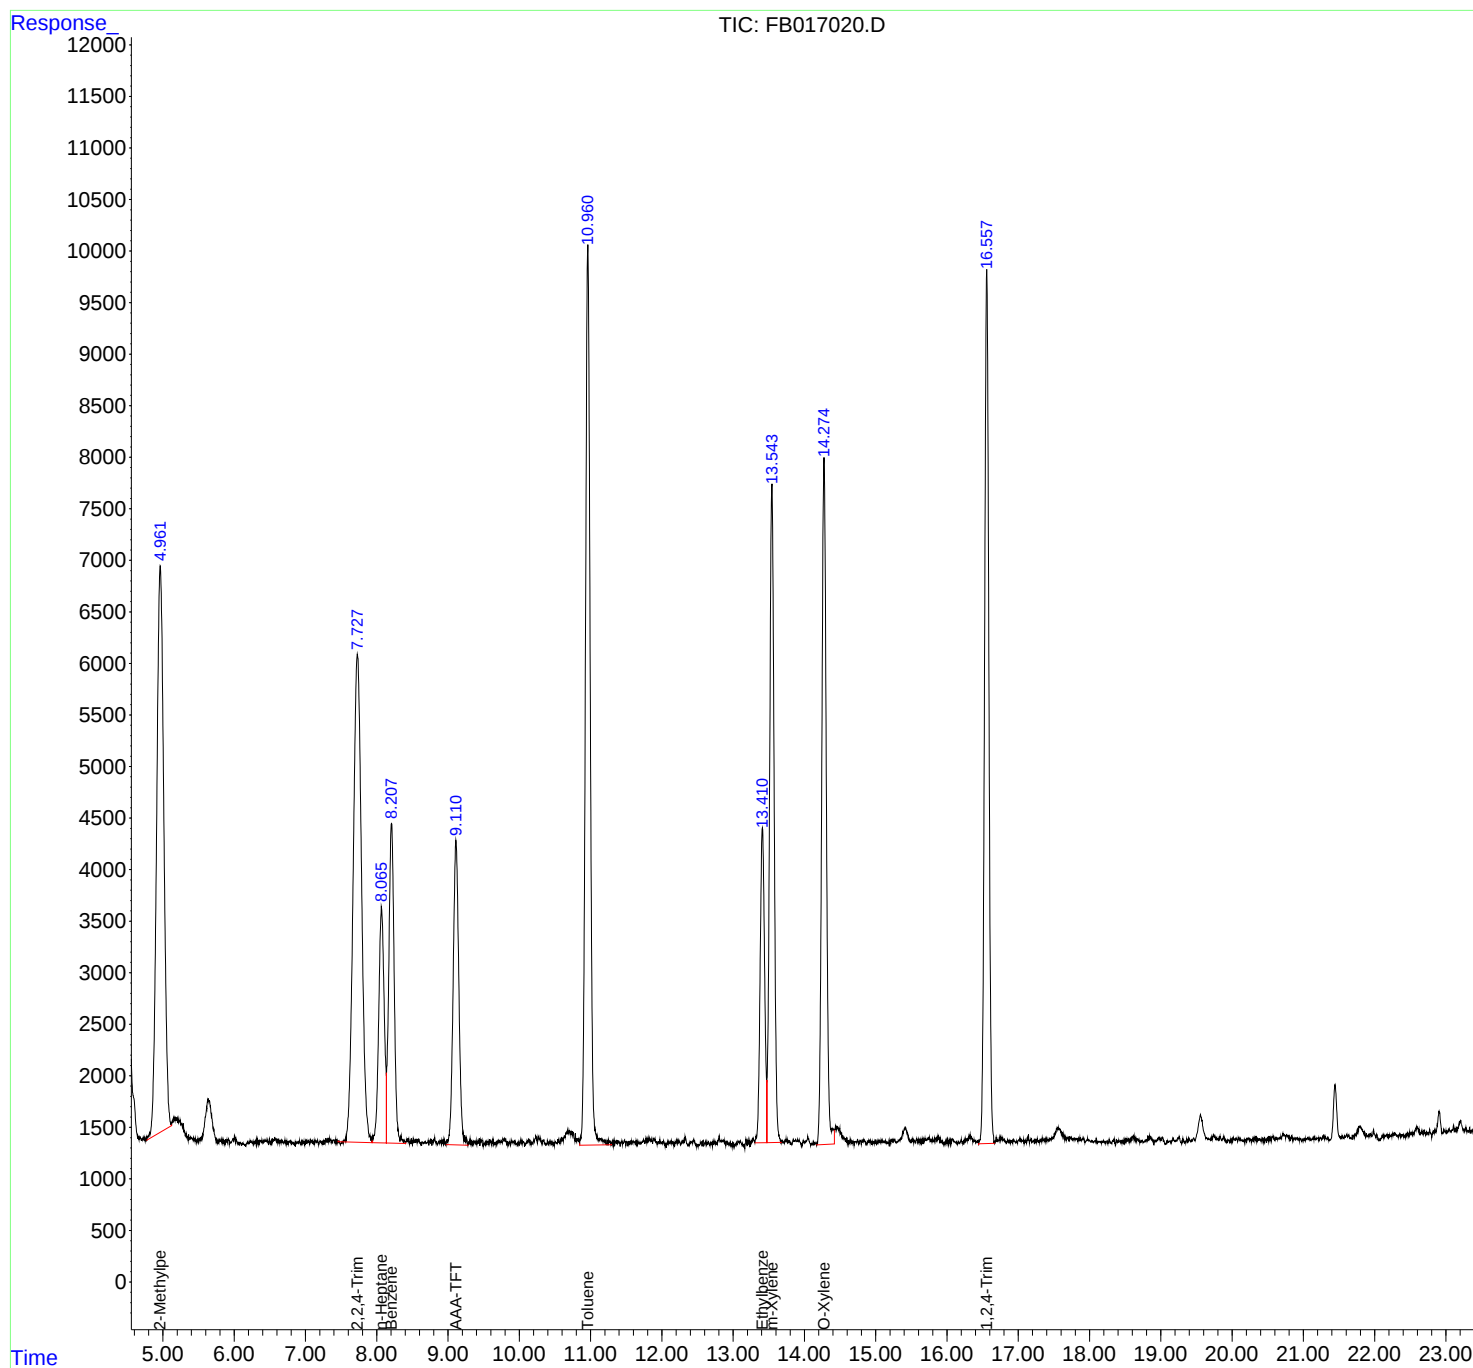

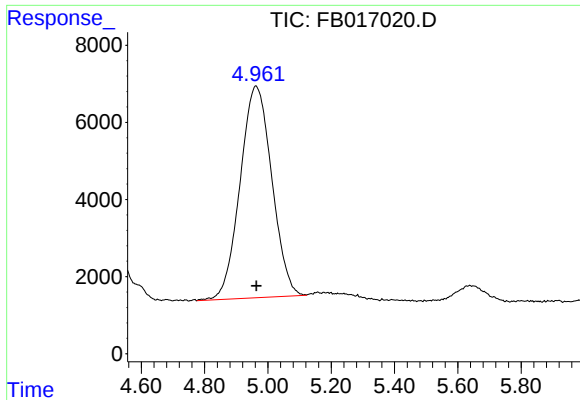


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: -0.001 min
Response: 382604
Conc: 26.89 ng/ml

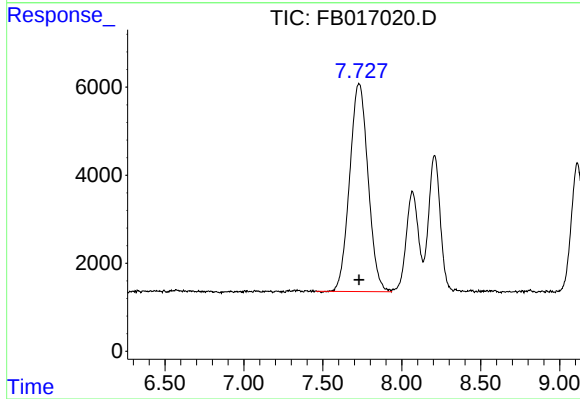


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: -0.001 min
Response: 383570
Conc: 27.96 ng/ml

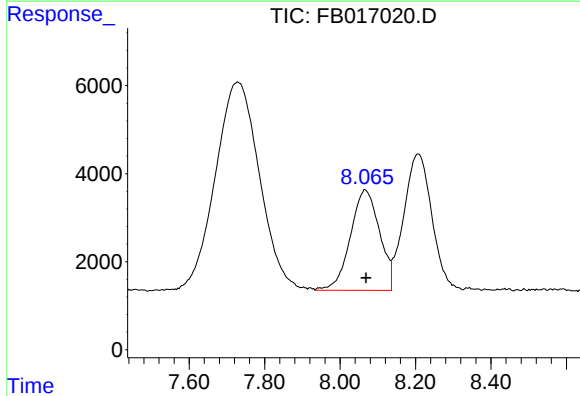


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: -0.001 min
Response: 122352
Conc: 8.76 ng/ml

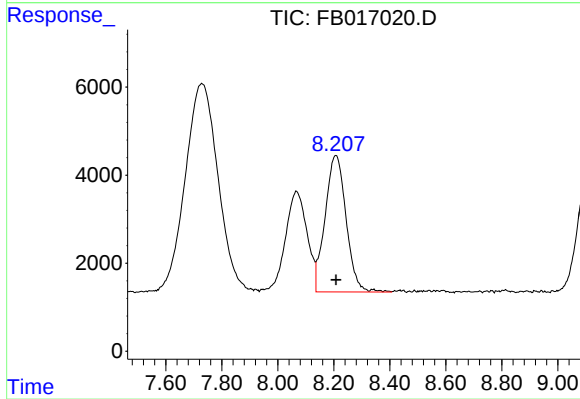


#4 Benzene

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 161862
Conc: 9.24 ng/ml

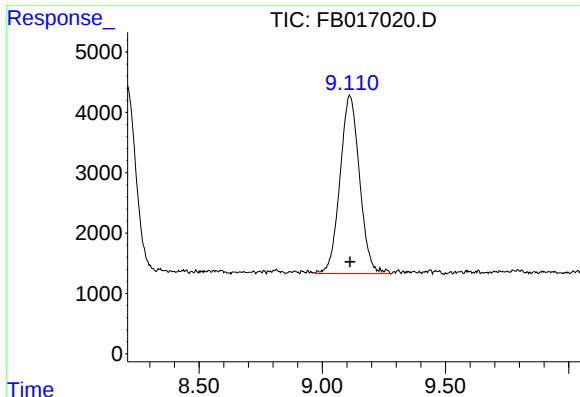


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: -0.002 min
Response: 162637
Conc: 20.44 ng/ml

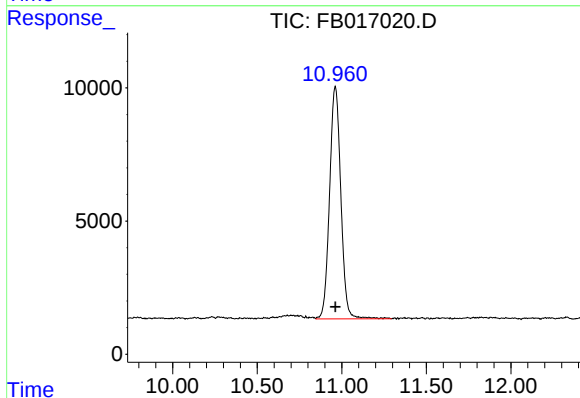


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.000 min
Response: 403768
Conc: 29.76 ng/ml

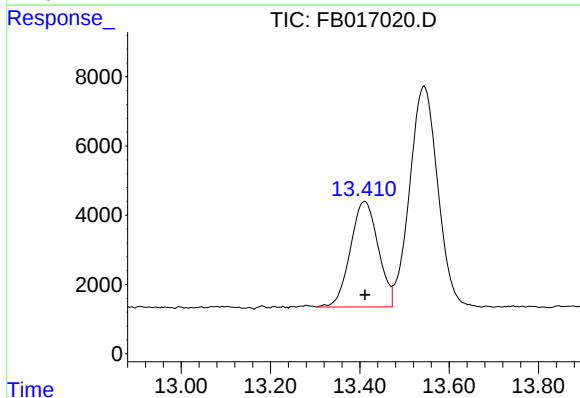


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 131648
Conc: 9.59 ng/ml

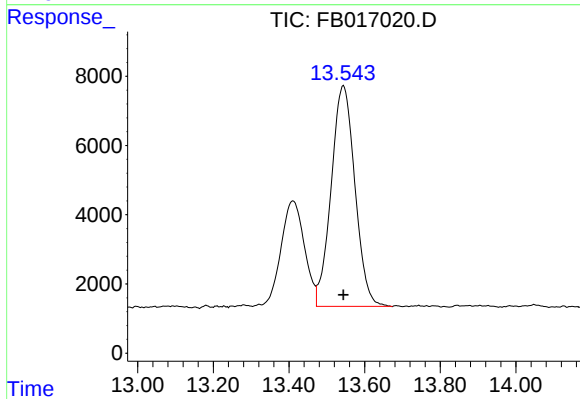


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 278525
Conc: 19.20 ng/ml

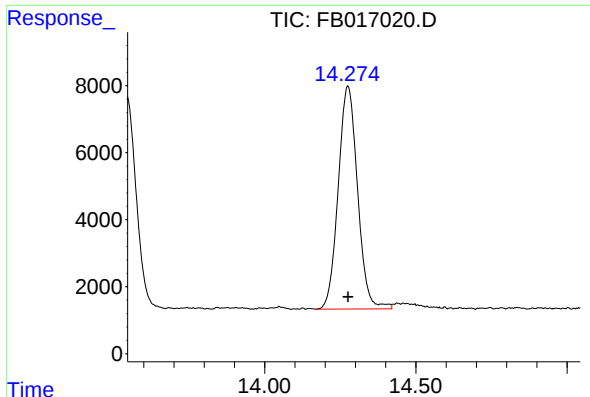

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 295809
Conc: 19.23 ng/ml

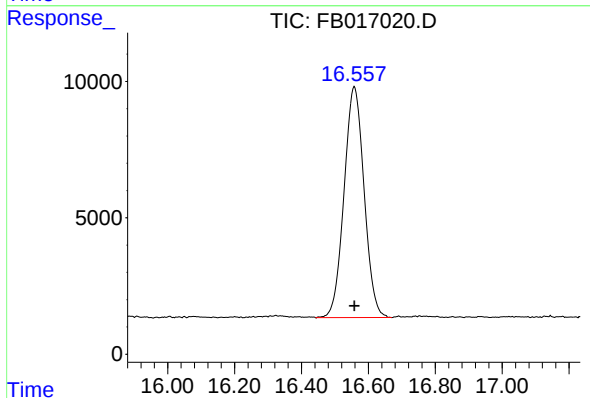

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 352861
Conc: 18.92 ng/ml