

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073119\
 Data File : FB021884.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jul 2019 11:13
 Operator : DD/AJ
 Sample : BSF0731S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 01 00:55:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	295403	21.647 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	773392	28.046 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	829431	31.377 ng/ml
3) t n-Heptane	7.949	254286	10.256 ng/ml
4) t Benzene	8.084	294611	10.084 ng/ml
6) t Toluene	10.830	613030	29.793 ng/ml
7) t Ethylbenzene	13.275	208624	10.028 ng/ml
8) t m-Xylene	13.407	440219	19.816 ng/ml
9) t O-Xylene	14.137	457217	19.877 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	488008	20.699 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073119\
Data File : FB021884.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2019 11:13
Operator : DD/AJ
Sample : BSF0731S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 01 00:55:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

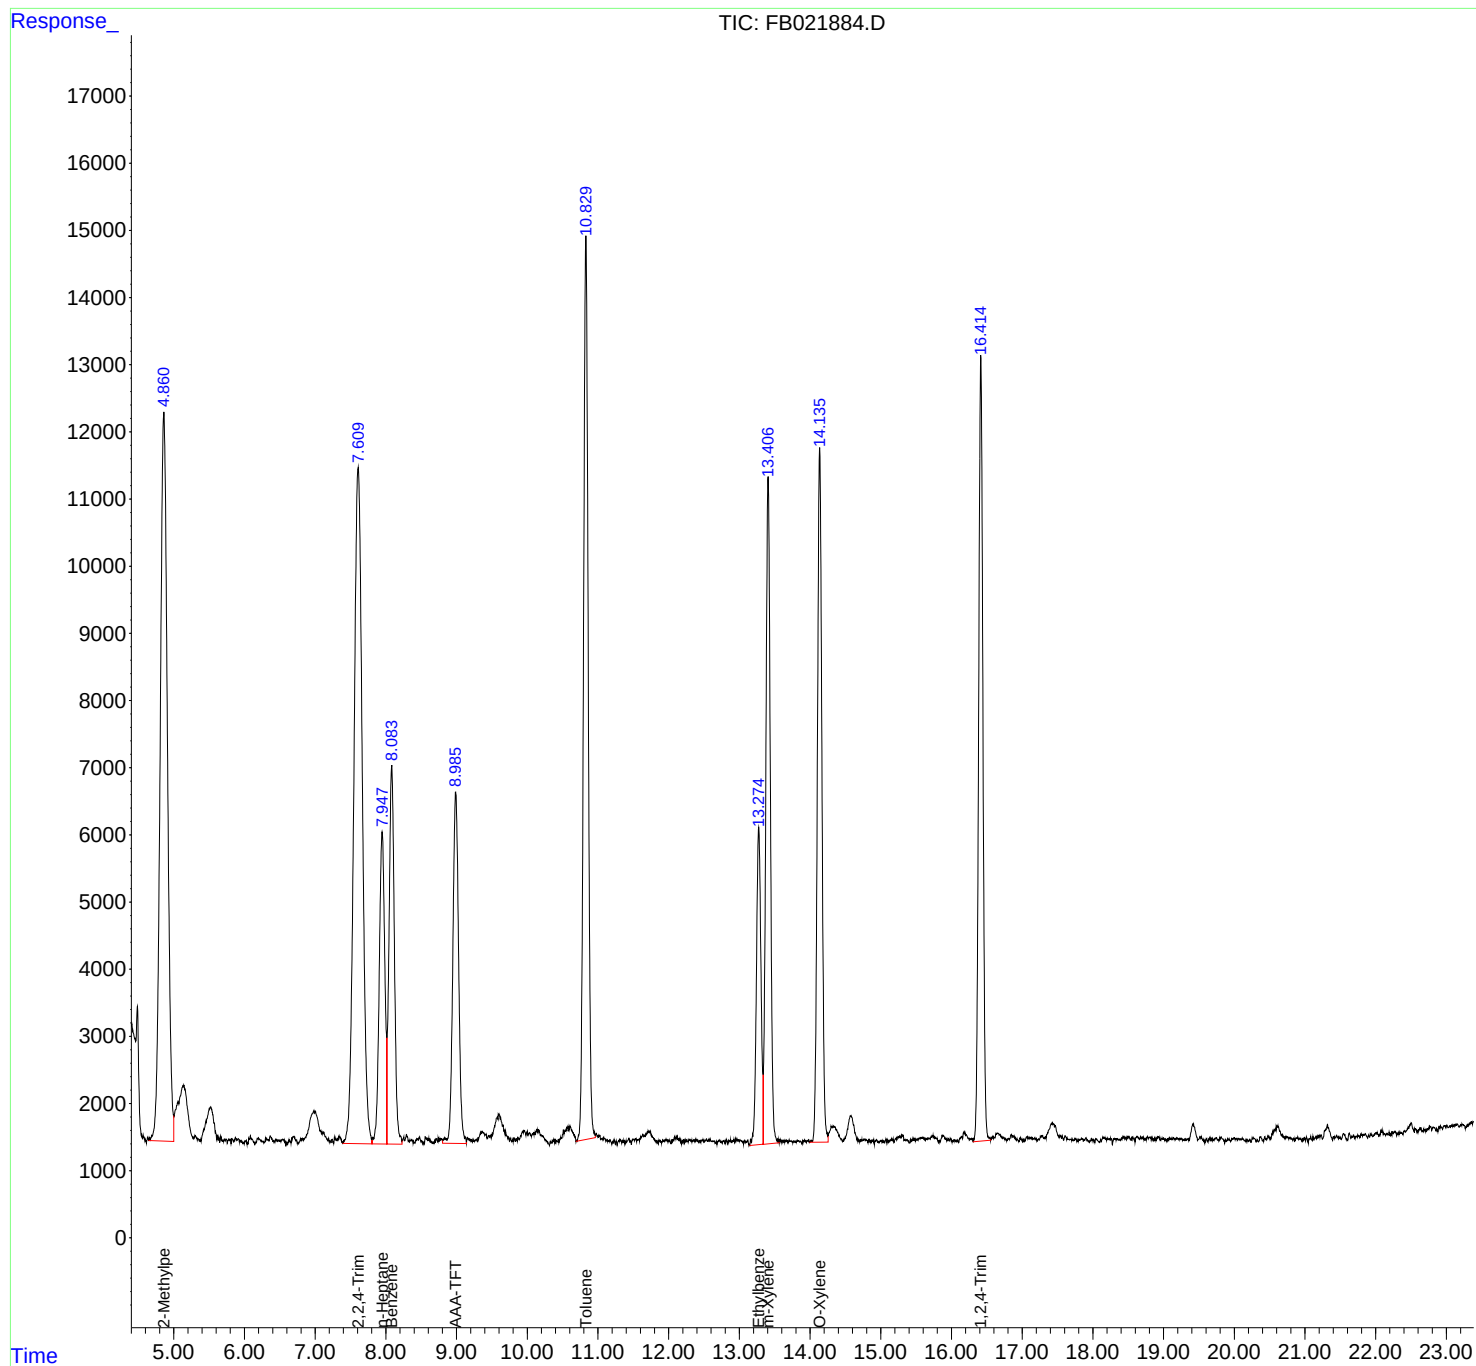

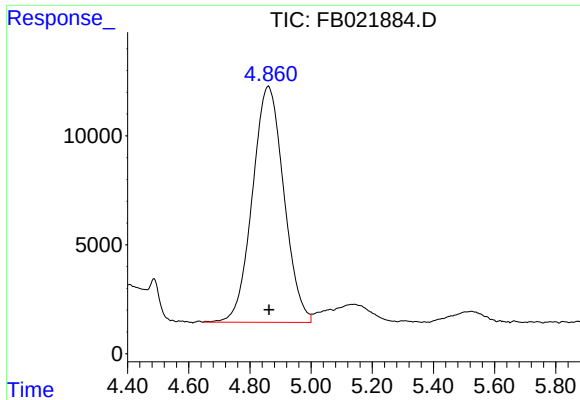


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 773392
Conc: 28.05 ng/ml

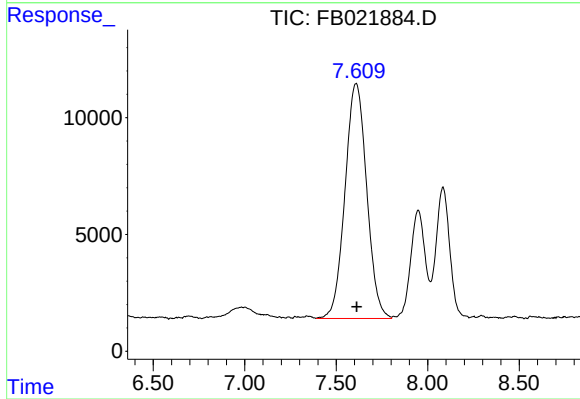


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 829431
Conc: 31.38 ng/ml

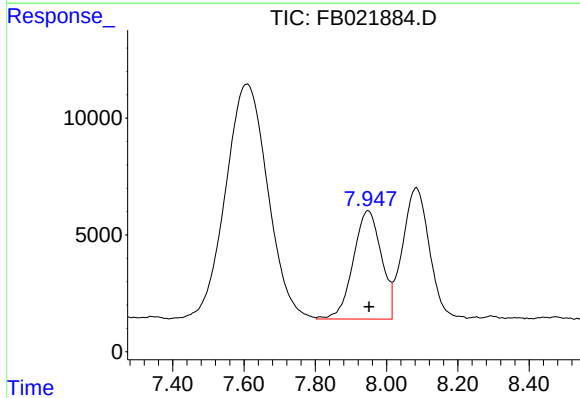


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.003 min
Response: 254286
Conc: 10.26 ng/ml

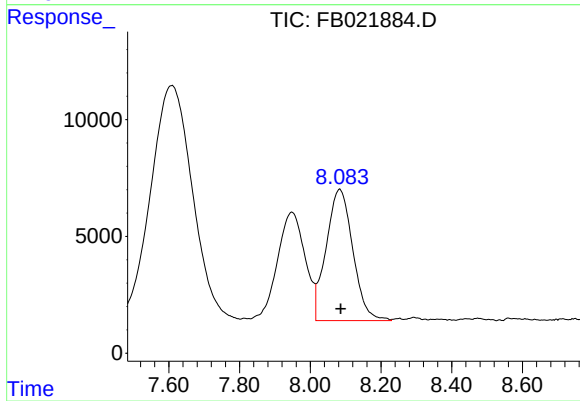


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 294611
Conc: 10.08 ng/ml

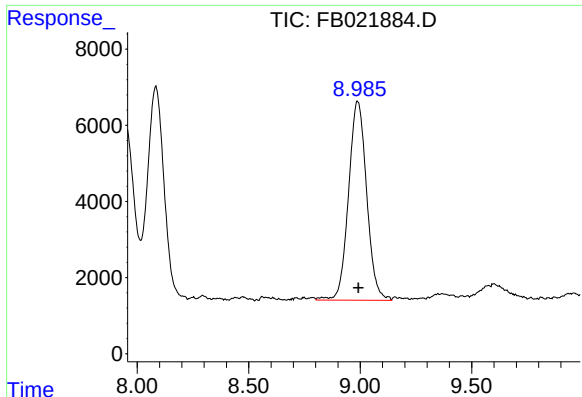


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 295403
Conc: 21.65 ng/ml

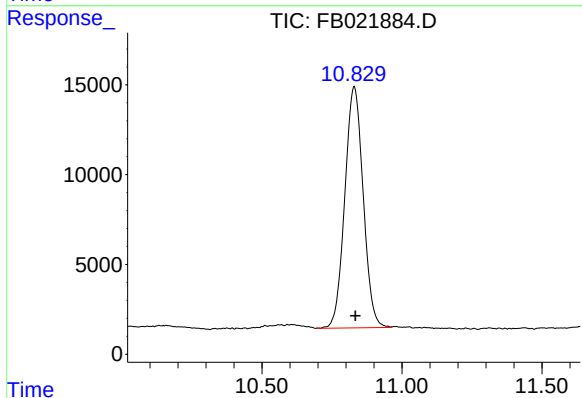


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 613030
Conc: 29.79 ng/ml

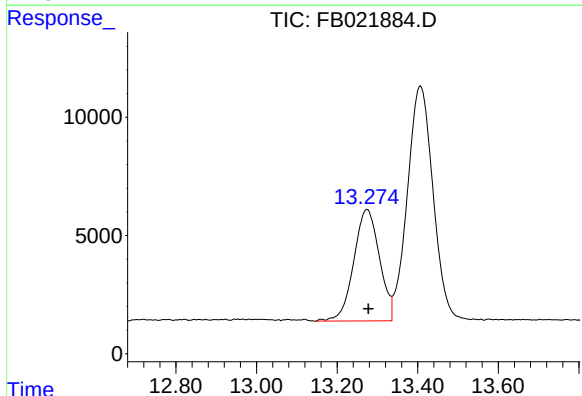


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: -0.003 min
Response: 208624
Conc: 10.03 ng/ml

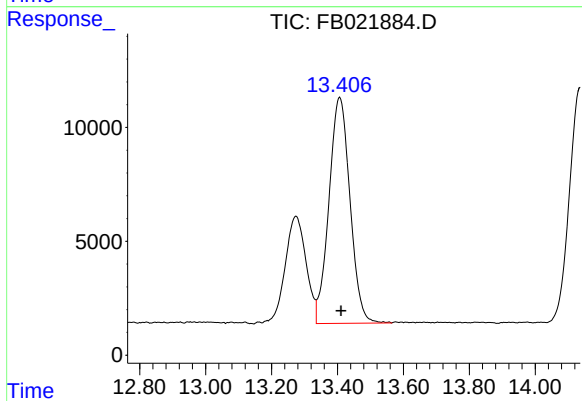


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.003 min
Response: 440219
Conc: 19.82 ng/ml

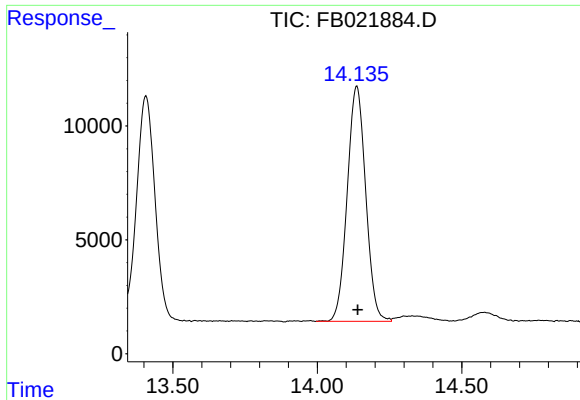

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.004 min
Response: 457217
Conc: 19.88 ng/ml

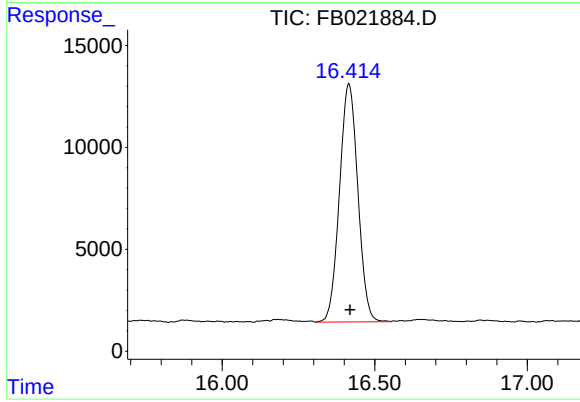

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.004 min
Response: 488008
Conc: 20.70 ng/ml