

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073119\
 Data File : FB021887.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jul 2019 14:01
 Operator : DD/AJ
 Sample : K3618-09MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 01 00:56:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	297127	21.773 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	681472	24.712 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	649095	24.555 ng/ml
3) t n-Heptane	7.953	191790	7.735 ng/ml
4) t Benzene	8.089	280230	9.592 ng/ml
6) t Toluene	10.835	578827	28.131 ng/ml
7) t Ethylbenzene	13.280	192136	9.235 ng/ml
8) t m-Xylene	13.413	397218	17.880 ng/ml
9) t O-Xylene	14.142	425723	18.508 ng/ml
10) t 1,2,4-Trimethylbenzene	16.421	389660	16.527 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073119\
Data File : FB021887.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2019 14:01
Operator : DD/AJ
Sample : K3618-09MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 01 00:56:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

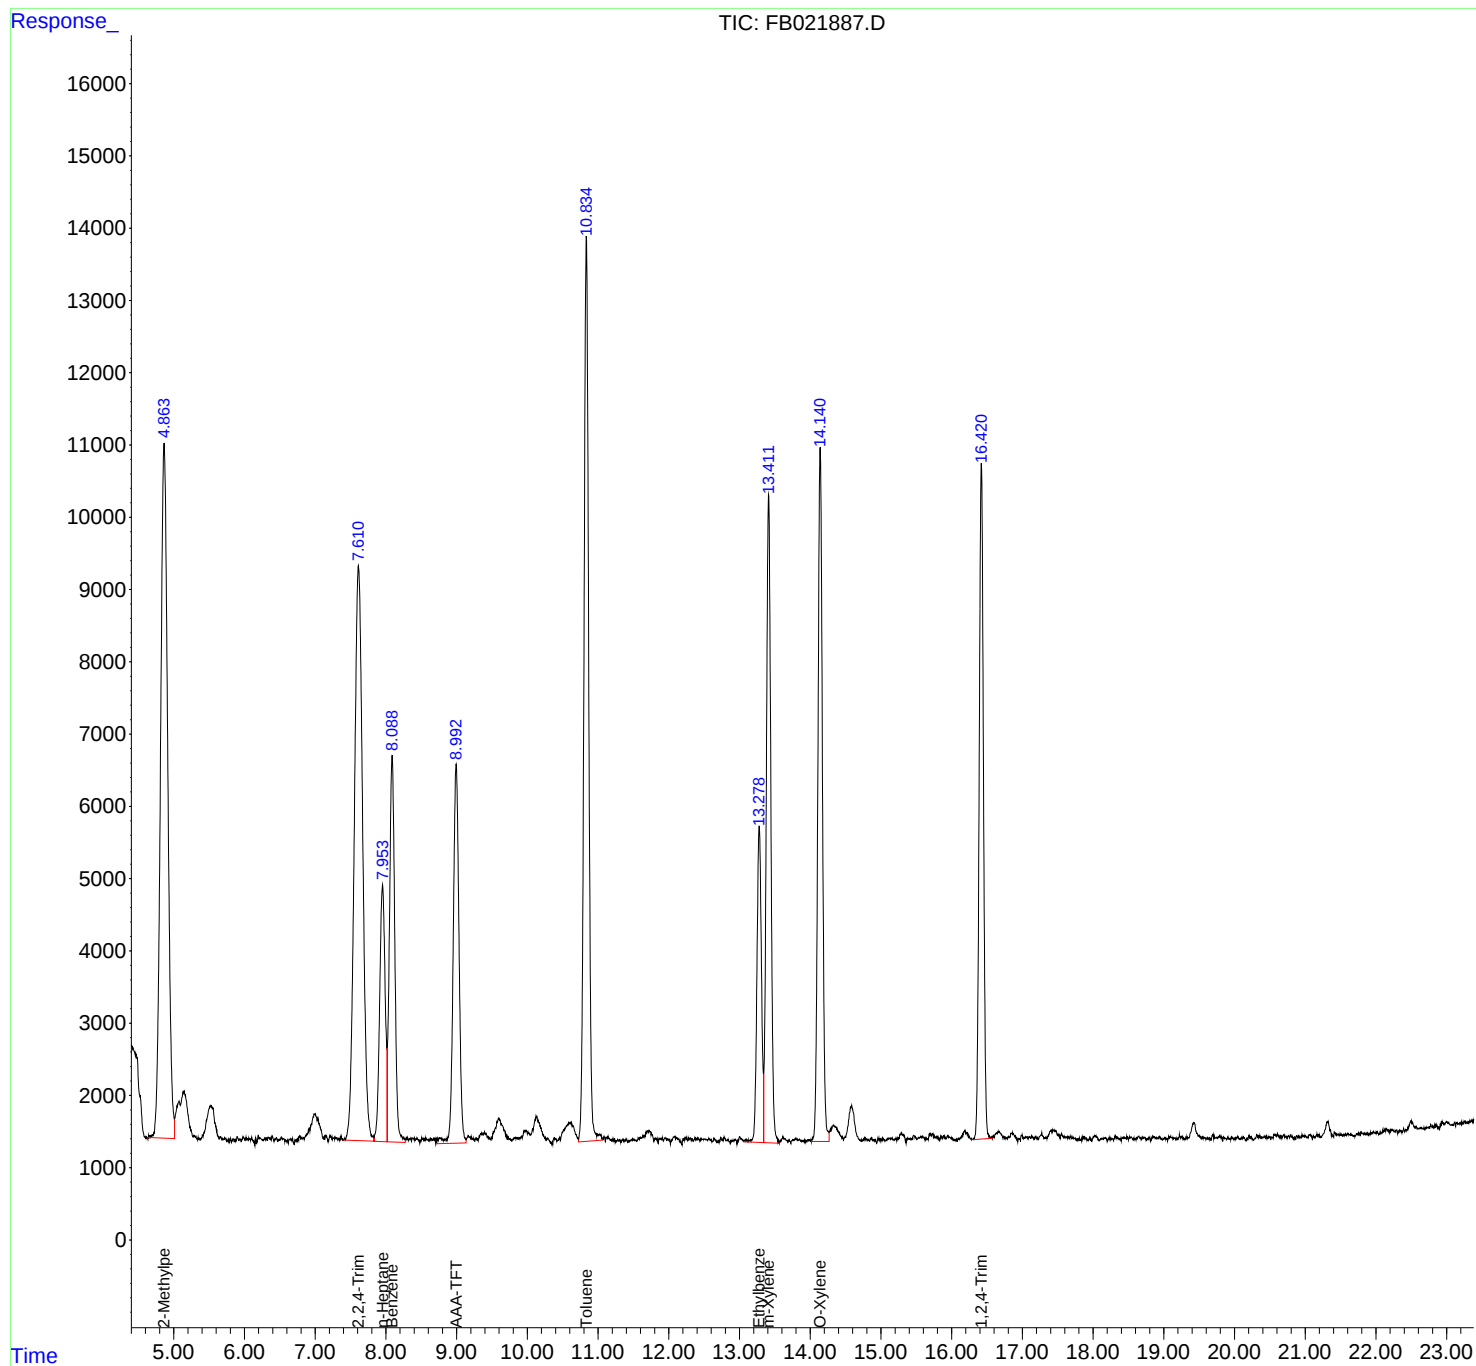

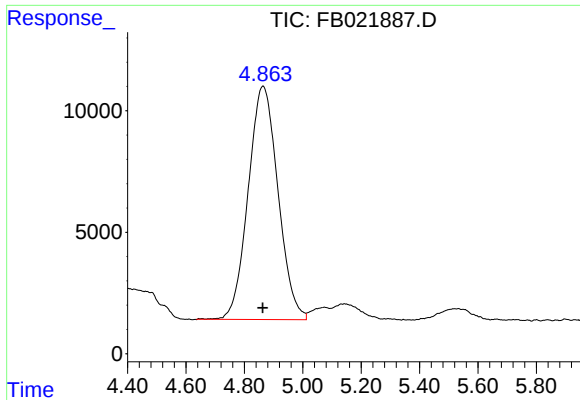


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 681472
Conc: 24.71 ng/ml

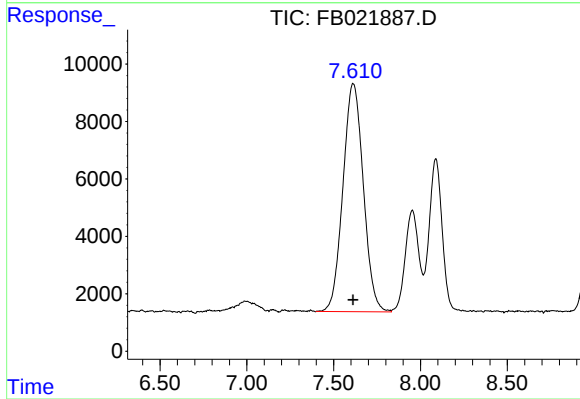


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 649095
Conc: 24.55 ng/ml

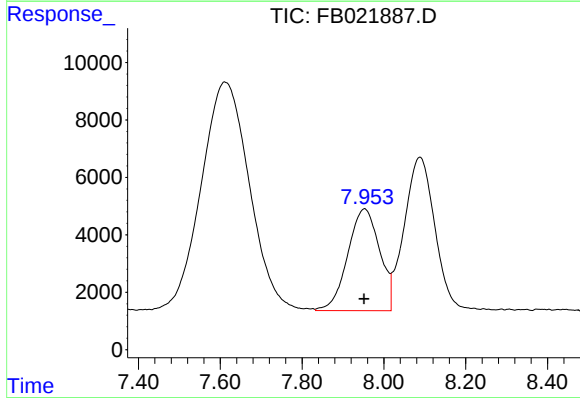


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 191790
Conc: 7.74 ng/ml

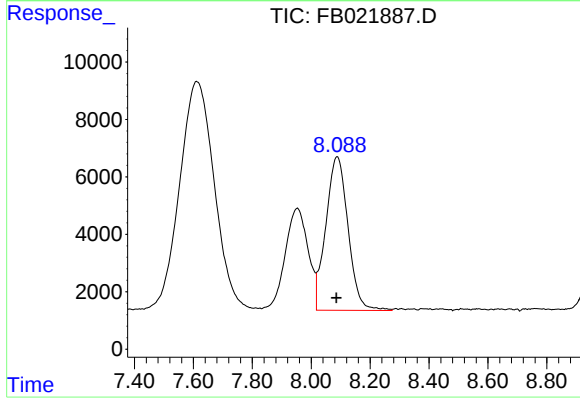


#4 Benzene

R.T.: 8.089 min
Delta R.T.: 0.003 min
Response: 280230
Conc: 9.59 ng/ml

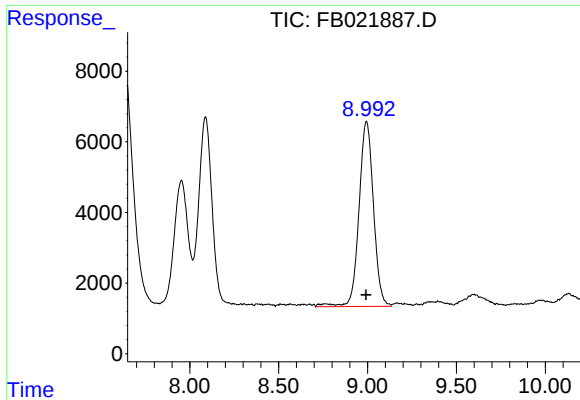


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 297127
Conc: 21.77 ng/ml

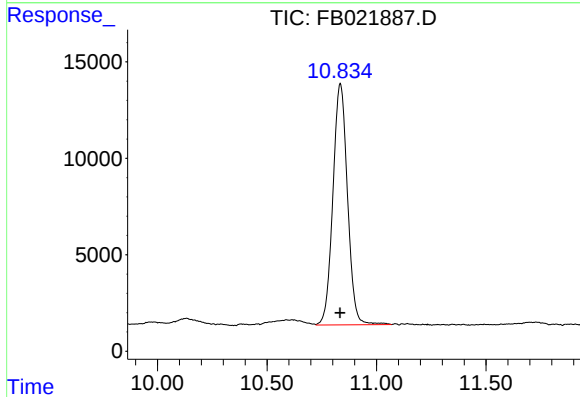


#6 Toluene

R.T.: 10.835 min
Delta R.T.: 0.002 min
Response: 578827
Conc: 28.13 ng/ml

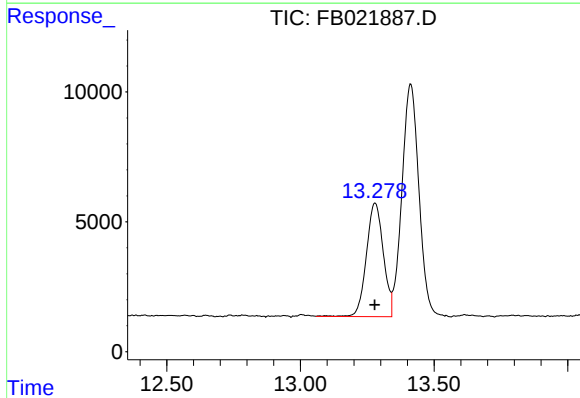


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 192136
Conc: 9.24 ng/ml

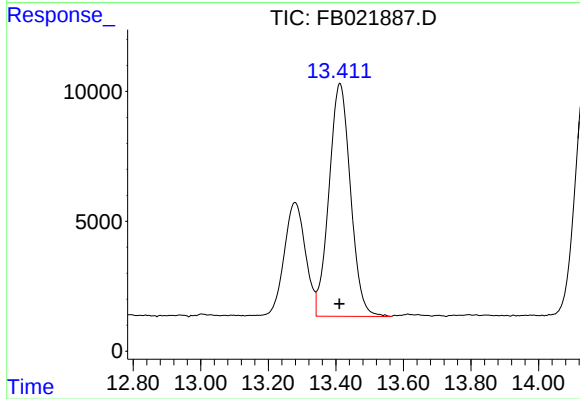

#8 m-Xylene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 397218
Conc: 17.88 ng/ml

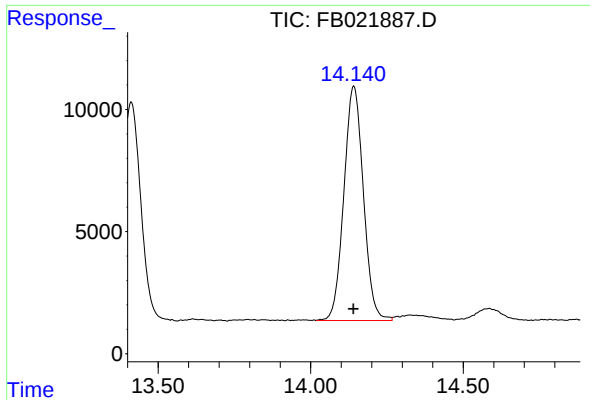


#9 O-Xylene

R.T.: 14.142 min

Delta R.T.: 0.001 min

Response: 425723

Conc: 18.51 ng/ml

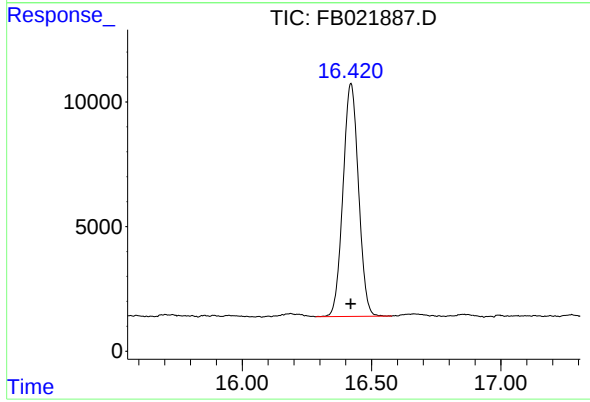

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min

Delta R.T.: 0.001 min

Response: 389660

Conc: 16.53 ng/ml