

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073123\
 Data File : FB030221.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jul 2023 9:40
 Operator : YP/AJ
 Sample : 20 PPB GRO CCC
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 31 15:34:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	260058	21.158 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	407005	24.638 ng/ml
2) t 2,2,4-Trimethylpentane	7.406	428472	23.090 ng/ml
3) t n-Heptane	7.742	152348	7.919 ng/ml
4) t Benzene	7.878	196492	8.353 ng/ml
6) t Toluene	10.609	576589	25.160 ng/ml
7) t Ethylbenzene	13.046	183905	8.569 ng/ml
8) t m-Xylene	13.178	357996	17.023 ng/ml
9) t O-Xylene	13.905	352840	17.192 ng/ml
10) t 1,2,4-Trimethylbenzene	16.180	366545	18.727 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB073123\
Data File : FB030221.D
Signal(s) : FID2B.CH
Acq On : 31 Jul 2023 9:40
Operator : YP/AJ
Sample : 20 PPB GRO CCC
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 31 15:34:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

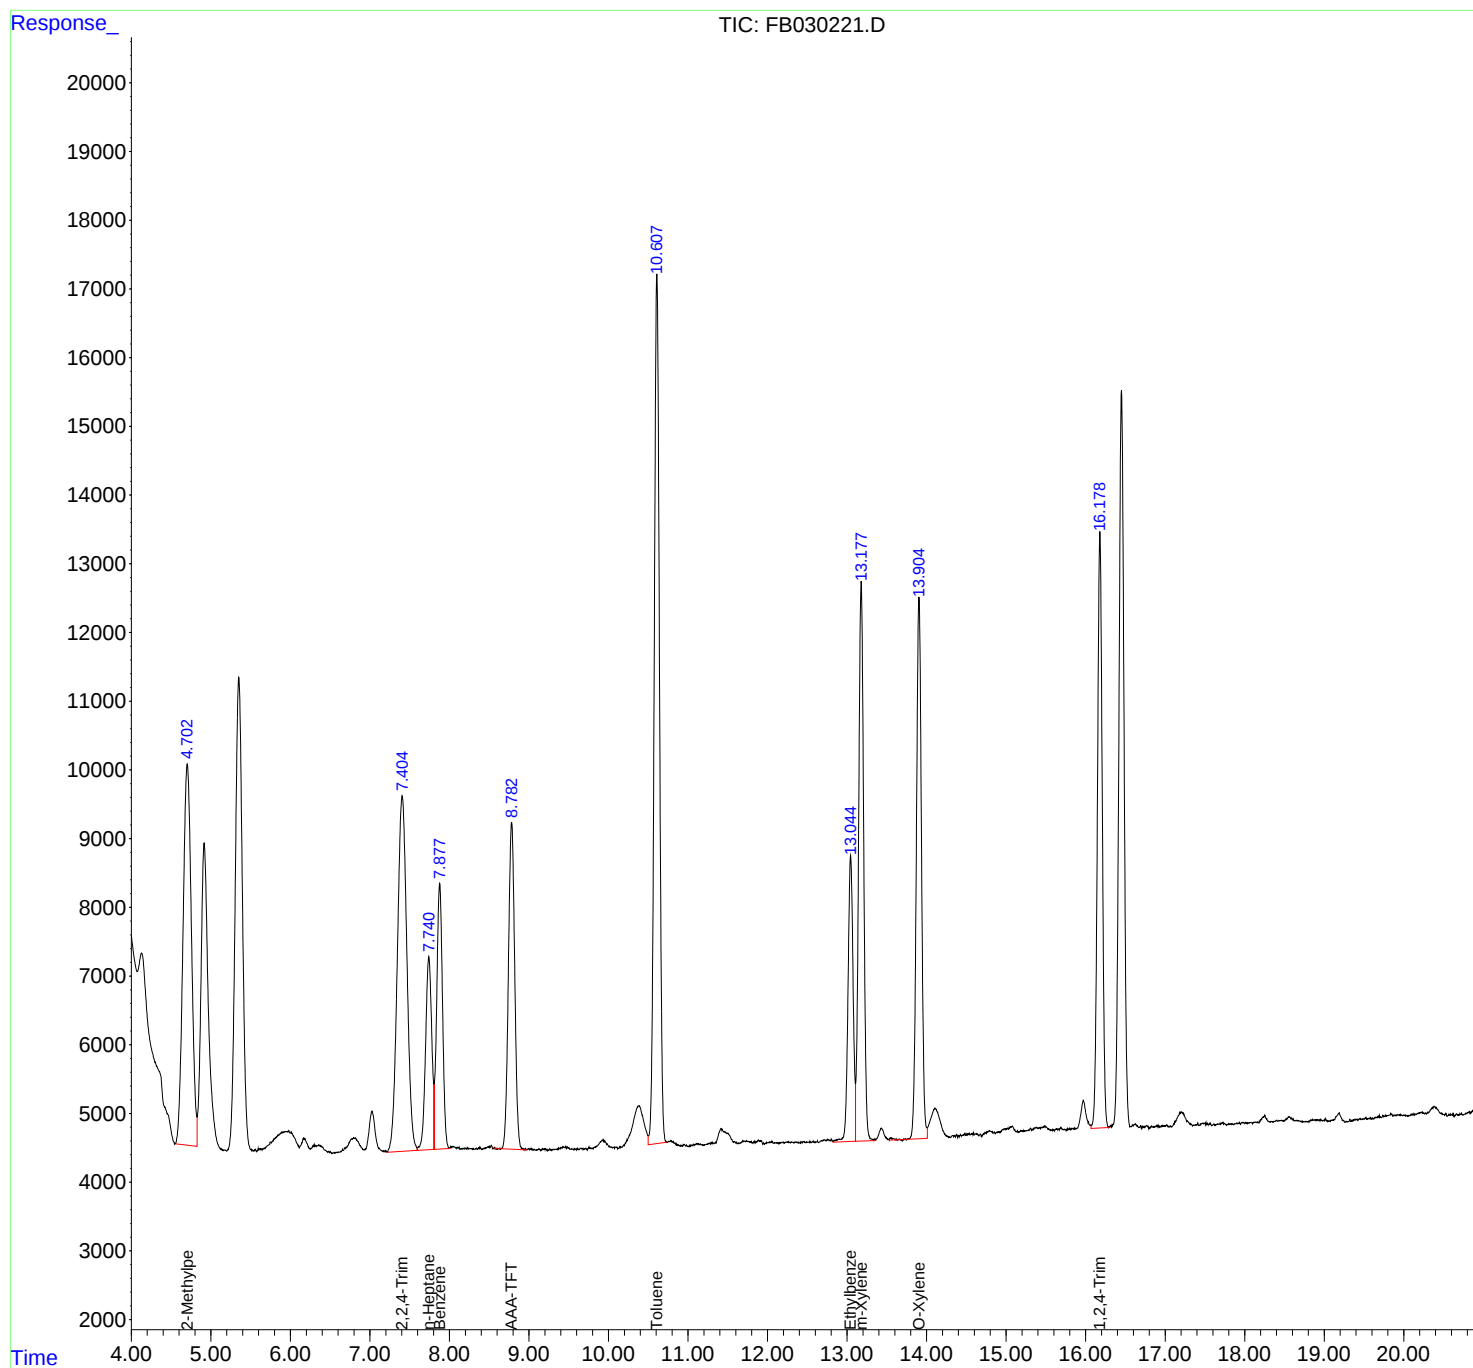

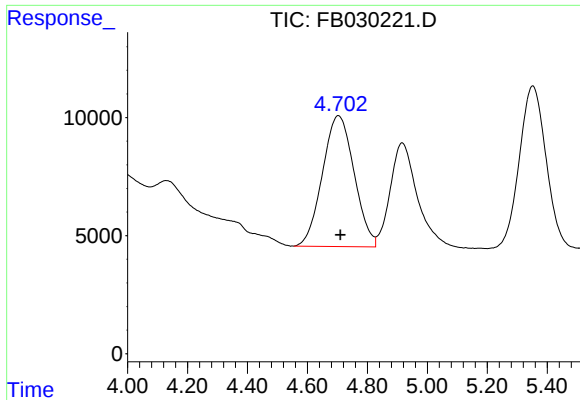


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: -0.006 min
Response: 407005
Conc: 24.64 ng/ml

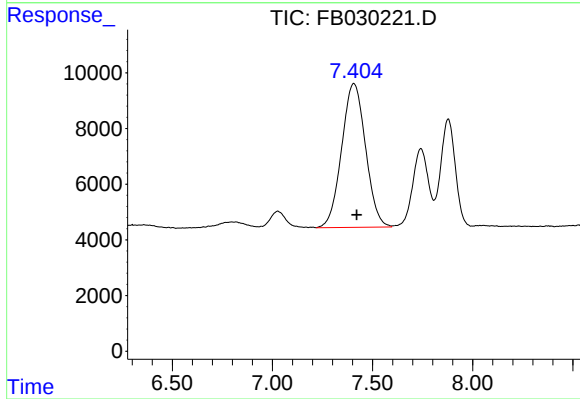


#2 2,2,4-Trimethylpentane

R.T.: 7.406 min
Delta R.T.: -0.015 min
Response: 428472
Conc: 23.09 ng/ml

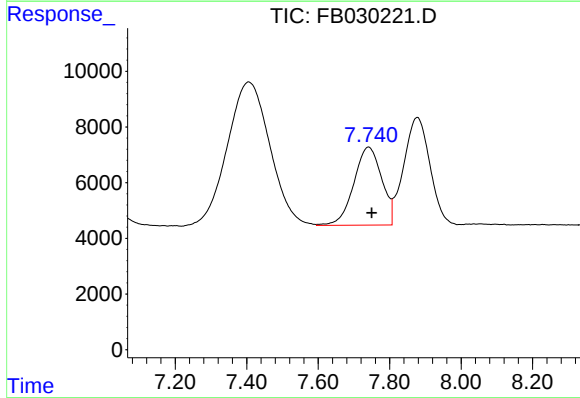


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: -0.009 min
Response: 152348
Conc: 7.92 ng/ml

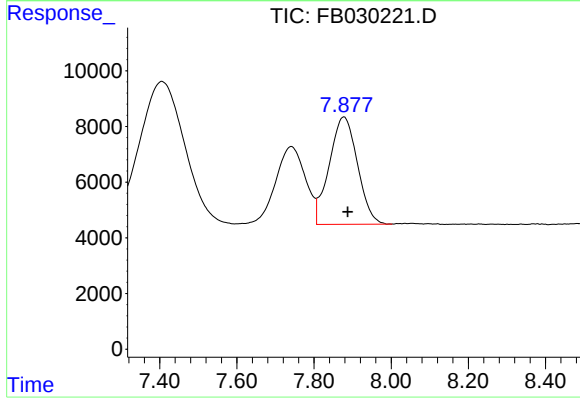


#4 Benzene

R.T.: 7.878 min
Delta R.T.: -0.009 min
Response: 196492
Conc: 8.35 ng/ml

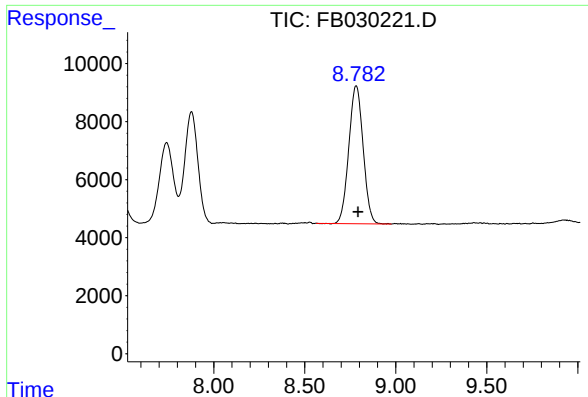


#5 AAA-TFT

R.T.: 8.783 min
Delta R.T.: -0.010 min
Response: 260058
Conc: 21.16 ng/ml

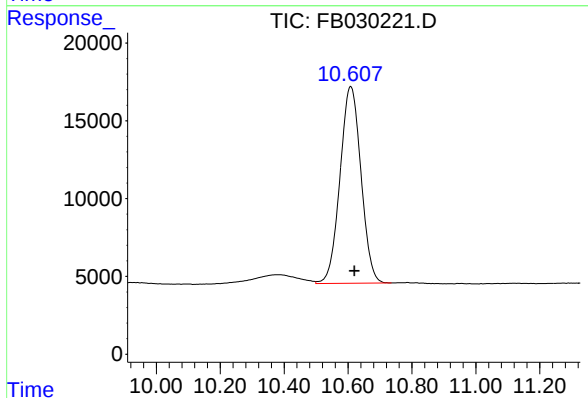


#6 Toluene

R.T.: 10.609 min
Delta R.T.: -0.011 min
Response: 576589
Conc: 25.16 ng/ml

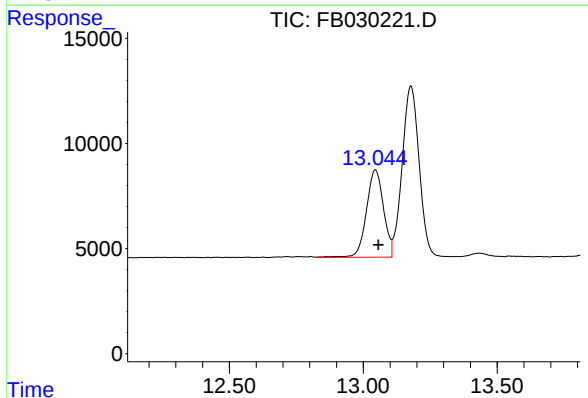


#7 Ethylbenzene

R.T.: 13.046 min
Delta R.T.: -0.011 min
Response: 183905
Conc: 8.57 ng/ml

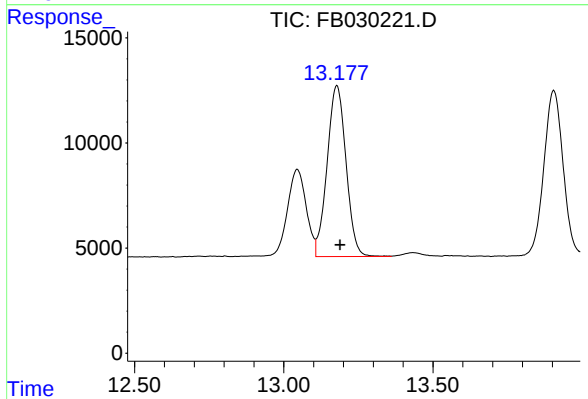


#8 m-Xylene

R.T.: 13.178 min
Delta R.T.: -0.011 min
Response: 357996
Conc: 17.02 ng/ml

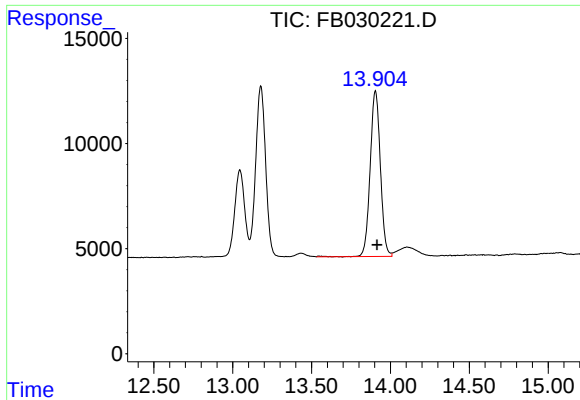

#9 O-Xylene

R.T.: 13.905 min
Delta R.T.: -0.011 min
Response: 352840
Conc: 17.19 ng/ml

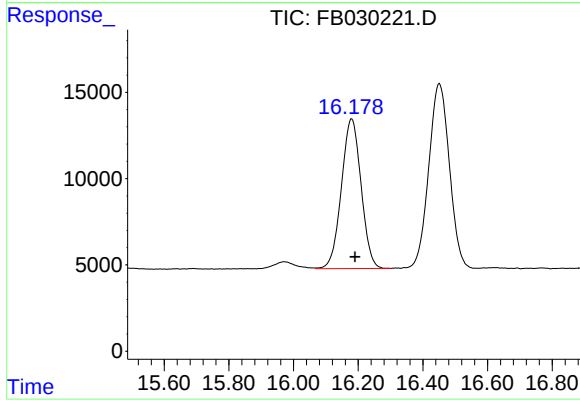

#10 1,2,4-Trimethylbenzene

R.T.: 16.180 min
Delta R.T.: -0.010 min
Response: 366545
Conc: 18.73 ng/ml