

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080218\
 Data File : FB017061.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2018 9:31
 Operator : MJ/SJ
 Sample : BSF0802S1
 Misc : 5.03g/5.00ml DI water
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 02 10:47:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.113	157689	19.820 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	397054	27.910 ng/ml
2) t 2,2,4-Trimethylpentane	7.730	402599	29.349 ng/ml
3) t n-Heptane	8.069	125162	8.963 ng/ml
4) t Benzene	8.207	164824	9.410 ng/ml
6) t Toluene	10.962	408798	30.134 ng/ml
7) t Ethylbenzene	13.412	138506	10.093 ng/ml
8) t m-Xylene	13.544	293082	20.203 ng/ml
9) t O-Xylene	14.276	304243	19.775 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	362474	19.434 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080218\
Data File : FB017061.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2018 9:31
Operator : MJ/SJ
Sample : BSF0802S1
Misc : 5.03g/5.00ml DI water
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 02 10:47:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

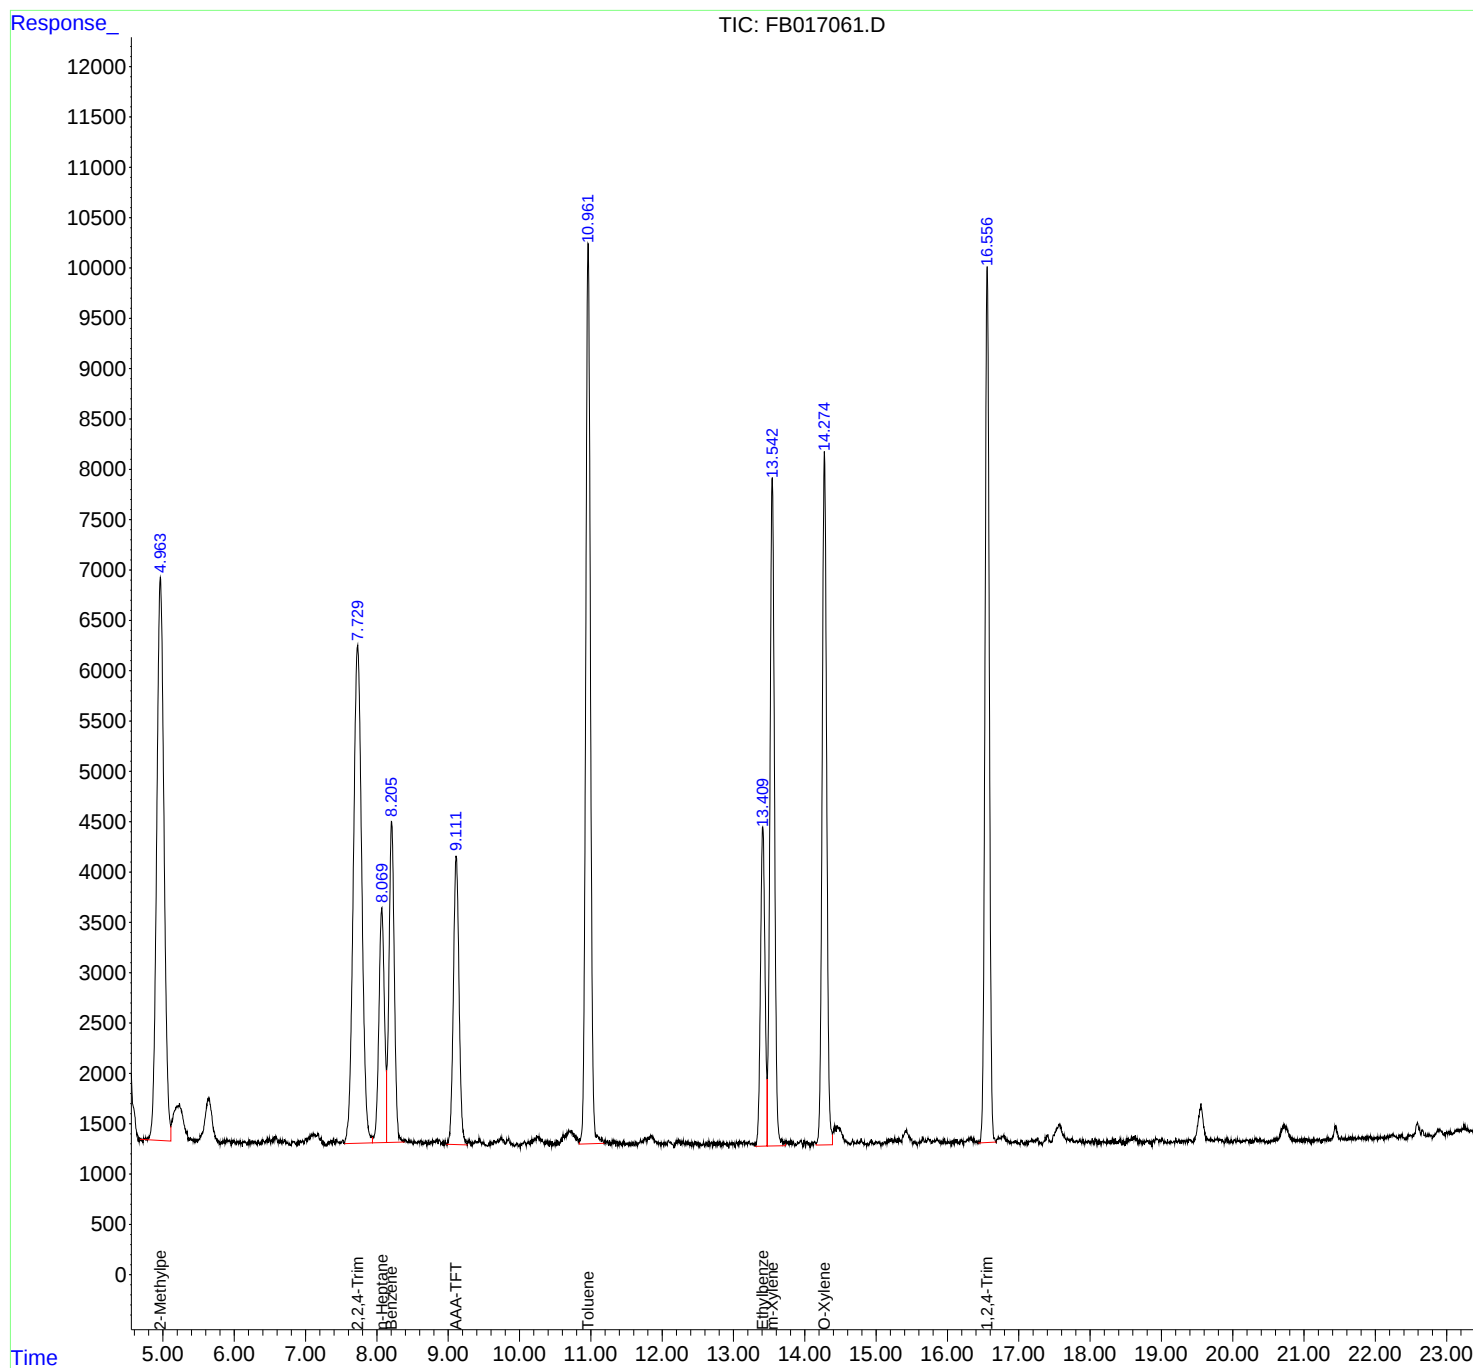


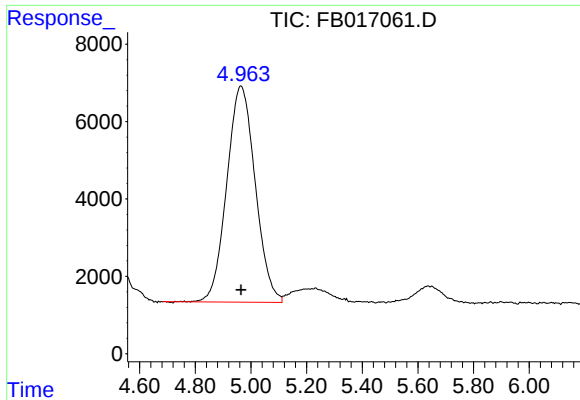

#1 2-Methylpentane


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 397054
Conc: 27.91 ng/ml

Instrument :
FID_B
ClientSampleId :

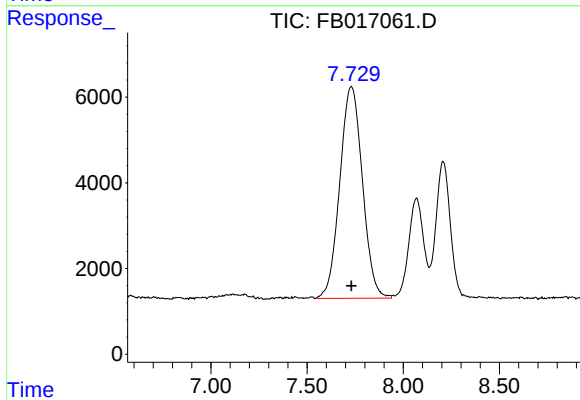


#2 2,2,4-Trimethylpentane

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 402599
Conc: 29.35 ng/ml

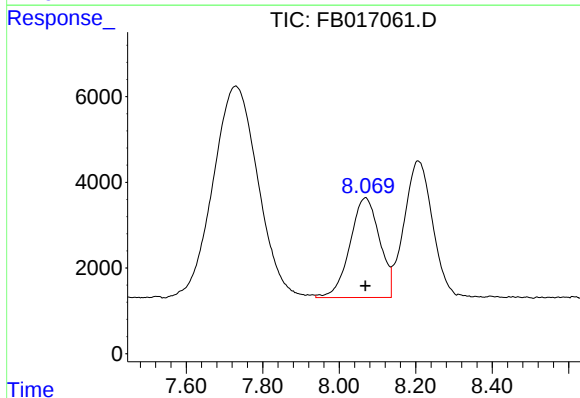


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 125162
Conc: 8.96 ng/ml

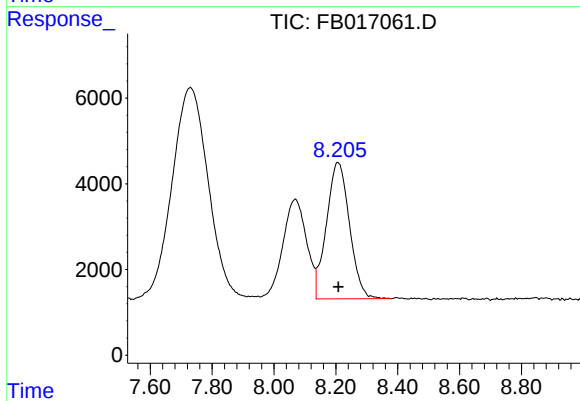

#4 Benzene


R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 164824
Conc: 9.41 ng/ml

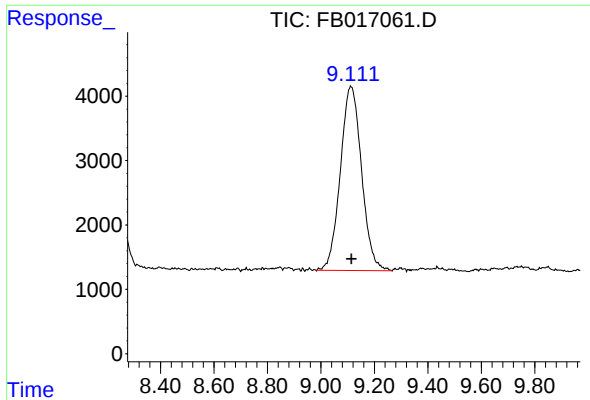

#5 AAA-TFT


R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 157689
Conc: 19.82 ng/ml

Instrument :
FID_B
ClientSampleId :

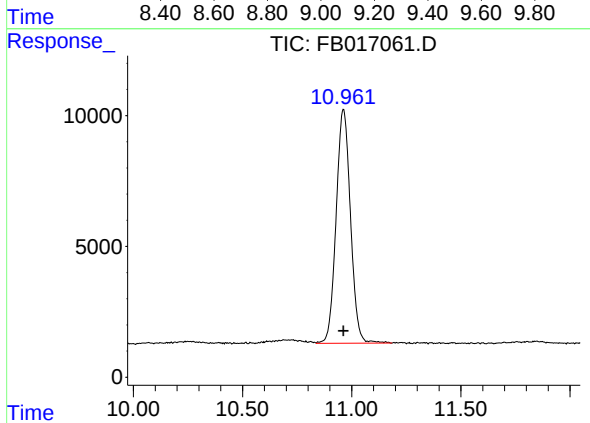


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.000 min
Response: 408798
Conc: 30.13 ng/ml

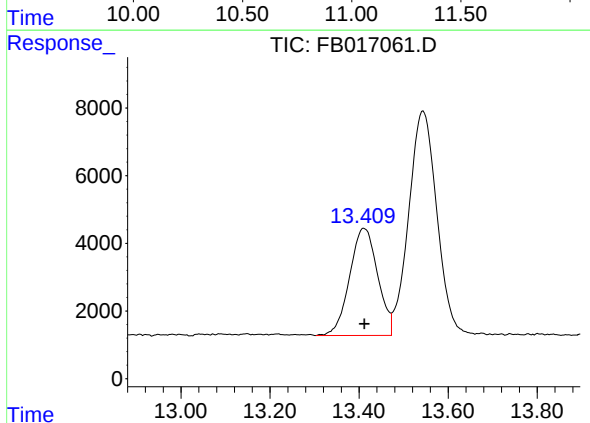


#7 Ethylbenzene

R.T.: 13.412 min
Delta R.T.: 0.000 min
Response: 138506
Conc: 10.09 ng/ml

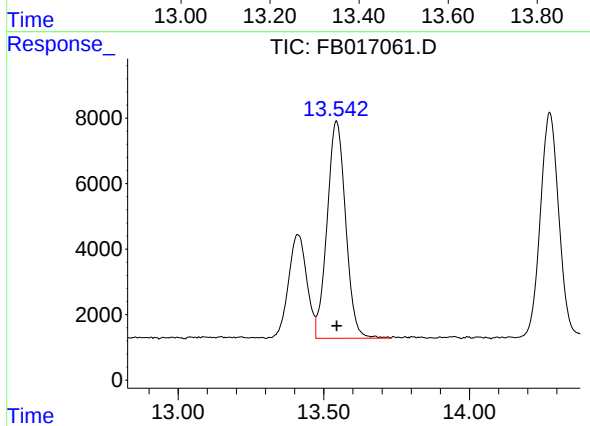

#8 m-Xylene


R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 293082
Conc: 20.20 ng/ml

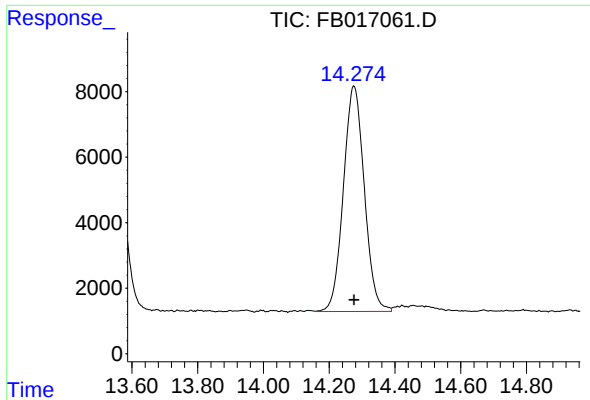

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.000 min
Response: 304243
Conc: 19.77 ng/ml

Instrument :
FID_B
ClientSampleId :

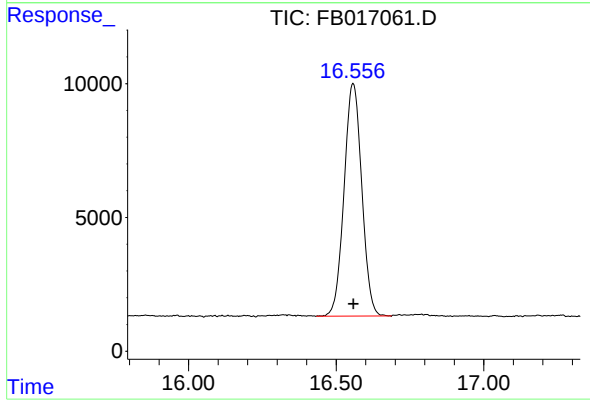

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 362474
Conc: 19.43 ng/ml