

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080119\
 Data File : FB021894.D
 Signal(s) : FID2B.CH
 Acq On : 1 Aug 2019 14:38
 Operator : DD/AJ
 Sample : K4066-06MSD
 Misc : 5.07/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 02 00:39:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	256944	18.828 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.863	598874	21.717 ng/ml
2) t	2,2,4-Trimethylpentane	7.612	583067	22.057 ng/ml
3) t	n-Heptane	7.950	172972	6.976 ng/ml
4) t	Benzene	8.085	256599	8.783 ng/ml
6) t	Toluene	10.831	532051	25.857 ng/ml
7) t	Ethylbenzene	13.276	187056	8.991 ng/ml
8) t	m-Xylene	13.409	396320	17.840 ng/ml
9) t	O-Xylene	14.138	414435	18.017 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	423910	17.980 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080119\
Data File : FB021894.D
Signal(s) : FID2B.CH
Acq On : 1 Aug 2019 14:38
Operator : DD/AJ
Sample : K4066-06MSD
Misc : 5.07/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 02 00:39:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

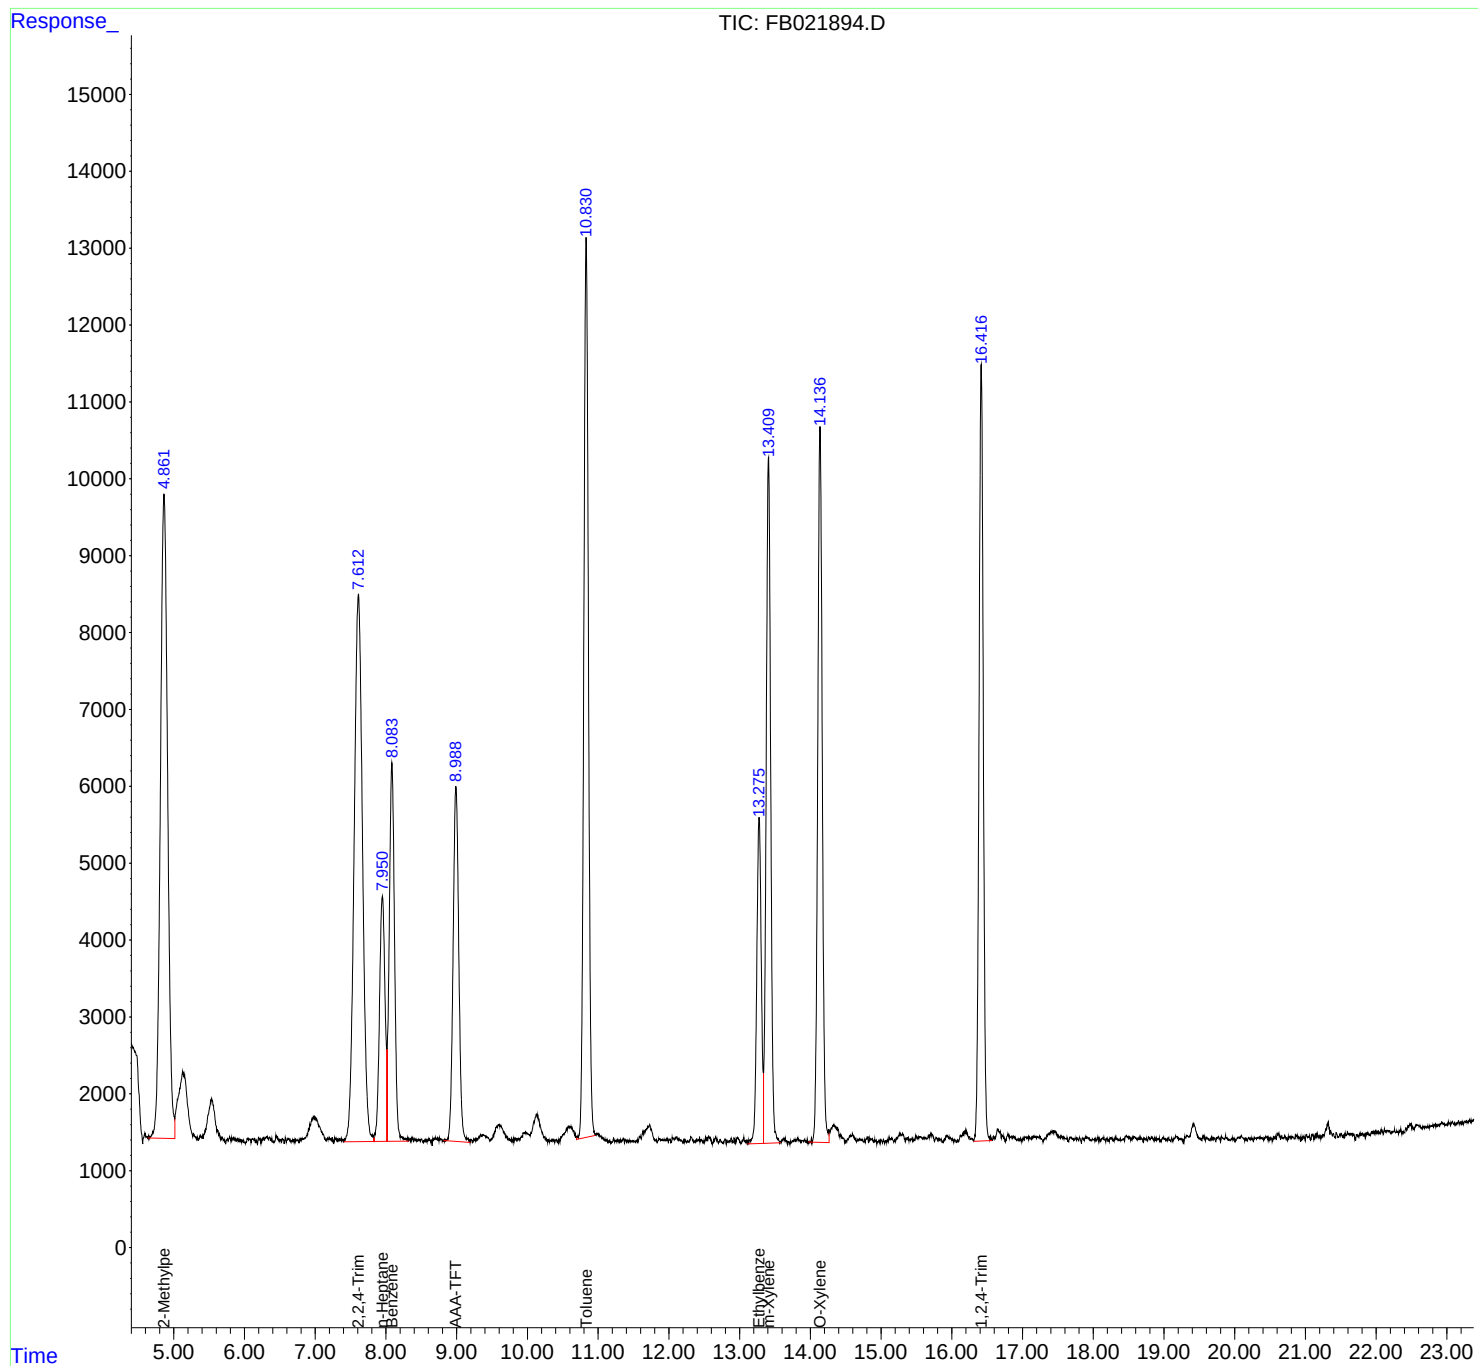

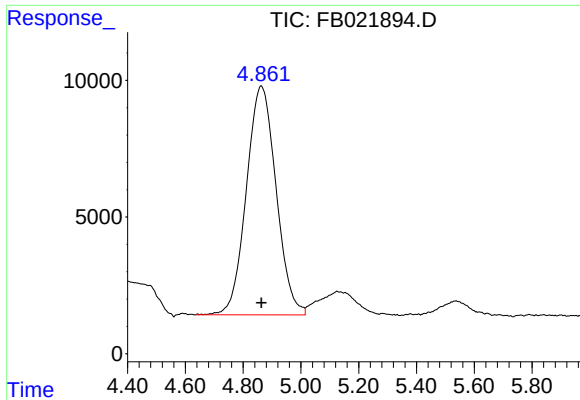


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 598874
Conc: 21.72 ng/ml

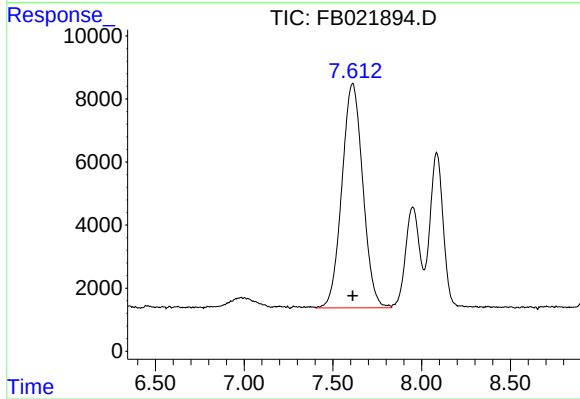


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 583067
Conc: 22.06 ng/ml

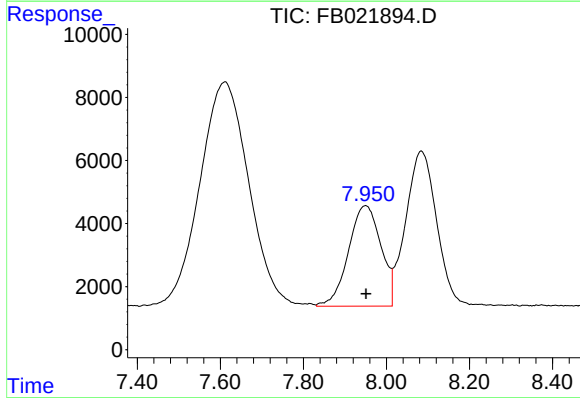


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 172972
Conc: 6.98 ng/ml

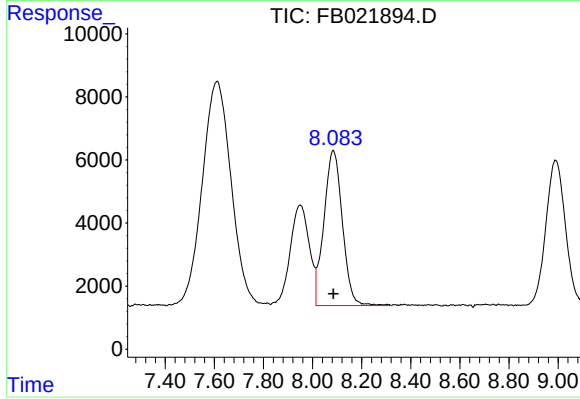


#4 Benzene

R.T.: 8.085 min
Delta R.T.: -0.001 min
Response: 256599
Conc: 8.78 ng/ml

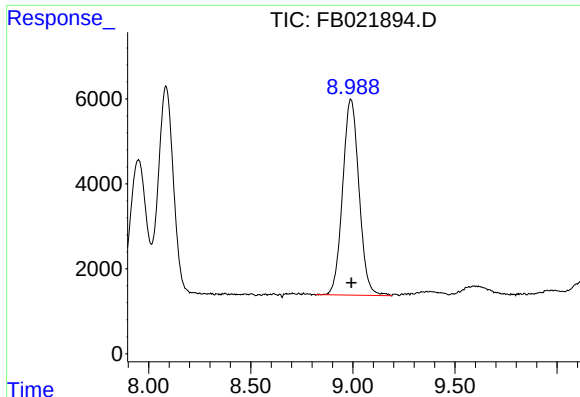


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 256944
Conc: 18.83 ng/ml

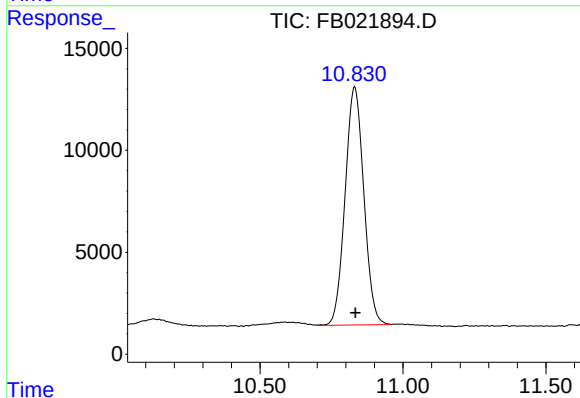


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 532051
Conc: 25.86 ng/ml

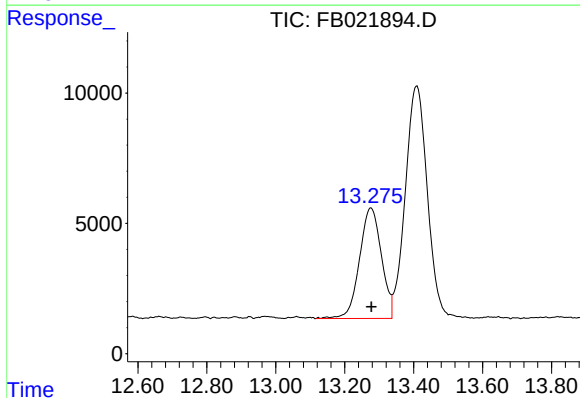


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.001 min
Response: 187056
Conc: 8.99 ng/ml

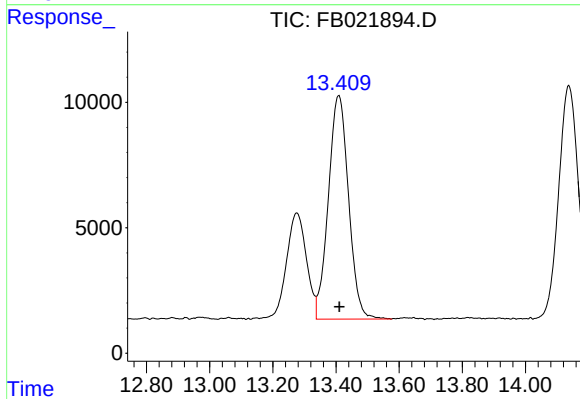


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 396320
Conc: 17.84 ng/ml

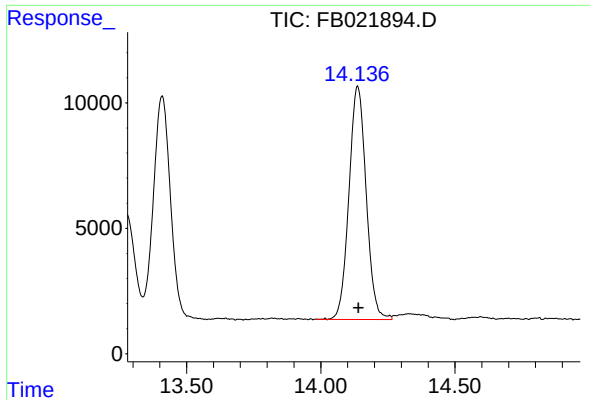

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.003 min
Response: 414435
Conc: 18.02 ng/ml

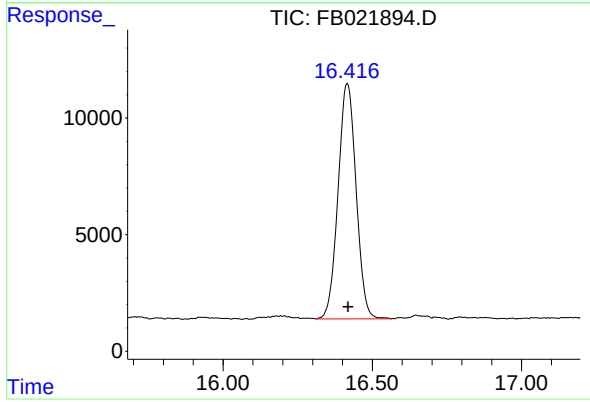

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.003 min
Response: 423910
Conc: 17.98 ng/ml