

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080119\
 Data File : FB021893.D
 Signal(s) : FID2B.CH
 Acq On : 1 Aug 2019 14:07
 Operator : DD/AJ
 Sample : K4066-06MS
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 02 00:39:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	259051	18.983 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	636866	23.095 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	627472	23.737 ng/ml
3) t n-Heptane	7.950	188651	7.609 ng/ml
4) t Benzene	8.086	256567	8.782 ng/ml
6) t Toluene	10.833	564299	27.425 ng/ml
7) t Ethylbenzene	13.278	189002	9.085 ng/ml
8) t m-Xylene	13.411	404793	18.221 ng/ml
9) t O-Xylene	14.140	429852	18.687 ng/ml
10) t 1,2,4-Trimethylbenzene	16.419	438584	18.602 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080119\
Data File : FB021893.D
Signal(s) : FID2B.CH
Acq On : 1 Aug 2019 14:07
Operator : DD/AJ
Sample : K4066-06MS
Misc : 5.05/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 02 00:39:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

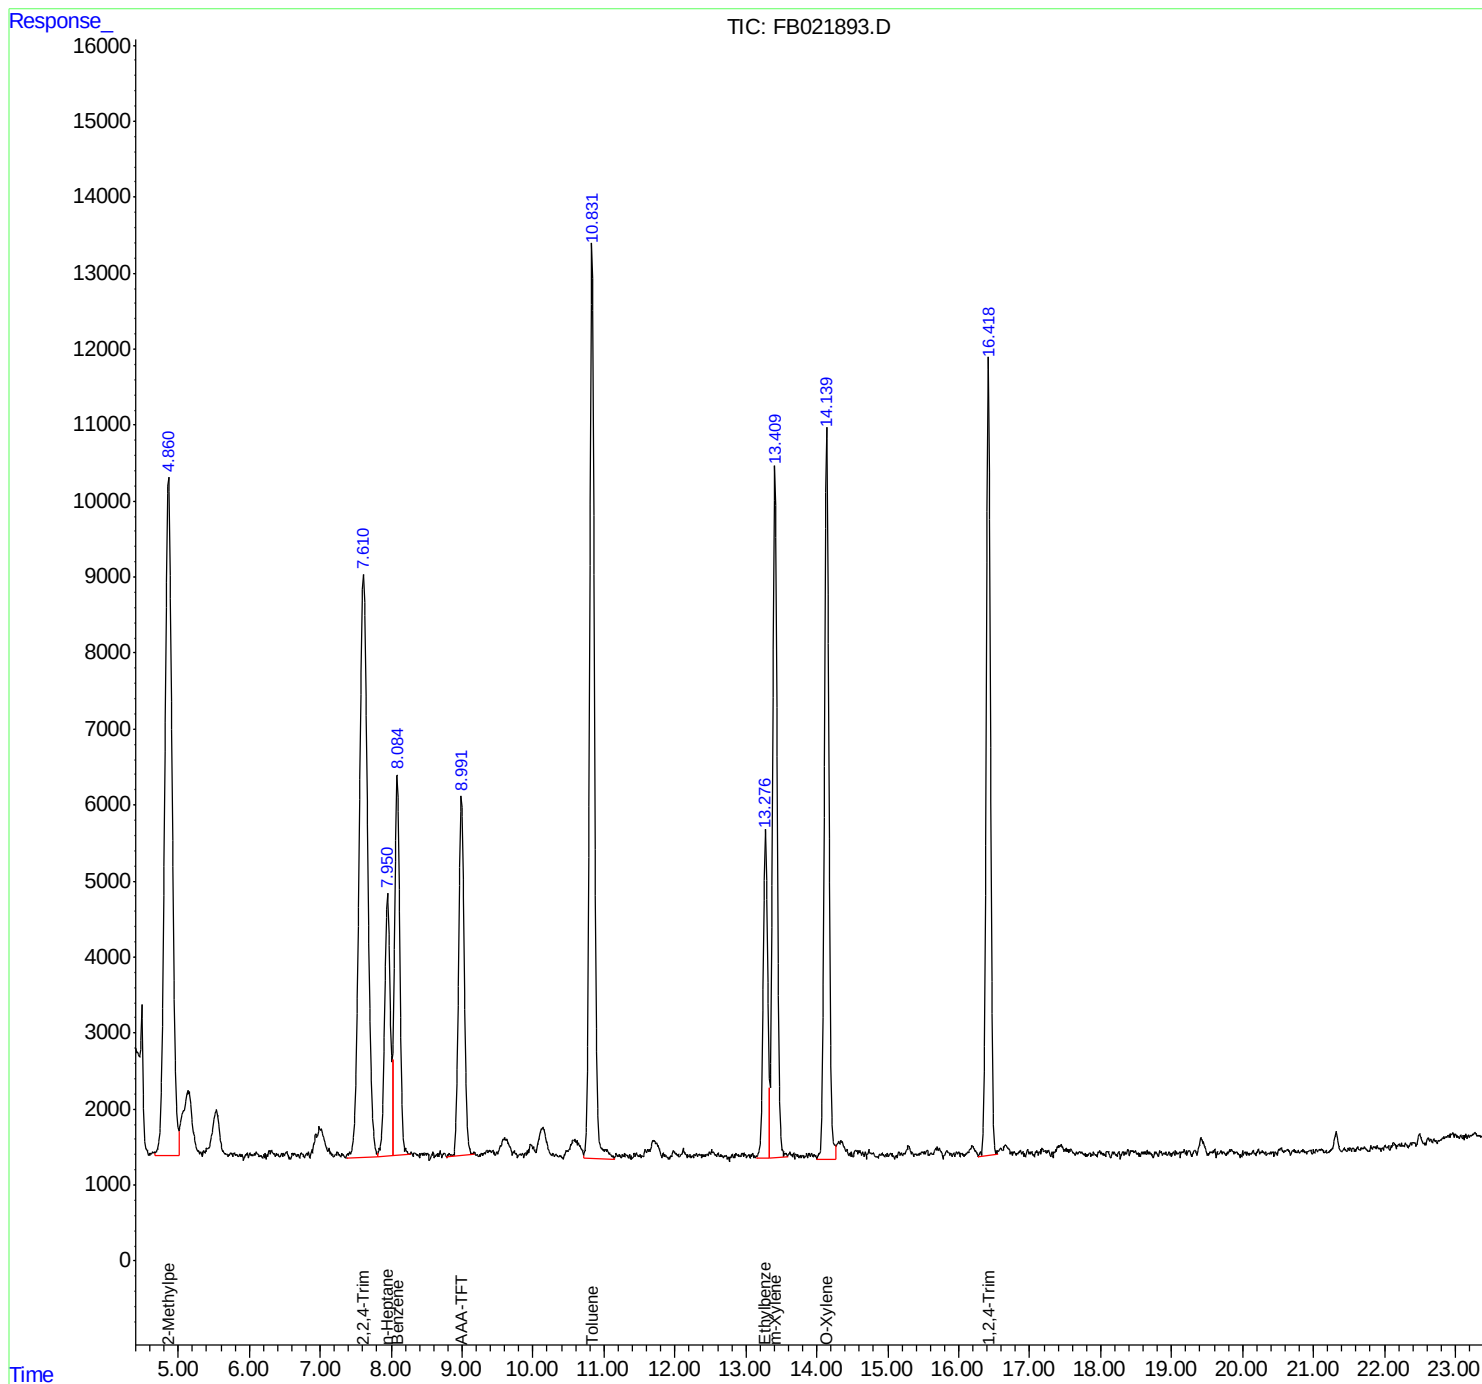

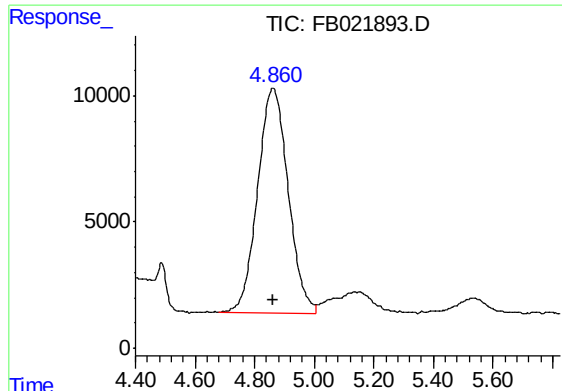


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 636866
Conc: 23.09 ng/ml

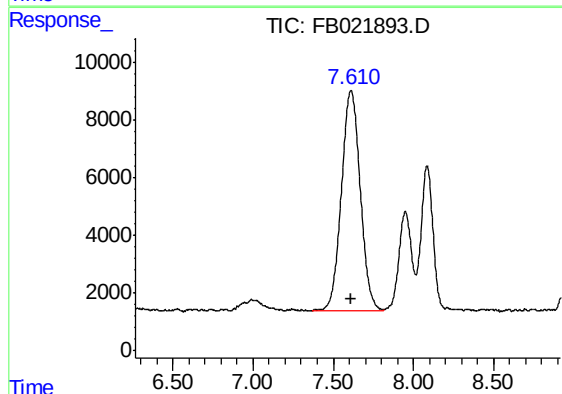


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 627472
Conc: 23.74 ng/ml

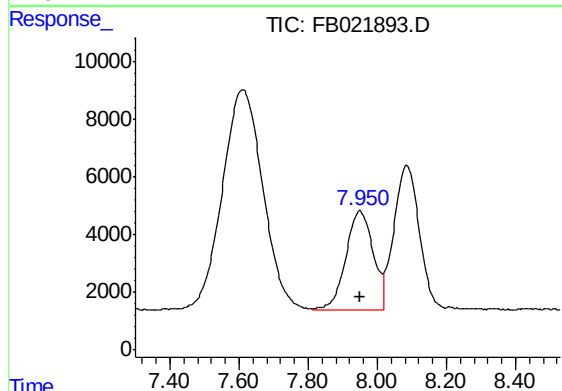


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 188651
Conc: 7.61 ng/ml

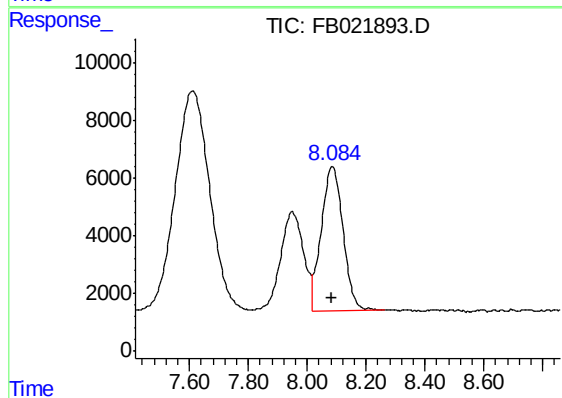


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 256567
Conc: 8.78 ng/ml

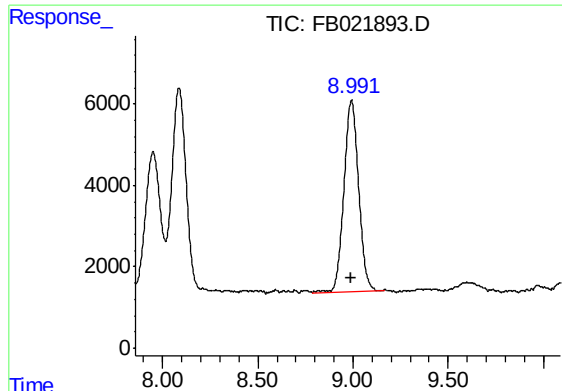


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 259051
Conc: 18.98 ng/ml

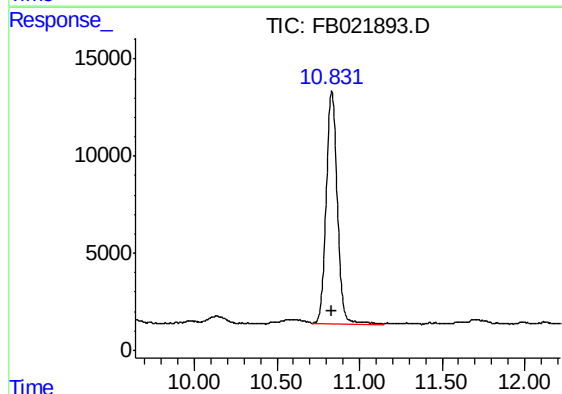


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 564299
Conc: 27.42 ng/ml

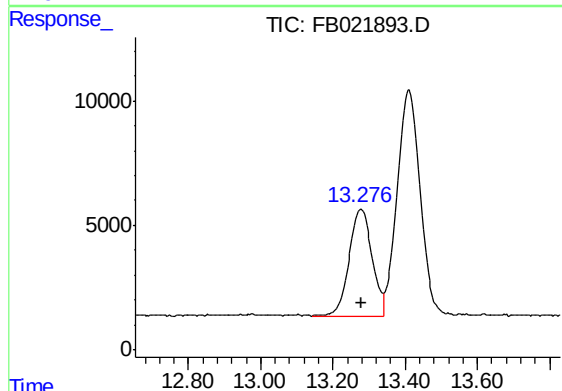


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 189002
Conc: 9.08 ng/ml

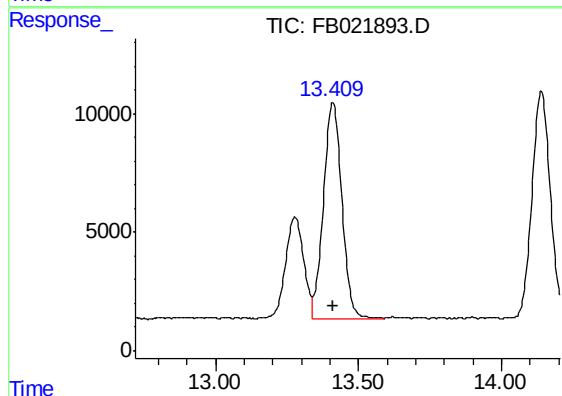


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 404793
Conc: 18.22 ng/ml

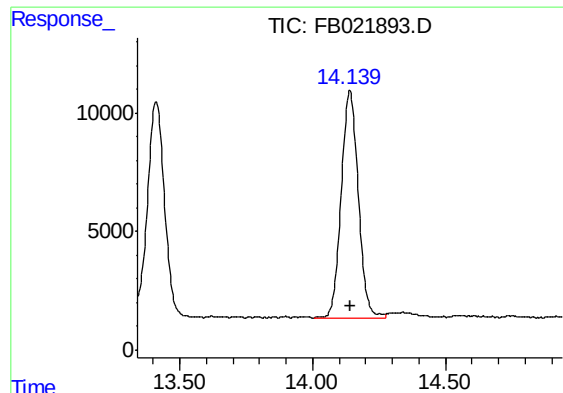

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 429852
Conc: 18.69 ng/ml

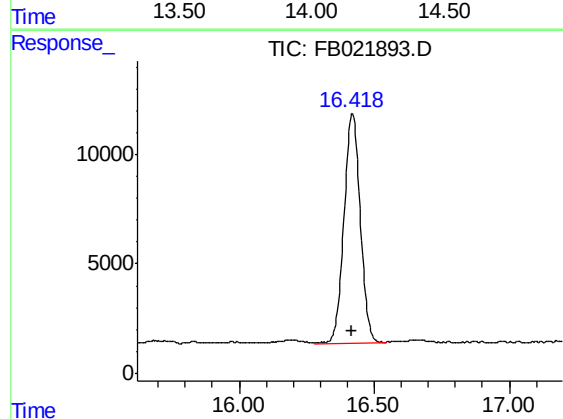

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.000 min
Response: 438584
Conc: 18.60 ng/ml