

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080219\
 Data File : FB021899.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2019 9:38
 Operator : DD/AJ
 Sample : BSF0802S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 02 22:53:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	313951	23.006 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	818585	29.685 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	864869	32.718 ng/ml
3) t n-Heptane	7.948	261290	10.538 ng/ml
4) t Benzene	8.085	314641	10.770 ng/ml
6) t Toluene	10.832	666549	32.394 ng/ml
7) t Ethylbenzene	13.276	222234	10.682 ng/ml
8) t m-Xylene	13.410	474963	21.380 ng/ml
9) t O-Xylene	14.138	503684	21.897 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	522523	22.163 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080219\
Data File : FB021899.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2019 9:38
Operator : DD/AJ
Sample : BSF0802S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 02 22:53:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

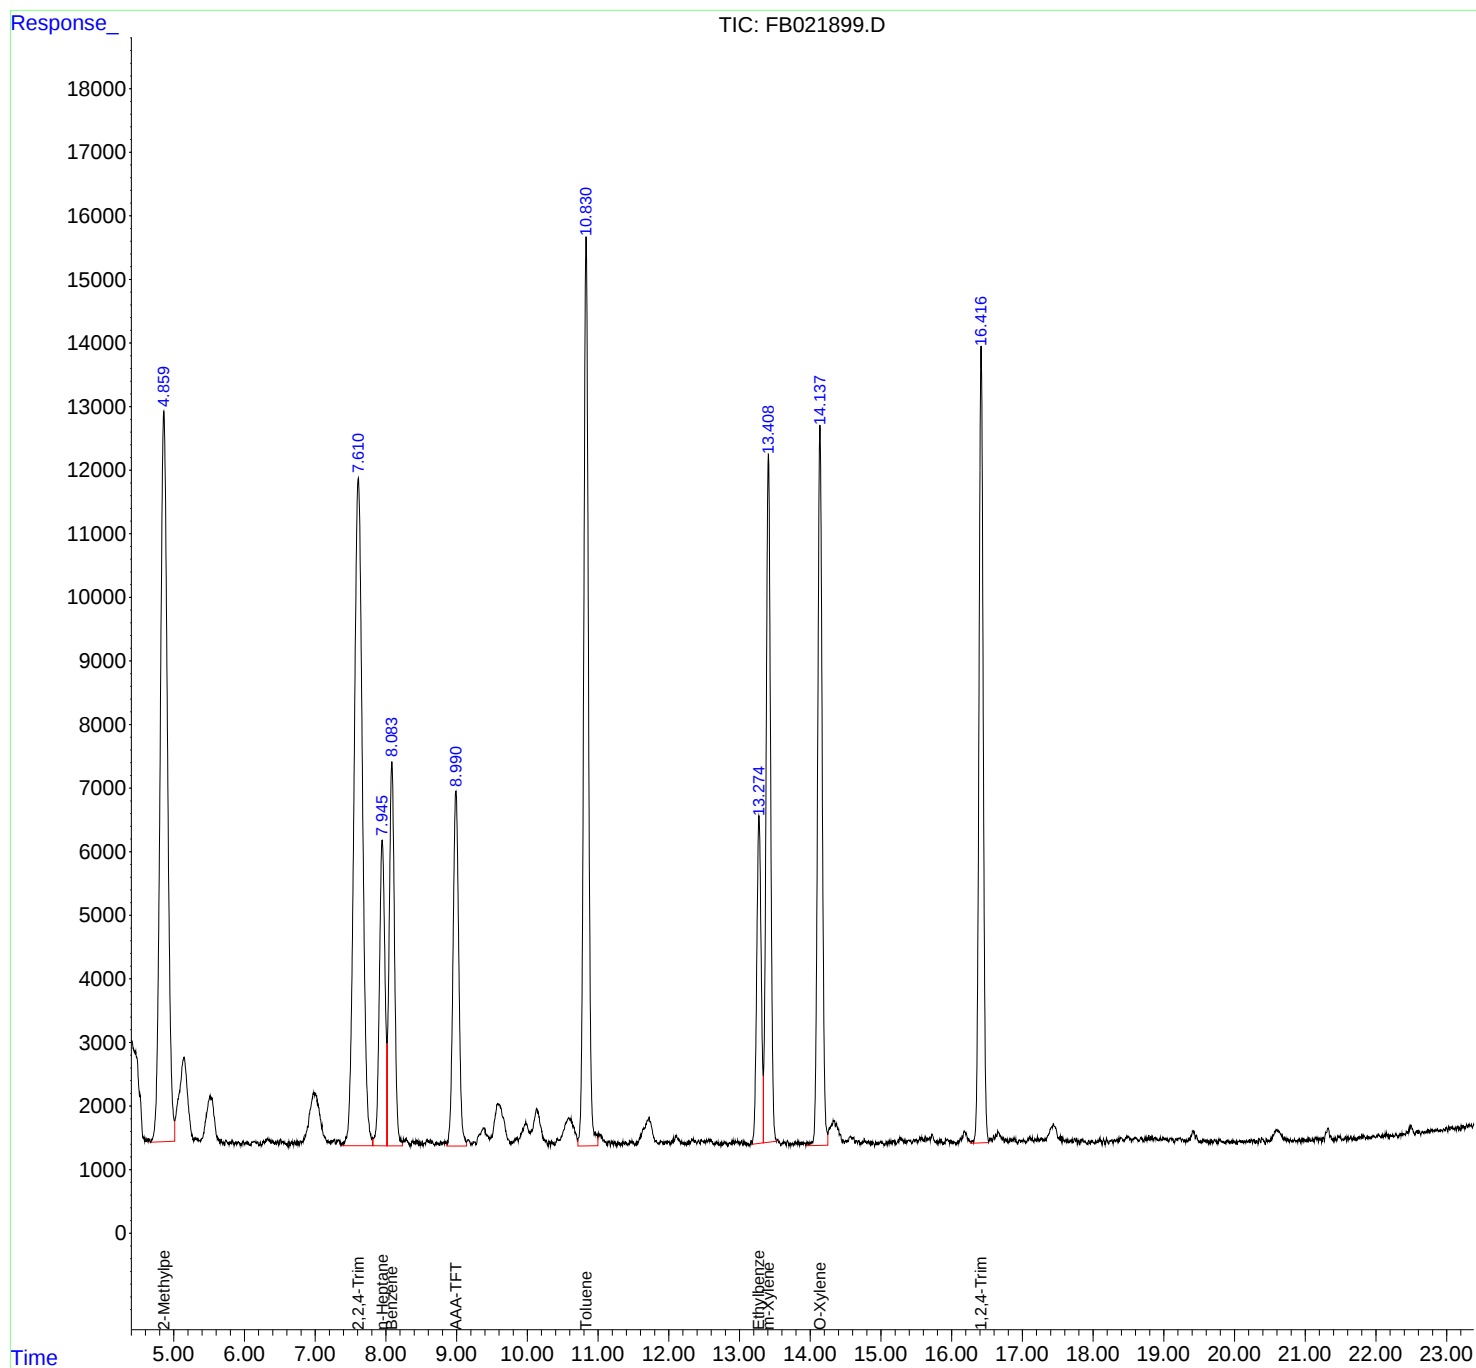

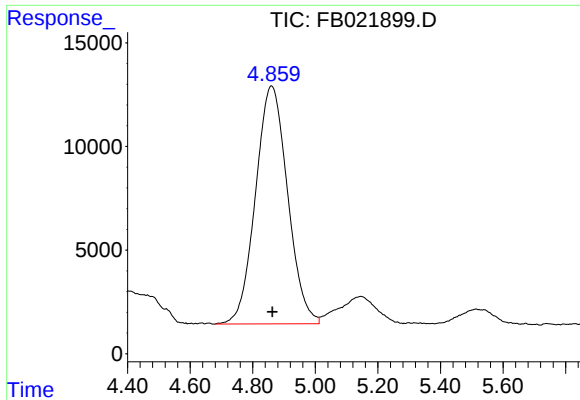


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.003 min
Response: 818585
Conc: 29.68 ng/ml

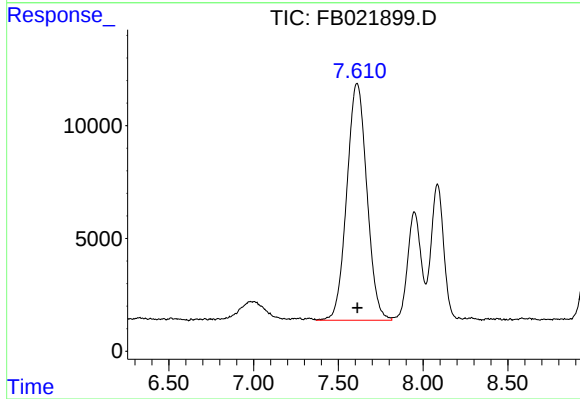


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.002 min
Response: 864869
Conc: 32.72 ng/ml

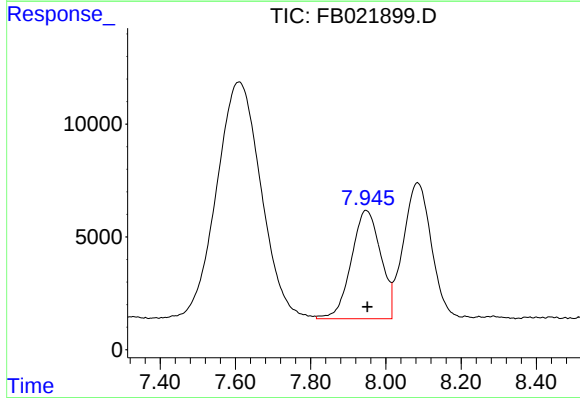


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 261290
Conc: 10.54 ng/ml

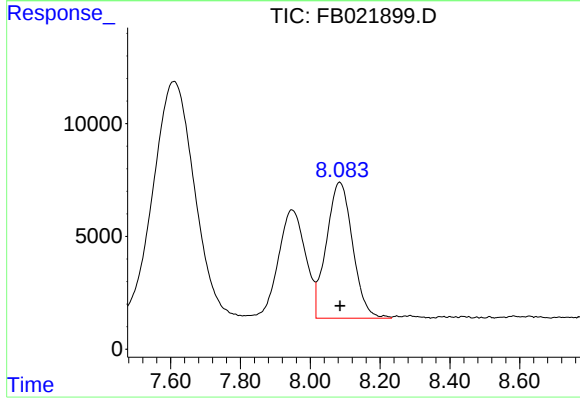


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 314641
Conc: 10.77 ng/ml

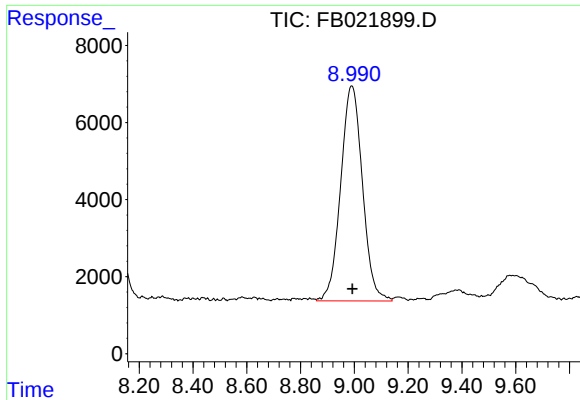


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 313951
Conc: 23.01 ng/ml

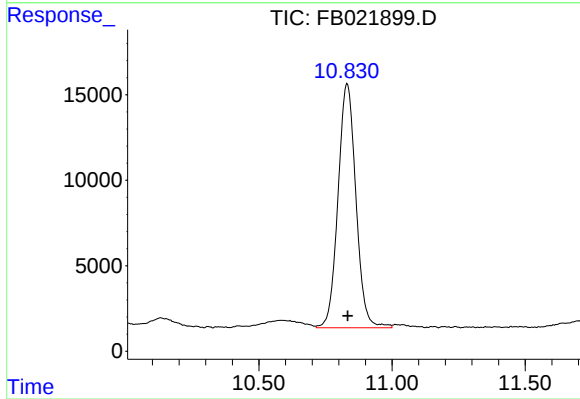


#6 Toluene

R.T.: 10.832 min
Delta R.T.: -0.002 min
Response: 666549
Conc: 32.39 ng/ml

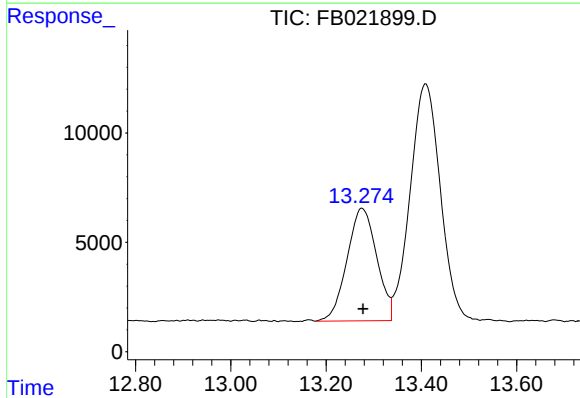


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.001 min
Response: 222234
Conc: 10.68 ng/ml

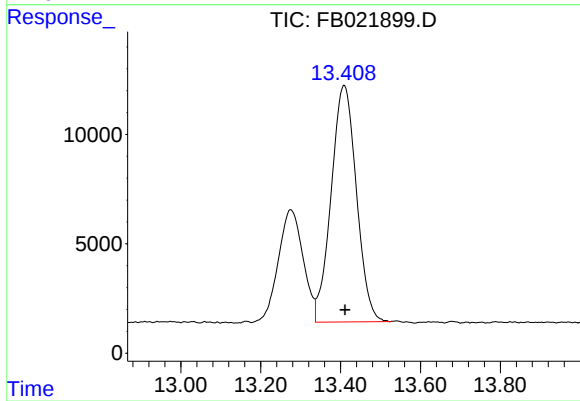


#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: -0.001 min
Response: 474963
Conc: 21.38 ng/ml

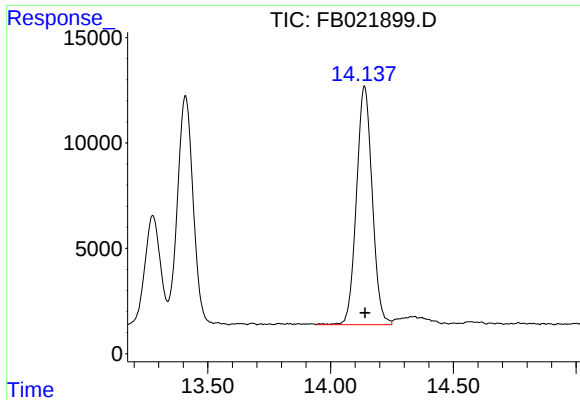

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 503684
Conc: 21.90 ng/ml

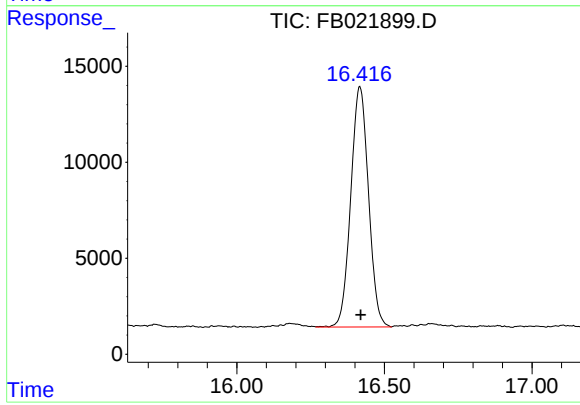

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 522523
Conc: 22.16 ng/ml