

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080219\
 Data File : FB021901.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2019 11:43
 Operator : DD/AJ
 Sample : K4124-03MS
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 02 22:53:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	274823	20.139 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	680962	24.694 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	683982	25.875 ng/ml
3) t n-Heptane	7.948	205021	8.269 ng/ml
4) t Benzene	8.083	273585	9.365 ng/ml
6) t Toluene	10.830	582565	28.312 ng/ml
7) t Ethylbenzene	13.277	198304	9.532 ng/ml
8) t m-Xylene	13.409	425420	19.150 ng/ml
9) t O-Xylene	14.138	438606	19.068 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	455831	19.334 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080219\
Data File : FB021901.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2019 11:43
Operator : DD/AJ
Sample : K4124-03MS
Misc : 5.01/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 02 22:53:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

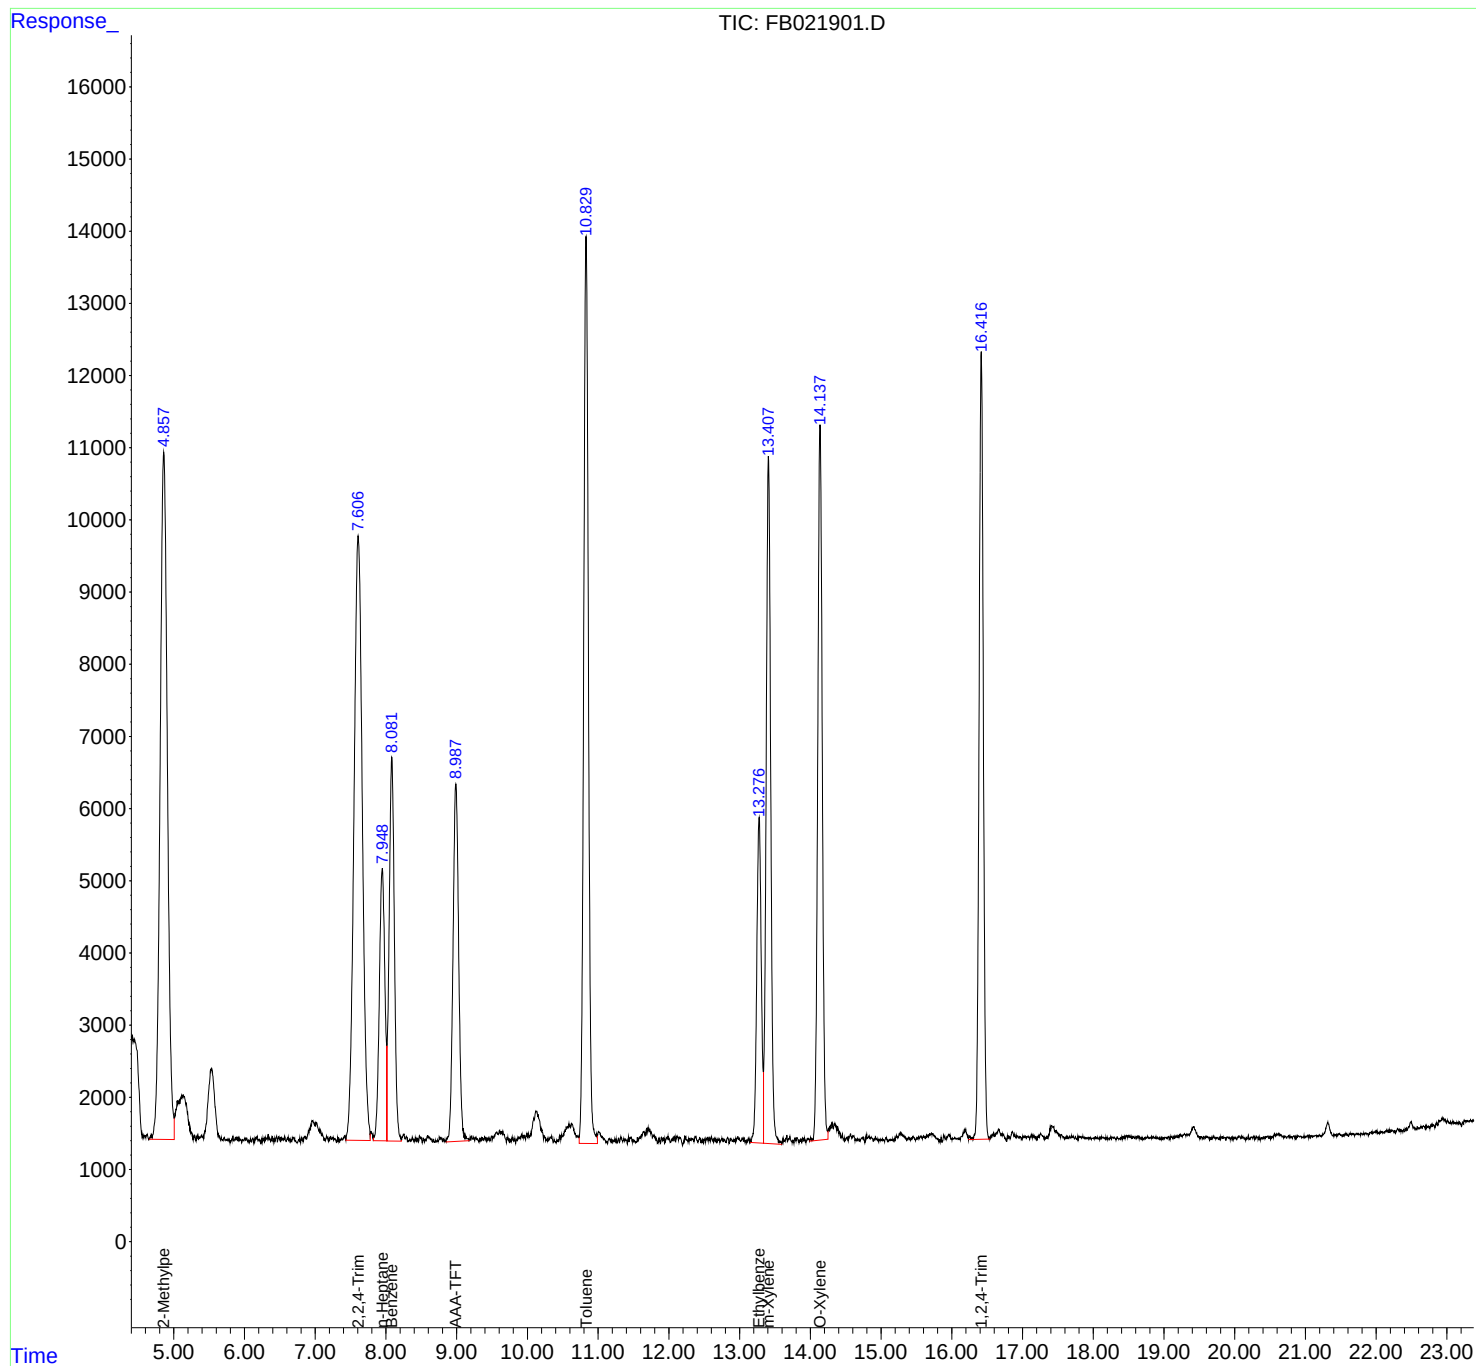

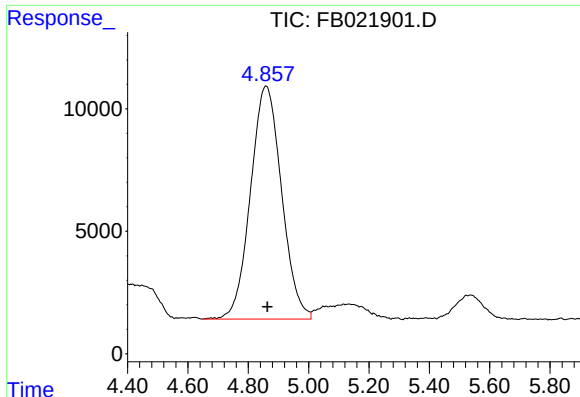


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.003 min
Response: 680962
Conc: 24.69 ng/ml

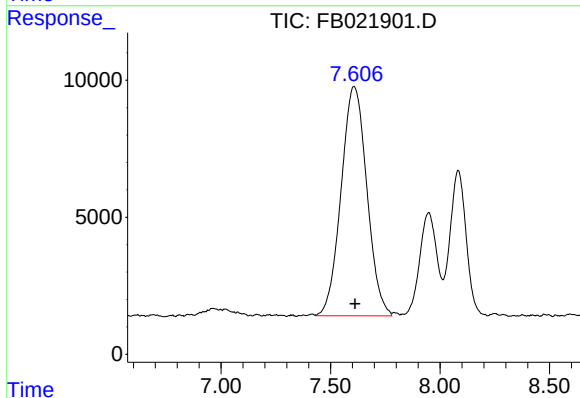


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: -0.005 min
Response: 683982
Conc: 25.87 ng/ml

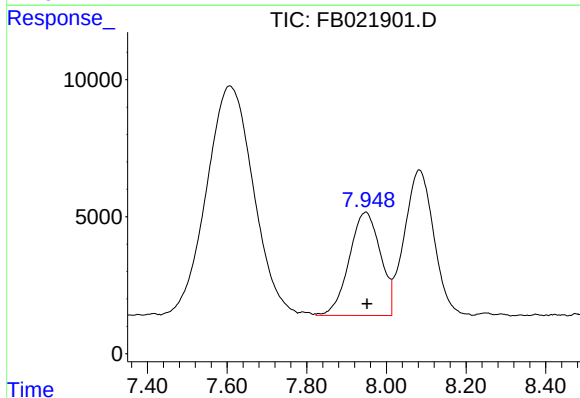


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 205021
Conc: 8.27 ng/ml

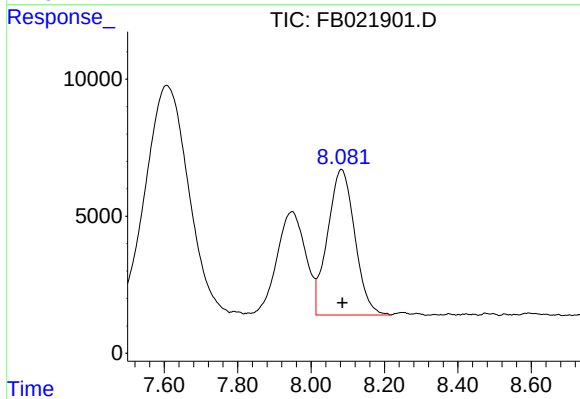


#4 Benzene

R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 273585
Conc: 9.36 ng/ml

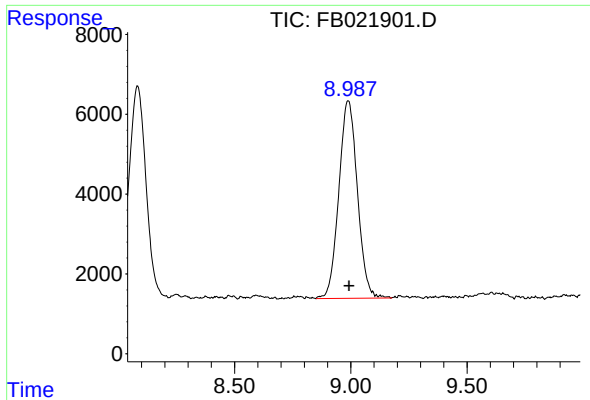


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 274823
Conc: 20.14 ng/ml

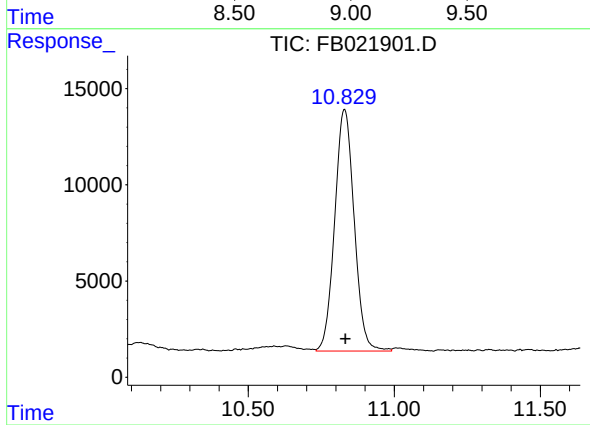


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 582565
Conc: 28.31 ng/ml

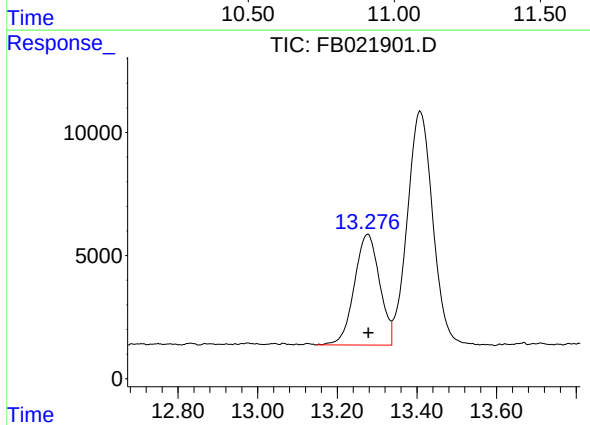


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.000 min
Response: 198304
Conc: 9.53 ng/ml

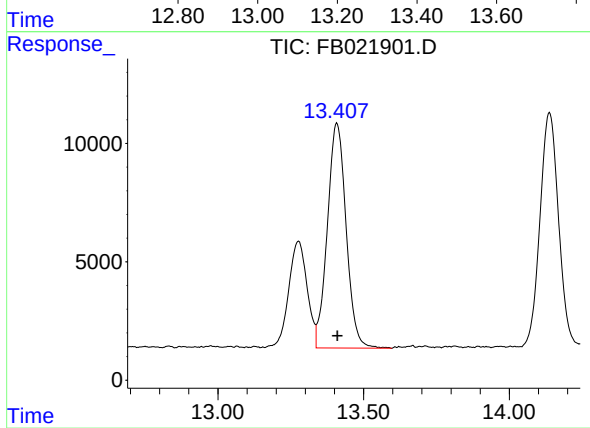

#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 425420
Conc: 19.15 ng/ml

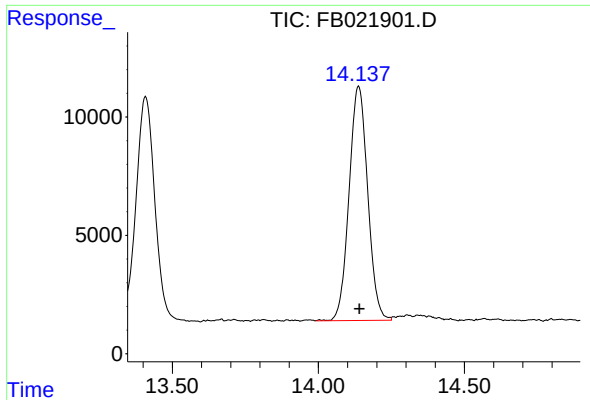


#9 O-Xylene

R.T.: 14.138 min

Delta R.T.: -0.002 min

Response: 438606

Conc: 19.07 ng/ml

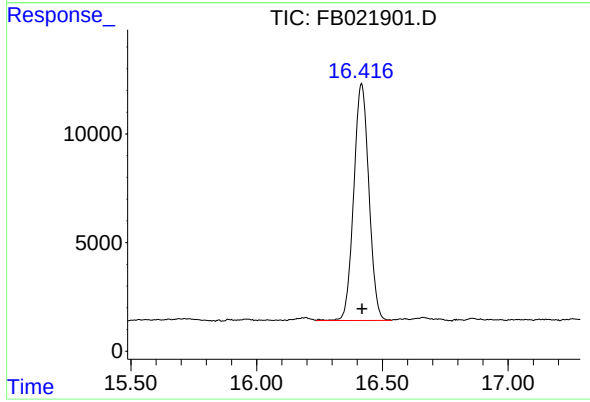

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min

Delta R.T.: -0.002 min

Response: 455831

Conc: 19.33 ng/ml