

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080219\
 Data File : FB021902.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2019 12:13
 Operator : DD/AJ
 Sample : K4124-03MSD
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 02 22:54:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	271190	19.872 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	616541	22.358 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	601546	22.756 ng/ml
3) t n-Heptane	7.949	175884	7.094 ng/ml
4) t Benzene	8.085	260476	8.916 ng/ml
6) t Toluene	10.830	552288	26.841 ng/ml
7) t Ethylbenzene	13.276	183491	8.820 ng/ml
8) t m-Xylene	13.409	389522	17.534 ng/ml
9) t O-Xylene	14.138	410893	17.863 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	425062	18.029 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080219\
Data File : FB021902.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2019 12:13
Operator : DD/AJ
Sample : K4124-03MSD
Misc : 5.02/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 02 22:54:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

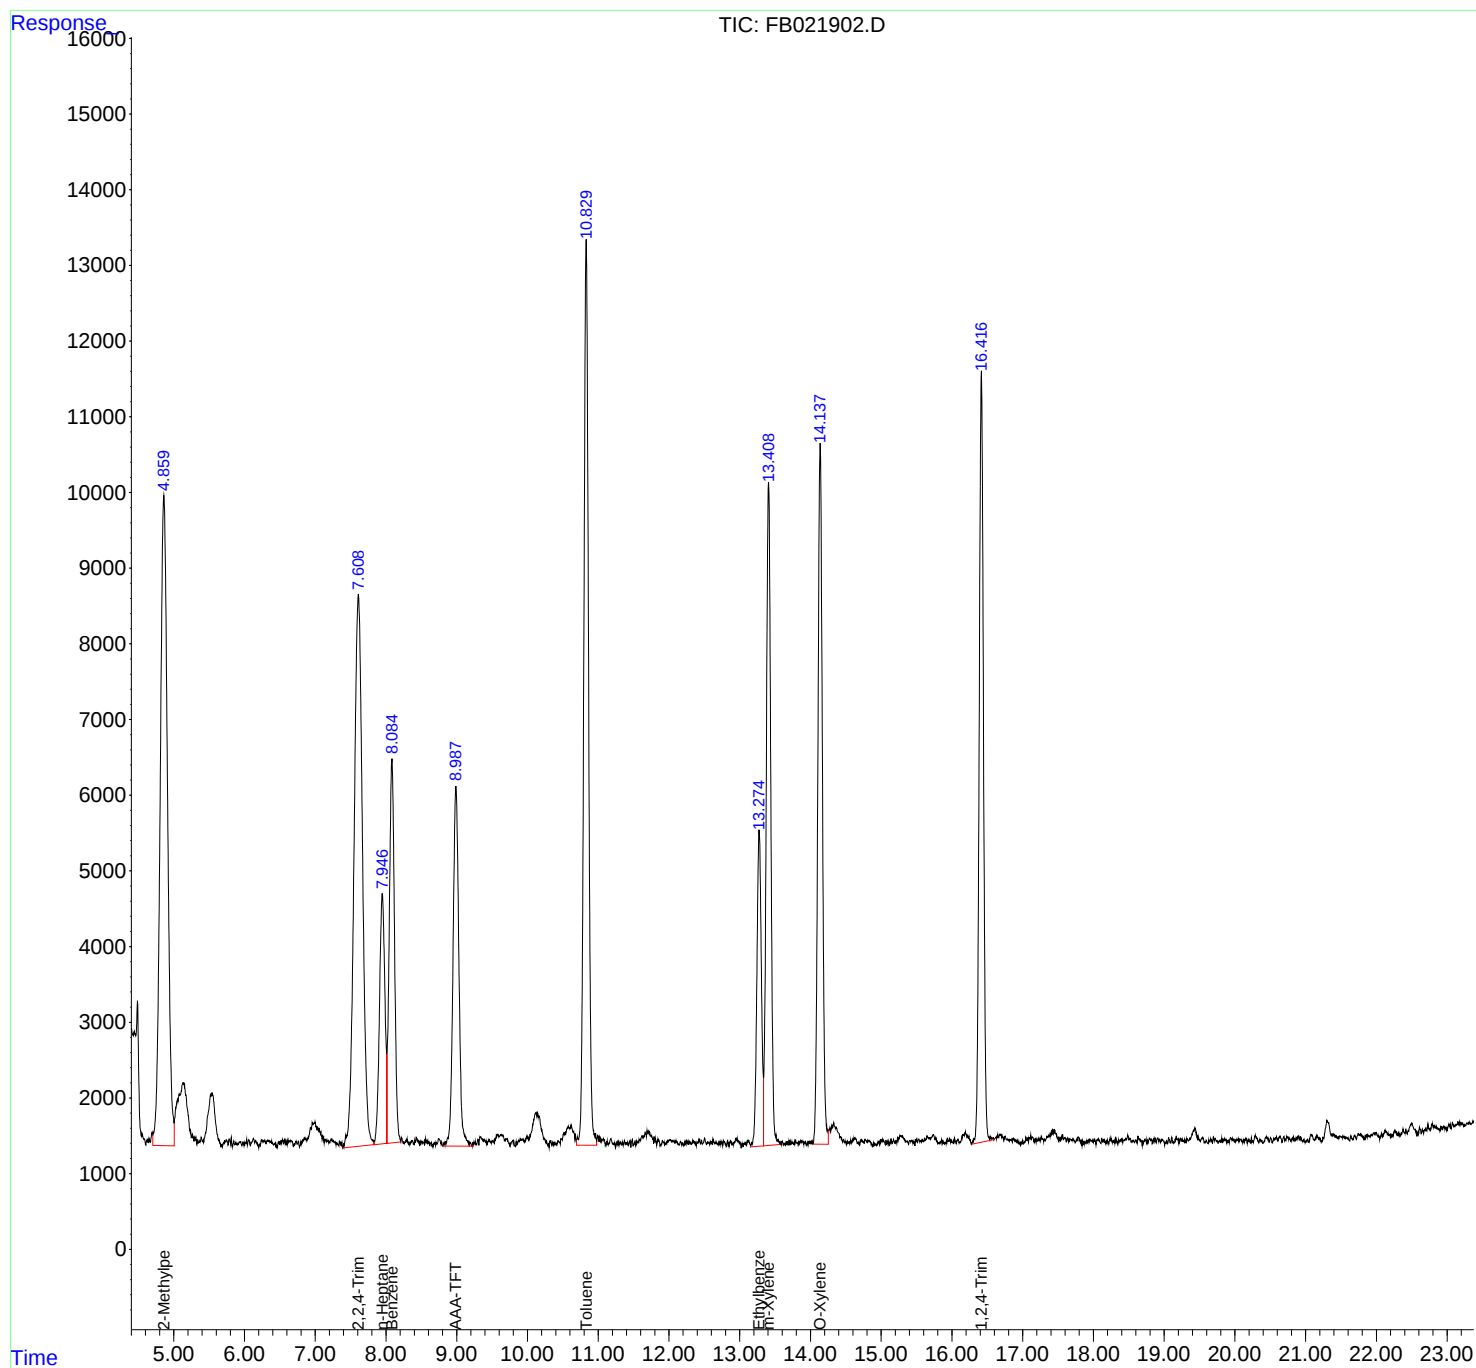

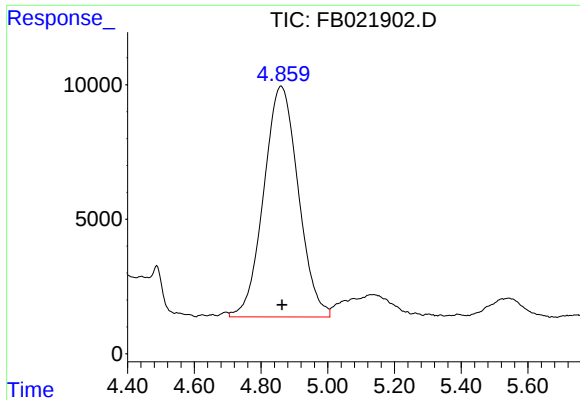


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 616541
Conc: 22.36 ng/ml

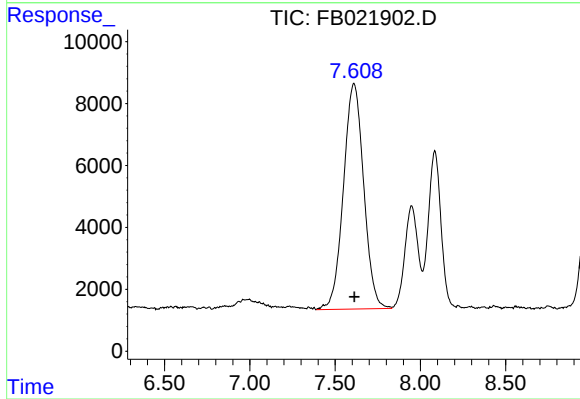


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.002 min
Response: 601546
Conc: 22.76 ng/ml

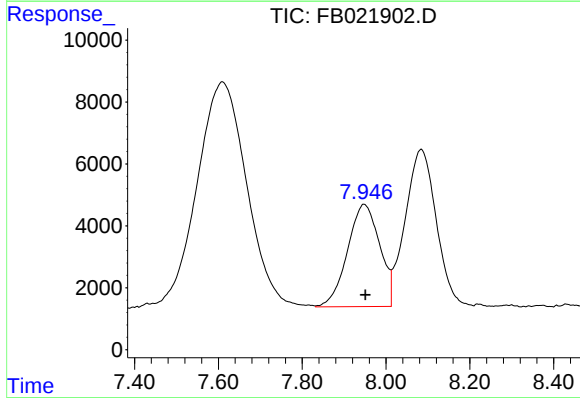


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.003 min
Response: 175884
Conc: 7.09 ng/ml

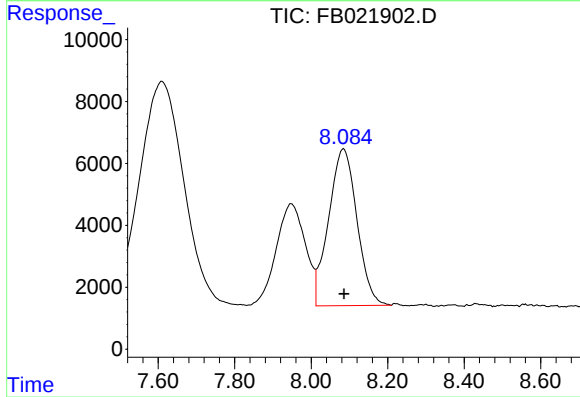


#4 Benzene

R.T.: 8.085 min
Delta R.T.: -0.001 min
Response: 260476
Conc: 8.92 ng/ml

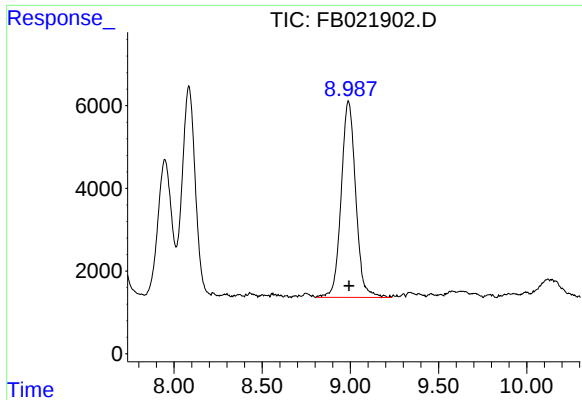


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 271190
Conc: 19.87 ng/ml

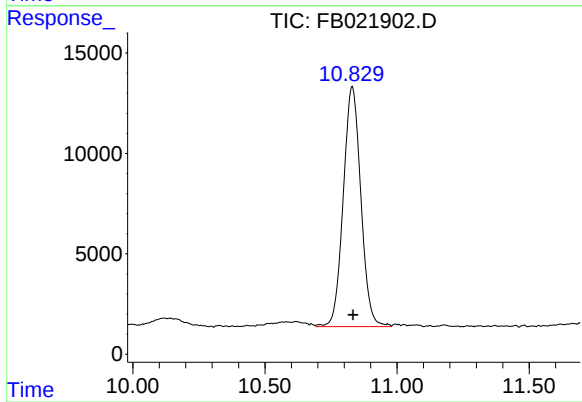


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 552288
Conc: 26.84 ng/ml

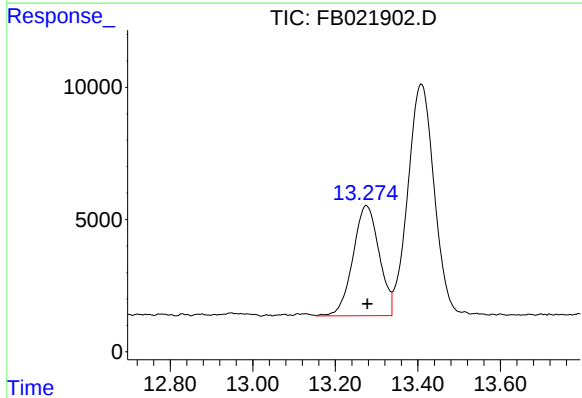


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 183491
Conc: 8.82 ng/ml

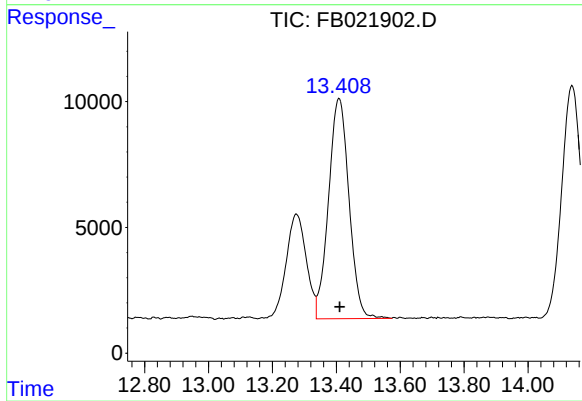


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 389522
Conc: 17.53 ng/ml

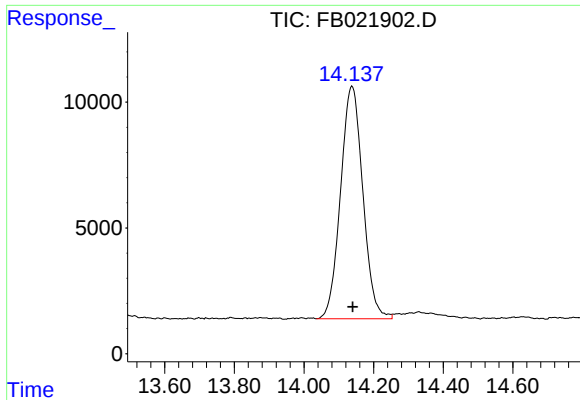

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 410893
Conc: 17.86 ng/ml

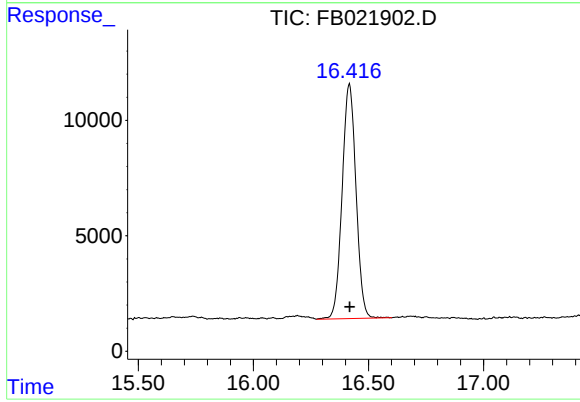

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 425062
Conc: 18.03 ng/ml