

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080222\
 Data File : FB027783.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2022 13:32
 Operator : AJ/MA
 Sample : BSF0802W2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 01:02:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	279004	23.973 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	544227	25.842 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	604058	29.109 ng/ml
3) t n-Heptane	7.755	198503	9.655 ng/ml
4) t Benzene	7.892	233936	9.969 ng/ml
6) t Toluene	10.625	672548	30.119 ng/ml
7) t Ethylbenzene	13.062	208124	9.932 ng/ml
8) t m-Xylene	13.195	415466	19.843 ng/ml
9) t O-Xylene	13.922	404324	19.759 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	390465	18.789 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080222\
Data File : FB027783.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2022 13:32
Operator : AJ/MA
Sample : BSF0802W2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 01:02:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

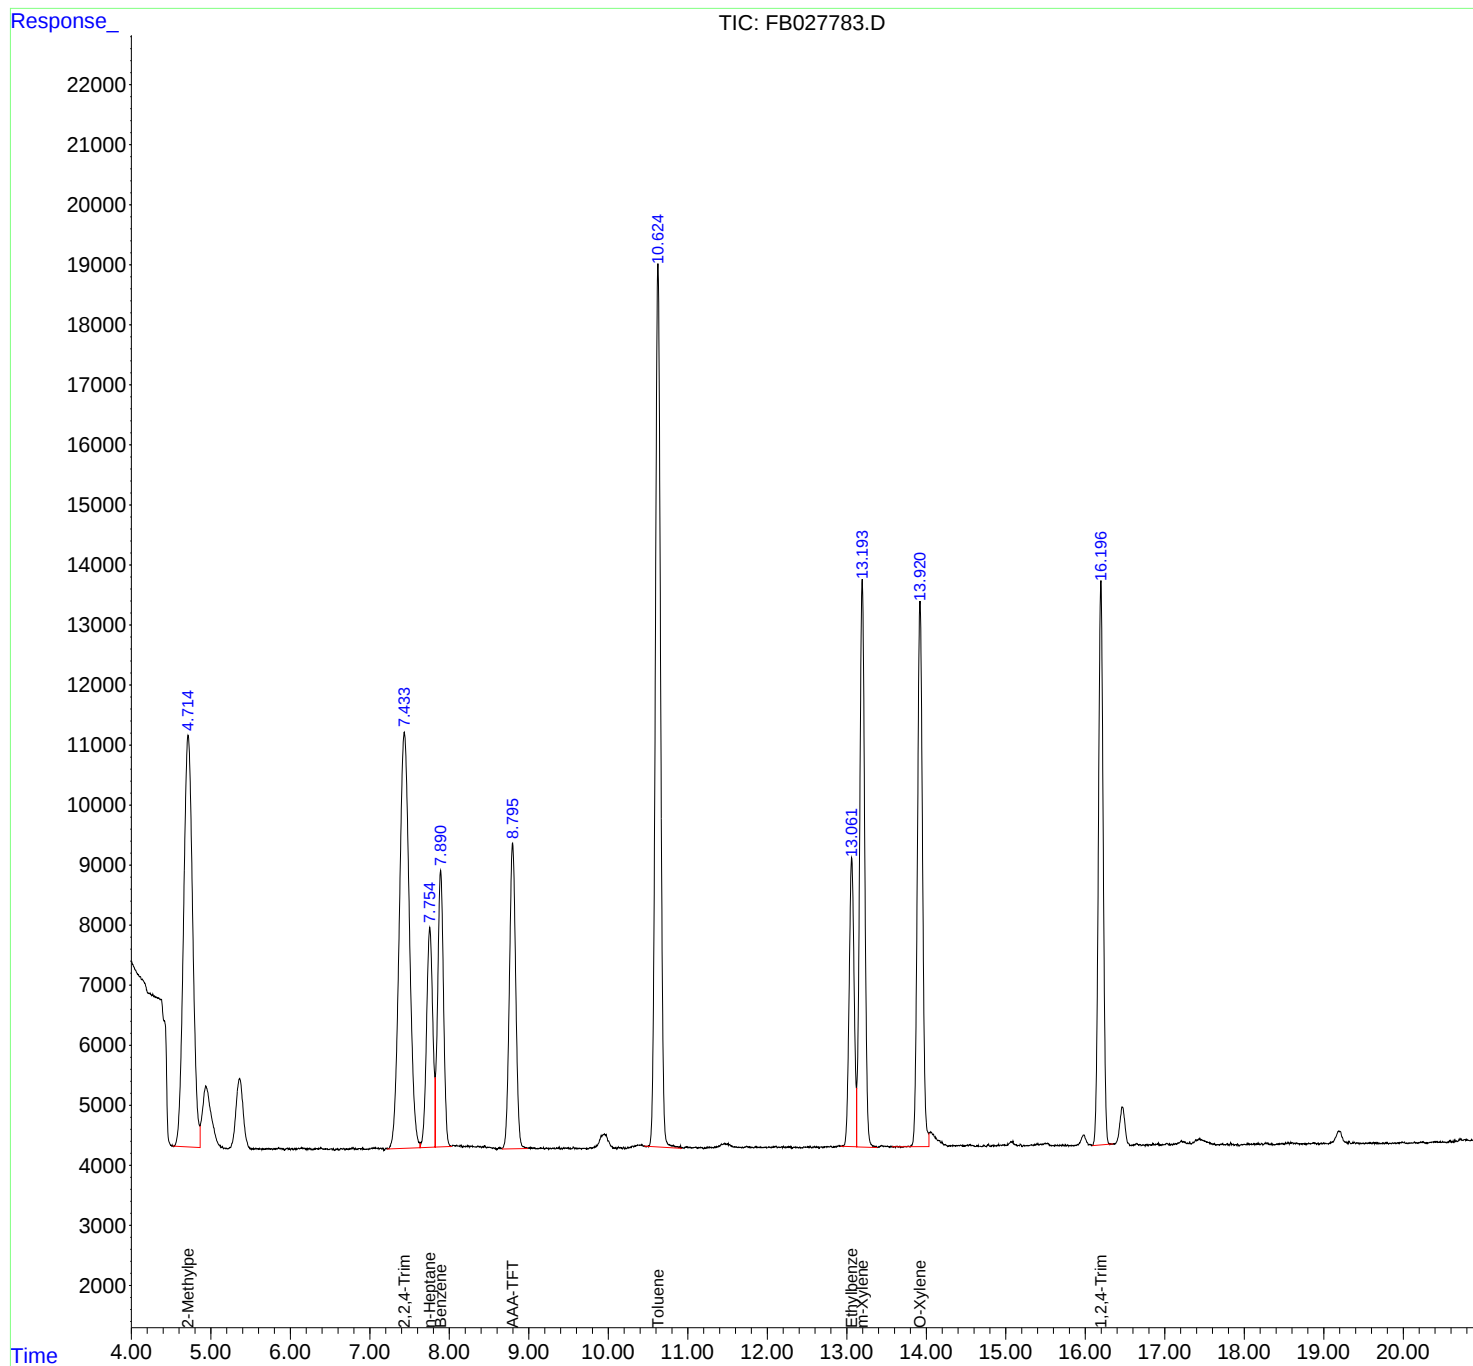

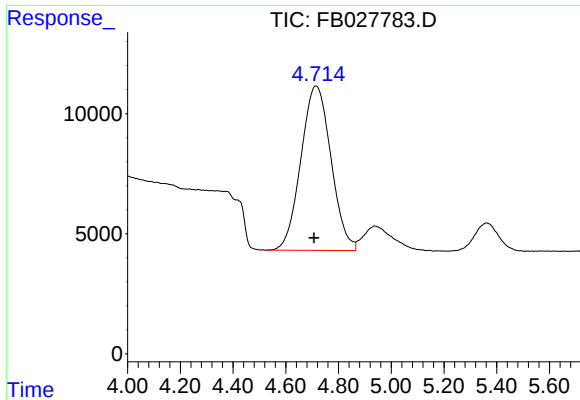


#1 2-Methylpentane

R.T.: 4.715 min
Delta R.T.: 0.008 min
Response: 544227
Conc: 25.84 ng/ml

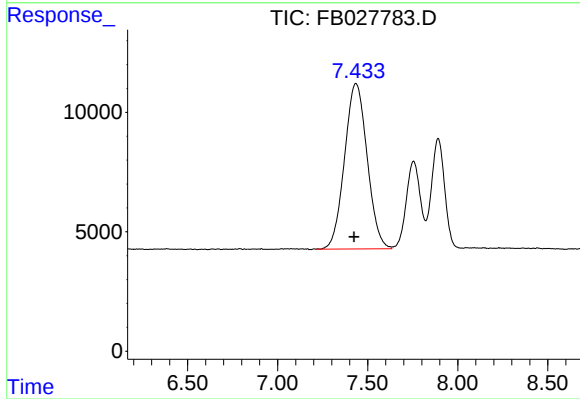


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.010 min
Response: 604058
Conc: 29.11 ng/ml

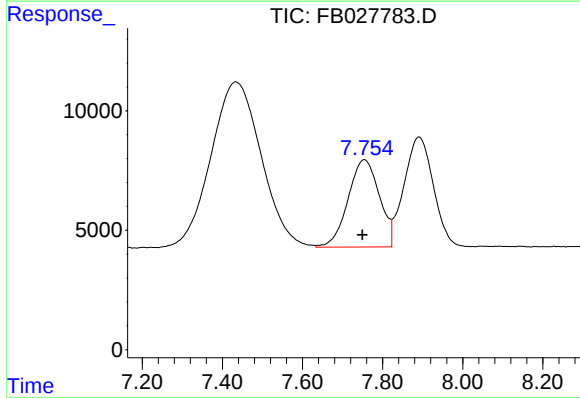


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.005 min
Response: 198503
Conc: 9.66 ng/ml

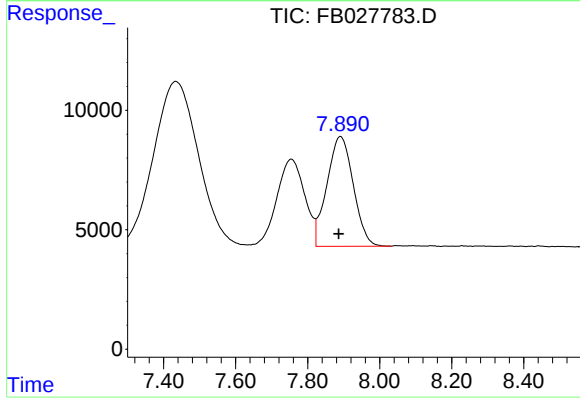


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.005 min
Response: 233936
Conc: 9.97 ng/ml

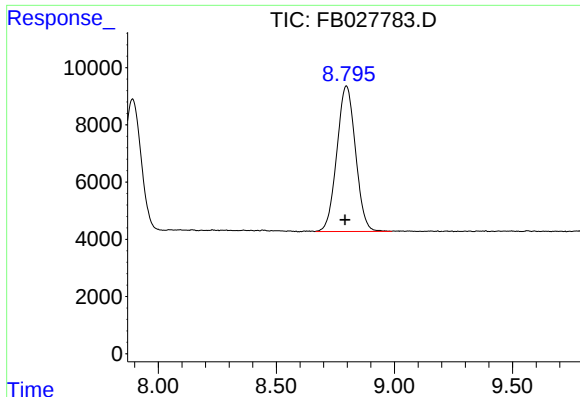


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 279004
Conc: 23.97 ng/ml

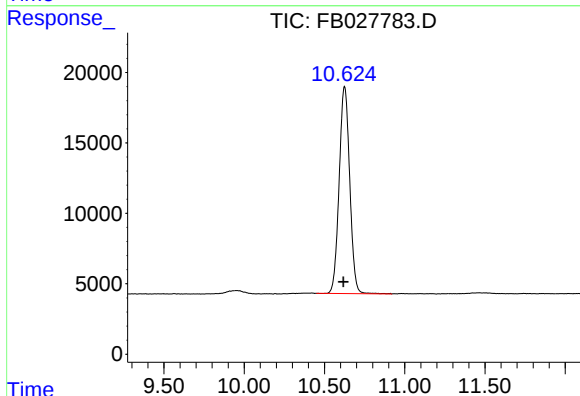


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 672548
Conc: 30.12 ng/ml

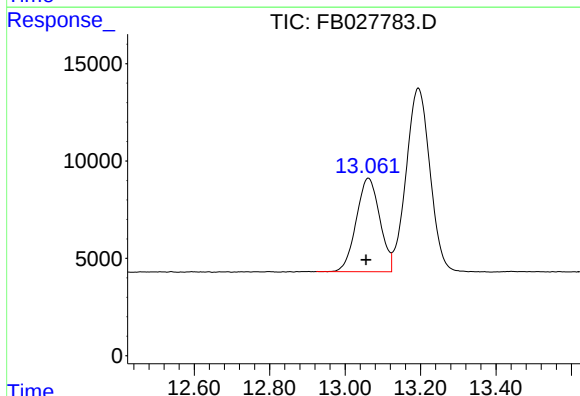


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.007 min
Response: 208124
Conc: 9.93 ng/ml

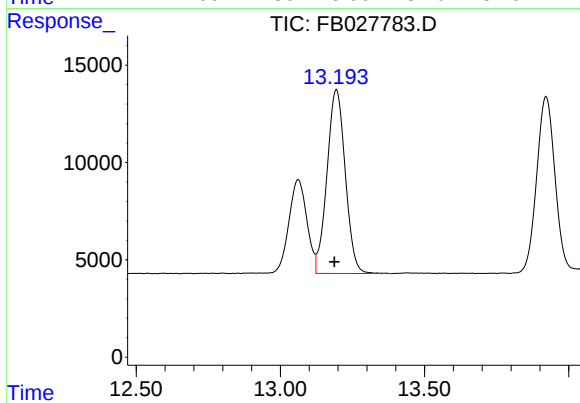


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: 0.007 min
Response: 415466
Conc: 19.84 ng/ml

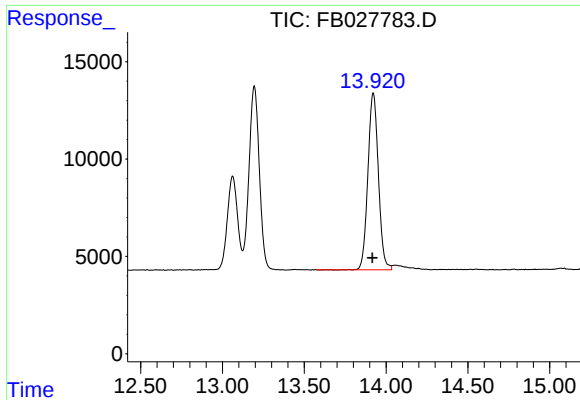

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 404324
Conc: 19.76 ng/ml

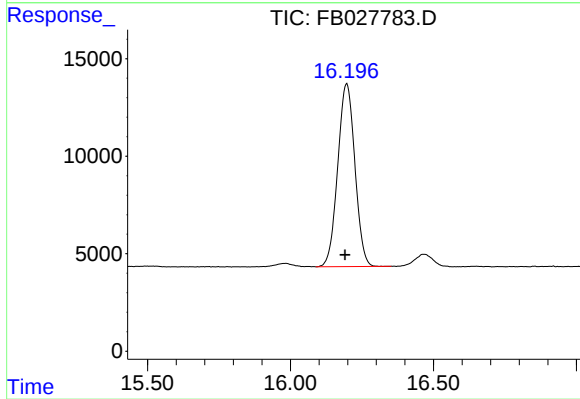

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.006 min
Response: 390465
Conc: 18.79 ng/ml