

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080222\
 Data File : FB027784.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2022 14:14
 Operator : AJ/MA
 Sample : N3980-07
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 01:15:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	216433	18.597 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	42714	2.028 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	36634	1.765 ng/ml
3) t n-Heptane	7.757	11774	0.573 ng/ml
4) t Benzene	7.896	13521	0.576 ng/ml
6) t Toluene	10.628	43629	1.954 ng/ml
7) t Ethylbenzene	13.065	13524	0.645 ng/ml
8) t m-Xylene	13.197	28801	1.376 ng/ml
9) t O-Xylene	13.921	28575	1.396 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	31563	1.519 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080222\
Data File : FB027784.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2022 14:14
Operator : AJ/MA
Sample : N3980-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 01:15:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

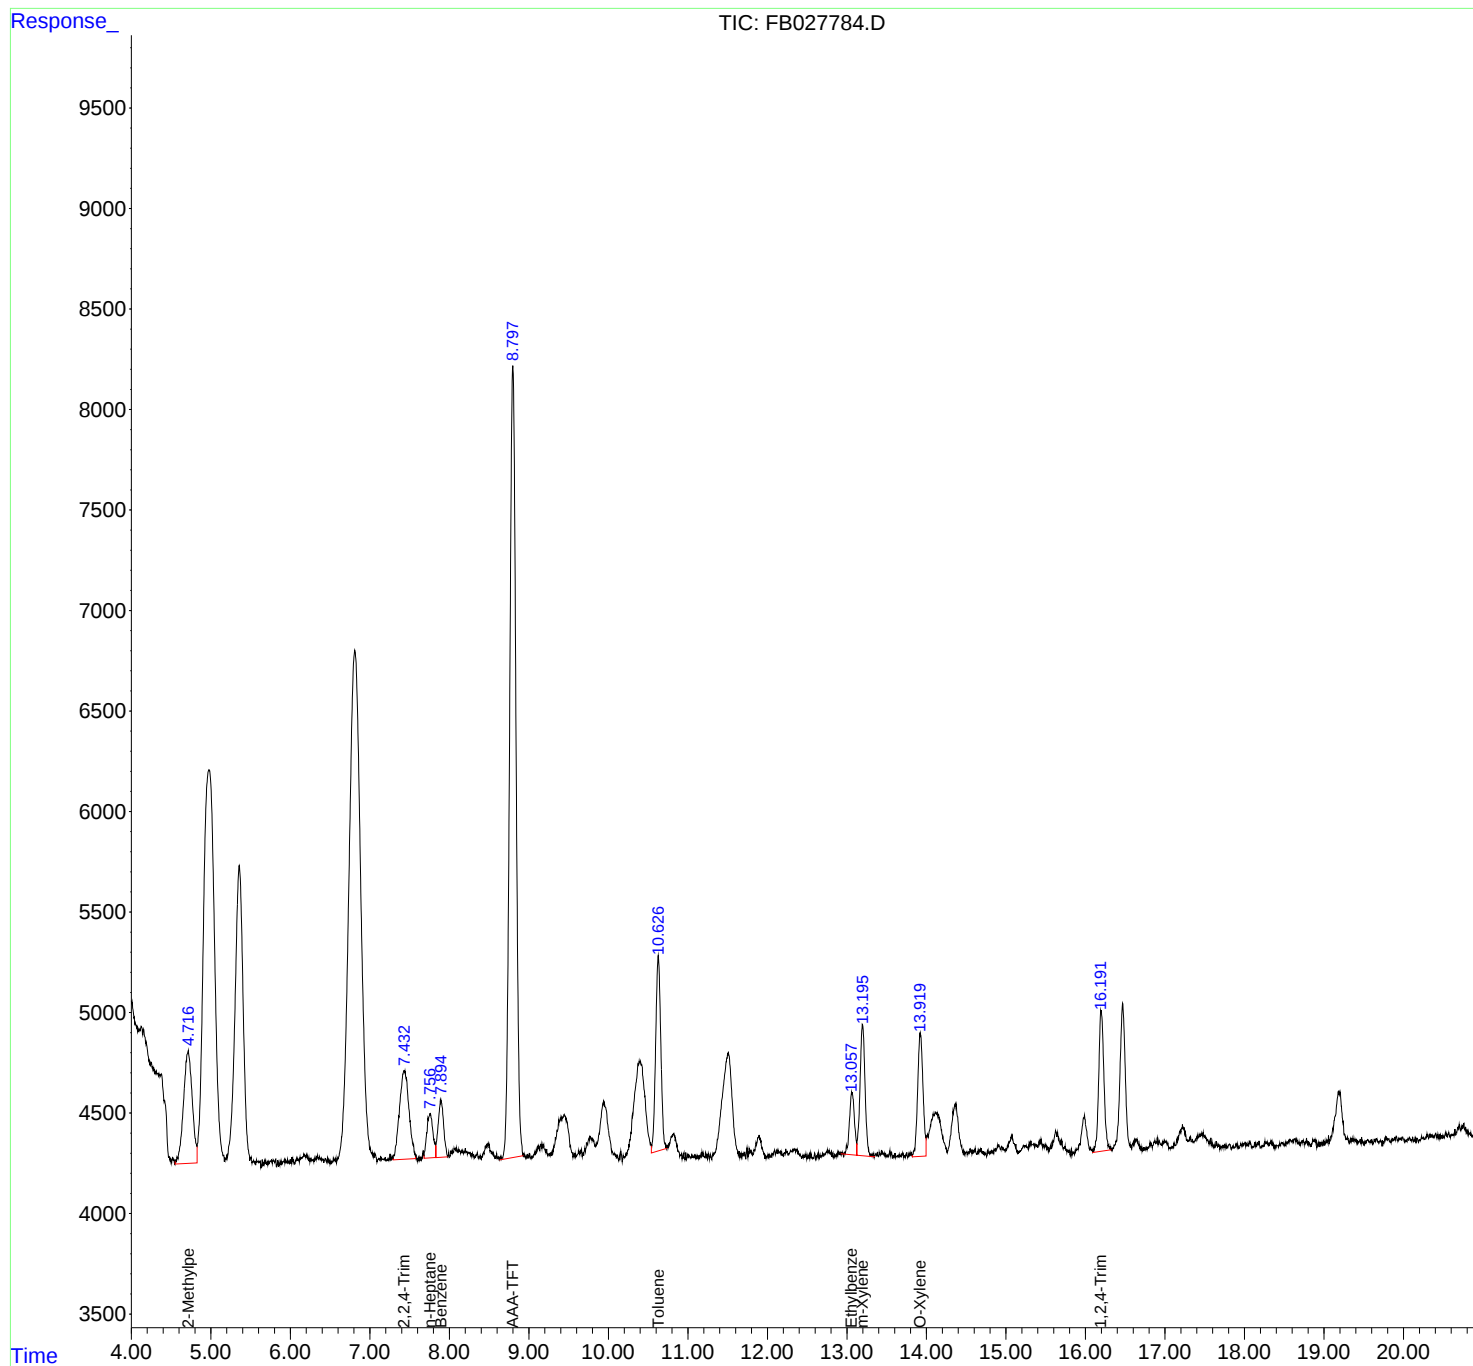

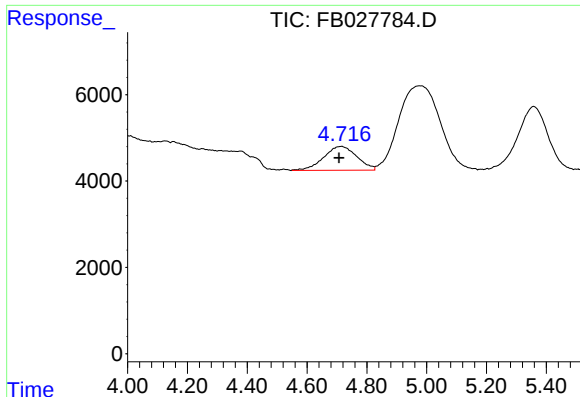


#1 2-Methylpentane

R.T.: 4.718 min
Delta R.T.: 0.011 min
Response: 42714
Conc: 2.03 ng/ml

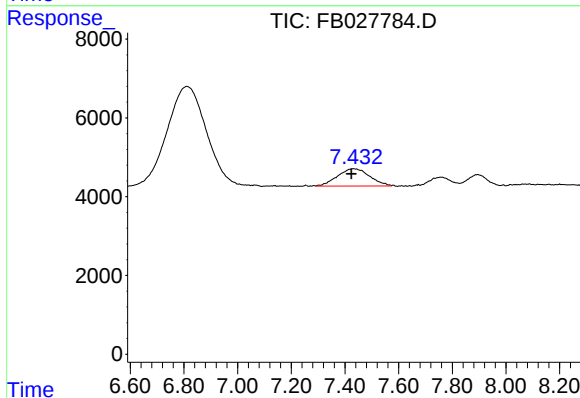


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.009 min
Response: 36634
Conc: 1.77 ng/ml

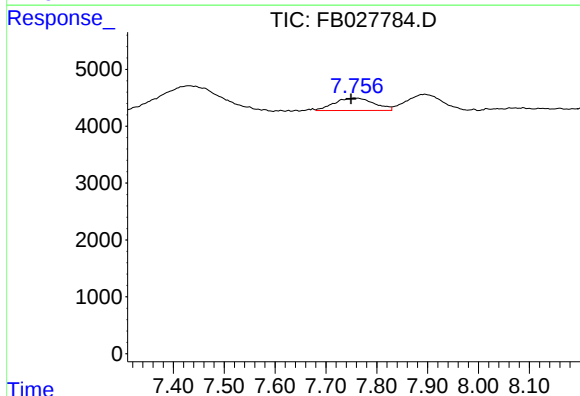


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.007 min
Response: 11774
Conc: 0.57 ng/ml

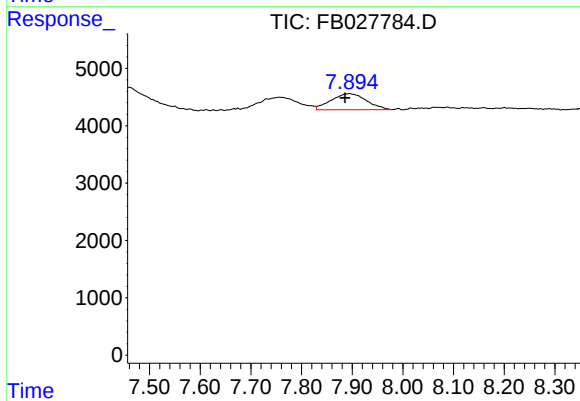


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.010 min
Response: 13521
Conc: 0.58 ng/ml

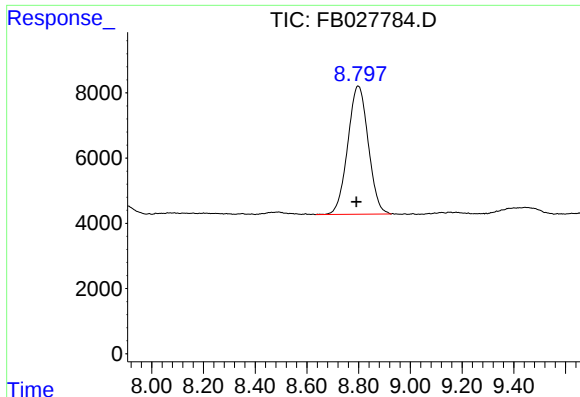


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.008 min
Response: 216433
Conc: 18.60 ng/ml

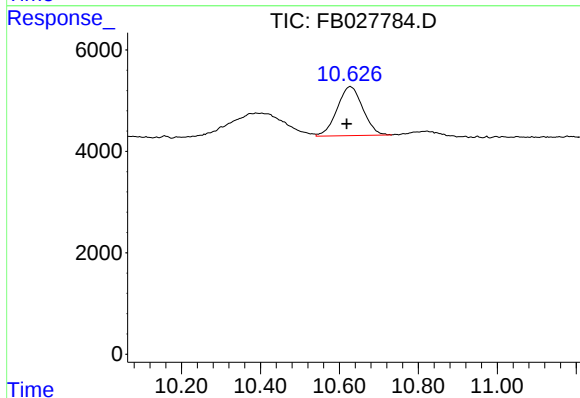


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.009 min
Response: 43629
Conc: 1.95 ng/ml

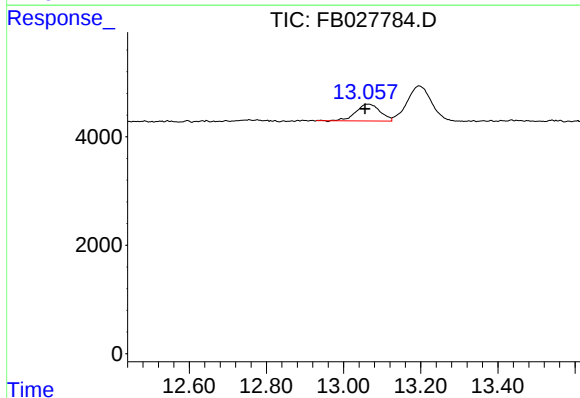


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.009 min
Response: 13524
Conc: 0.65 ng/ml

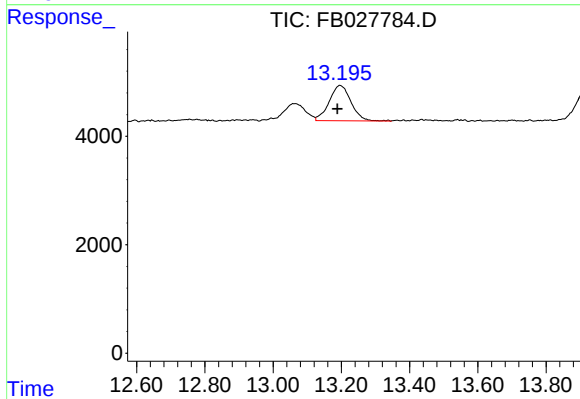


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: 0.009 min
Response: 28801
Conc: 1.38 ng/ml

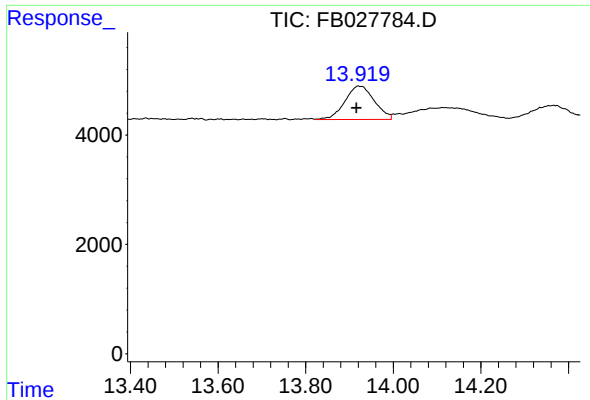

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 28575
Conc: 1.40 ng/ml

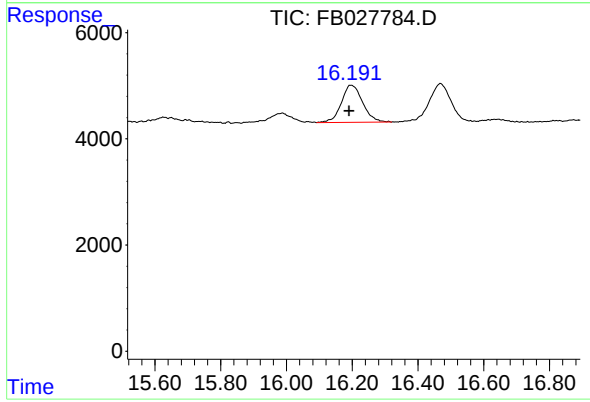

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.007 min
Response: 31563
Conc: 1.52 ng/ml