

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080222\
 Data File : FB027785.D
 Signal(s) : FID2B.CH
 Acq On : 2 Aug 2022 14:51
 Operator : AJ/MA
 Sample : N3980-07
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 01:02:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	224403	19.281 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	129289	6.139 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	139858	6.740 ng/ml
3) t n-Heptane	7.756	45650	2.221 ng/ml
4) t Benzene	7.895	55591	2.369 ng/ml
6) t Toluene	10.628	156026	6.987 ng/ml
7) t Ethylbenzene	13.064	49379	2.357 ng/ml
8) t m-Xylene	13.197	100136	4.783 ng/ml
9) t O-Xylene	13.924	97697	4.775 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	97084	4.672 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080222\
Data File : FB027785.D
Signal(s) : FID2B.CH
Acq On : 2 Aug 2022 14:51
Operator : AJ/MA
Sample : N3980-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 01:02:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

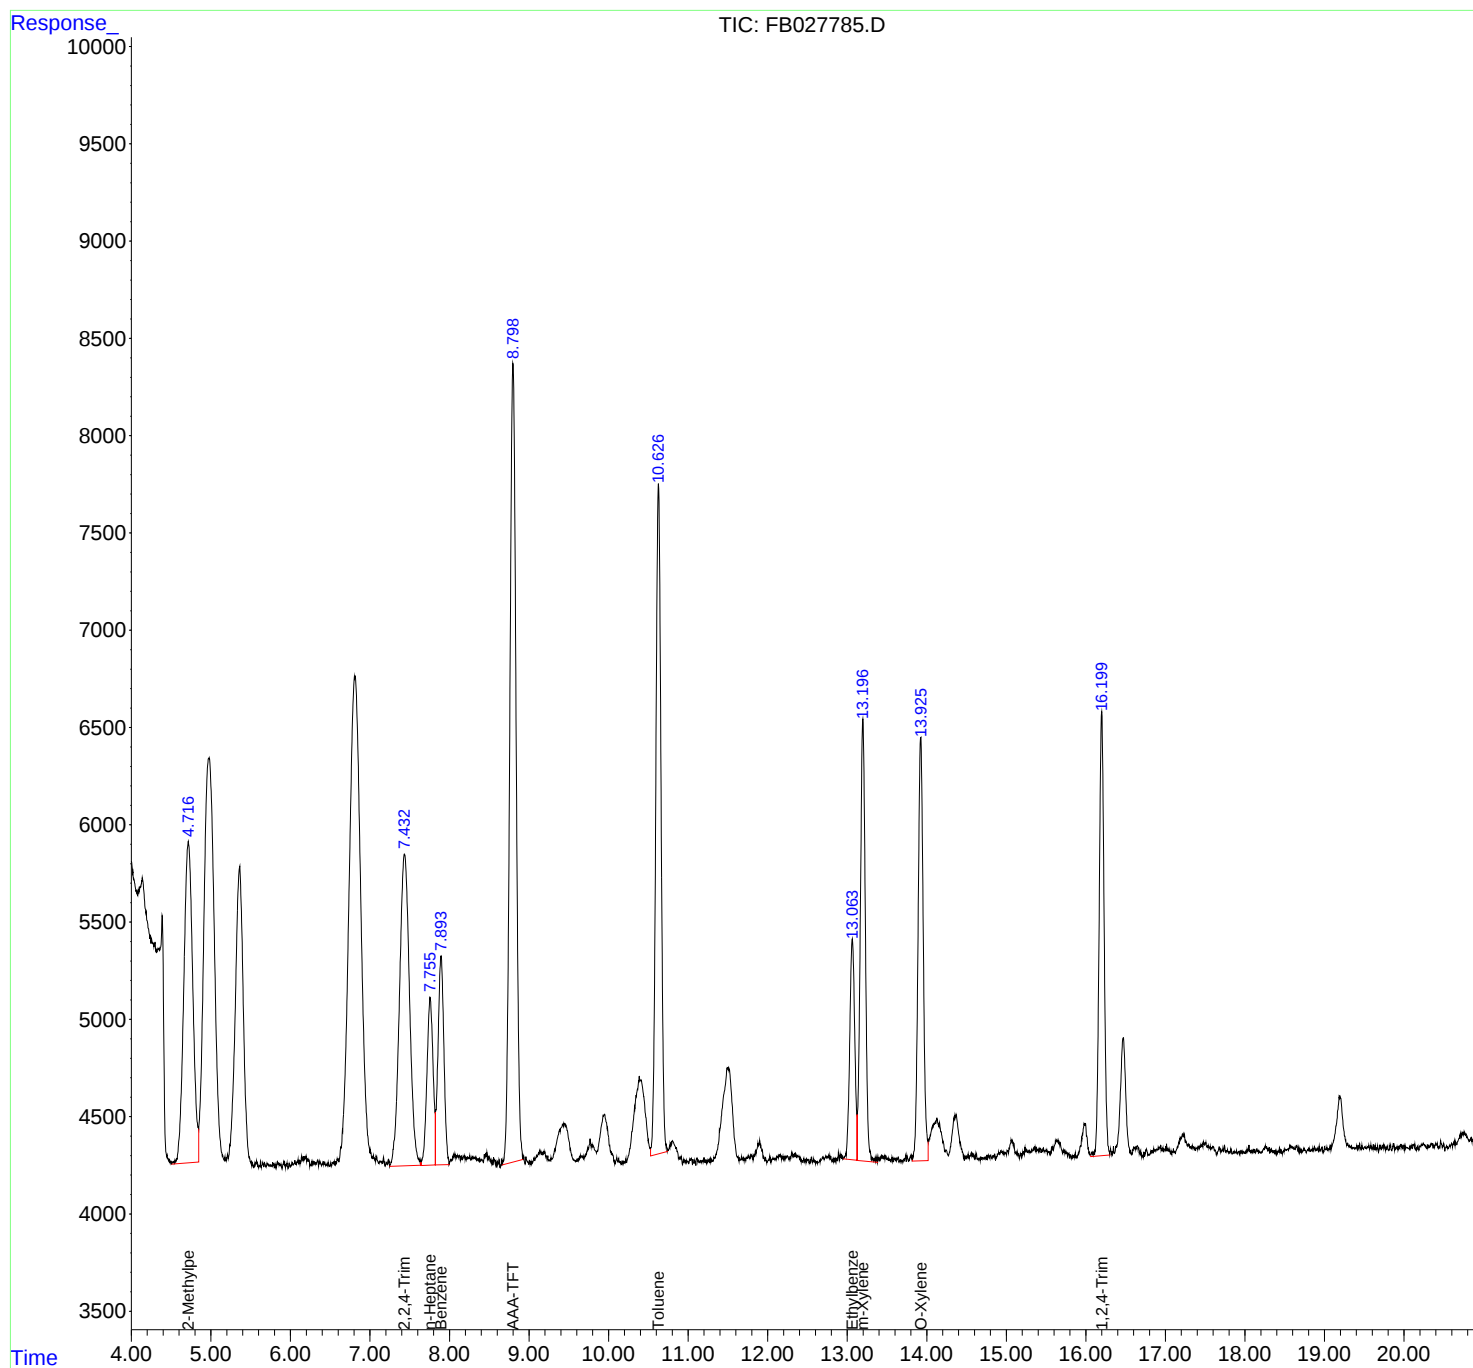

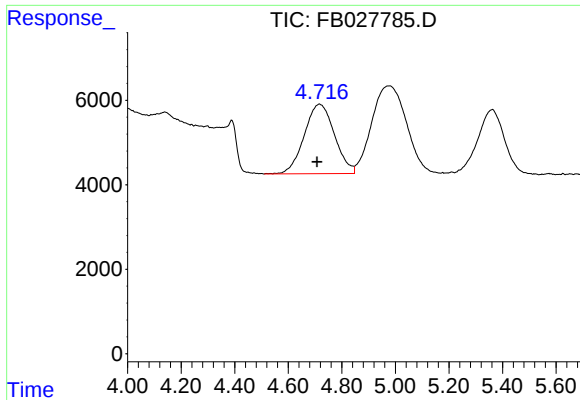


#1 2-Methylpentane

R.T.: 4.717 min
Delta R.T.: 0.010 min
Response: 129289
Conc: 6.14 ng/ml

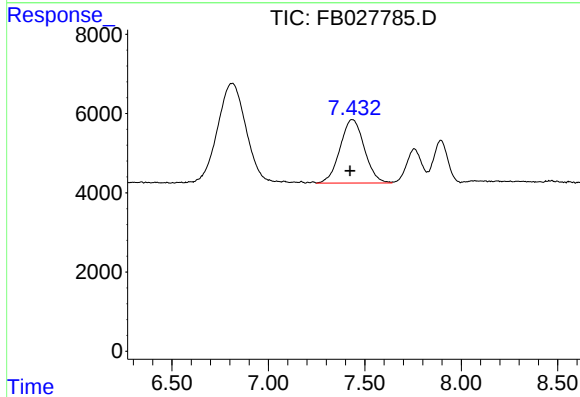


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.010 min
Response: 139858
Conc: 6.74 ng/ml

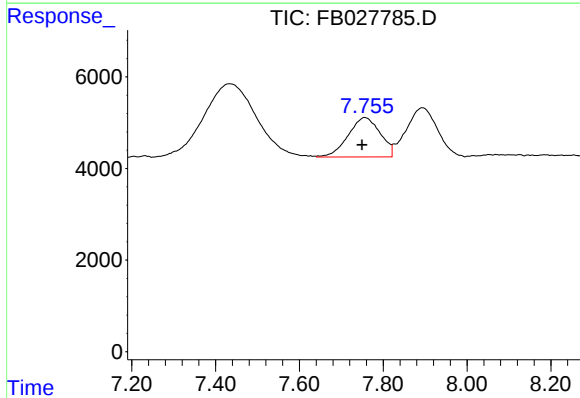


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.007 min
Response: 45650
Conc: 2.22 ng/ml

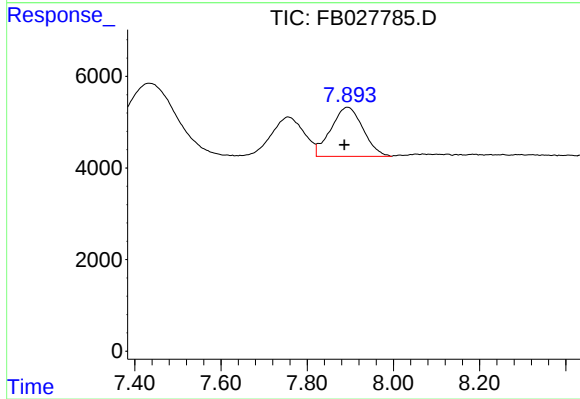


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.008 min
Response: 55591
Conc: 2.37 ng/ml

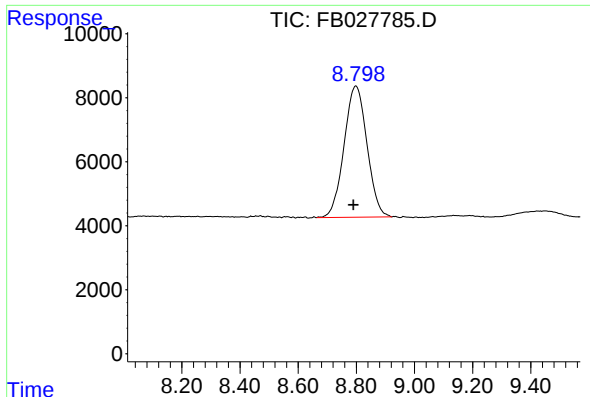


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.008 min
Response: 224403
Conc: 19.28 ng/ml

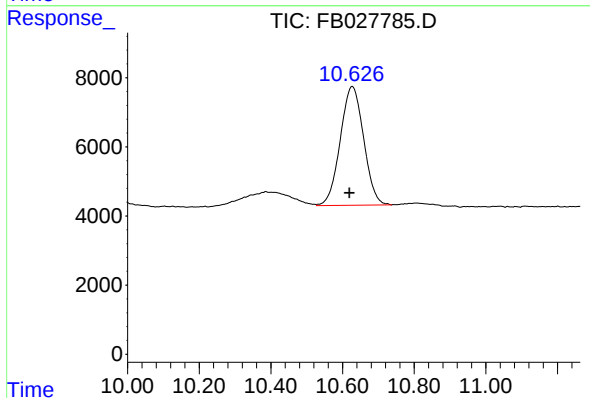


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.009 min
Response: 156026
Conc: 6.99 ng/ml

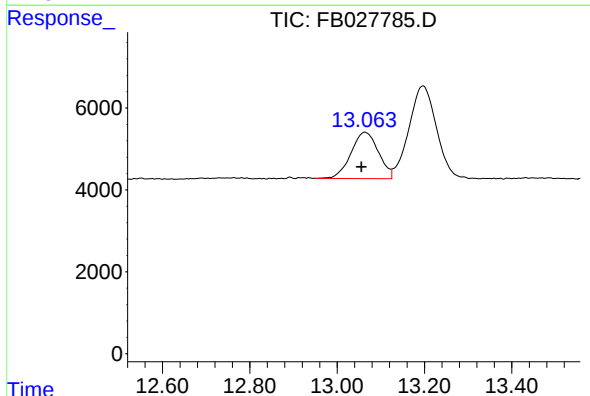


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.008 min
Response: 49379
Conc: 2.36 ng/ml

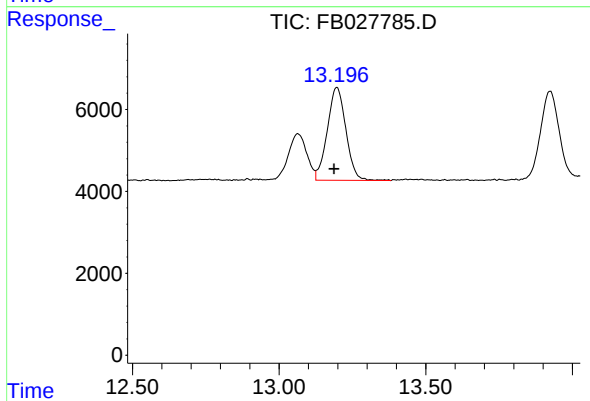


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: 0.010 min
Response: 100136
Conc: 4.78 ng/ml

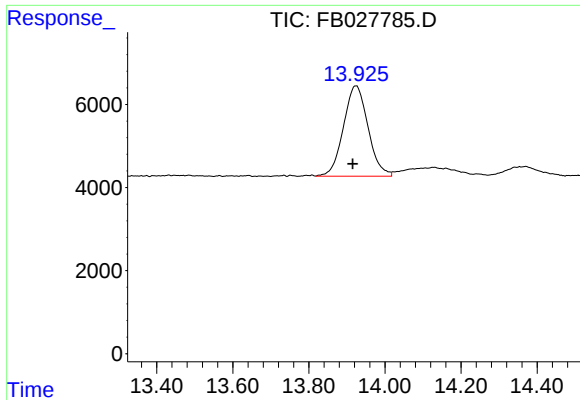

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.009 min
Response: 97697
Conc: 4.77 ng/ml

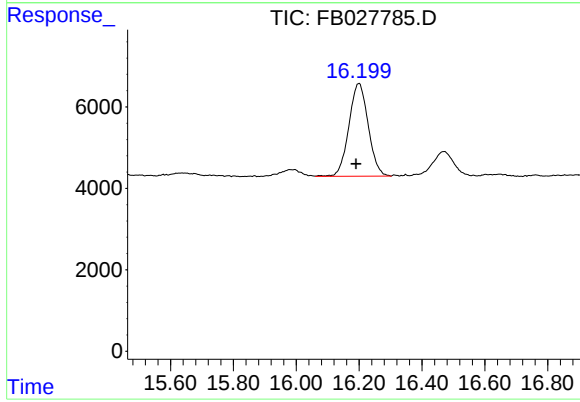

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.010 min
Response: 97084
Conc: 4.67 ng/ml