

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080318\
 Data File : FB017111.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2018 13:46
 Operator : MJ/SJ
 Sample : J4307-20MSD
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 09:17:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.114	168515	21.293 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.966	452520	31.349 ng/ml
2) t 2,2,4-Trimethylpentane	7.731	440828	31.513 ng/ml
3) t n-Heptane	8.070	138328	9.837 ng/ml
4) t Benzene	8.210	174125	9.912 ng/ml
6) t Toluene	10.964	409015	29.784 ng/ml
7) t Ethylbenzene	13.413	130874	9.597 ng/ml
8) t m-Xylene	13.546	274187	19.057 ng/ml
9) t O-Xylene	14.278	290054	19.019 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	345293	18.708 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080318\
Data File : FB017111.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2018 13:46
Operator : MJ/SJ
Sample : J4307-20MSD
Misc : 5.00g/5.00ml DI water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 09:17:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

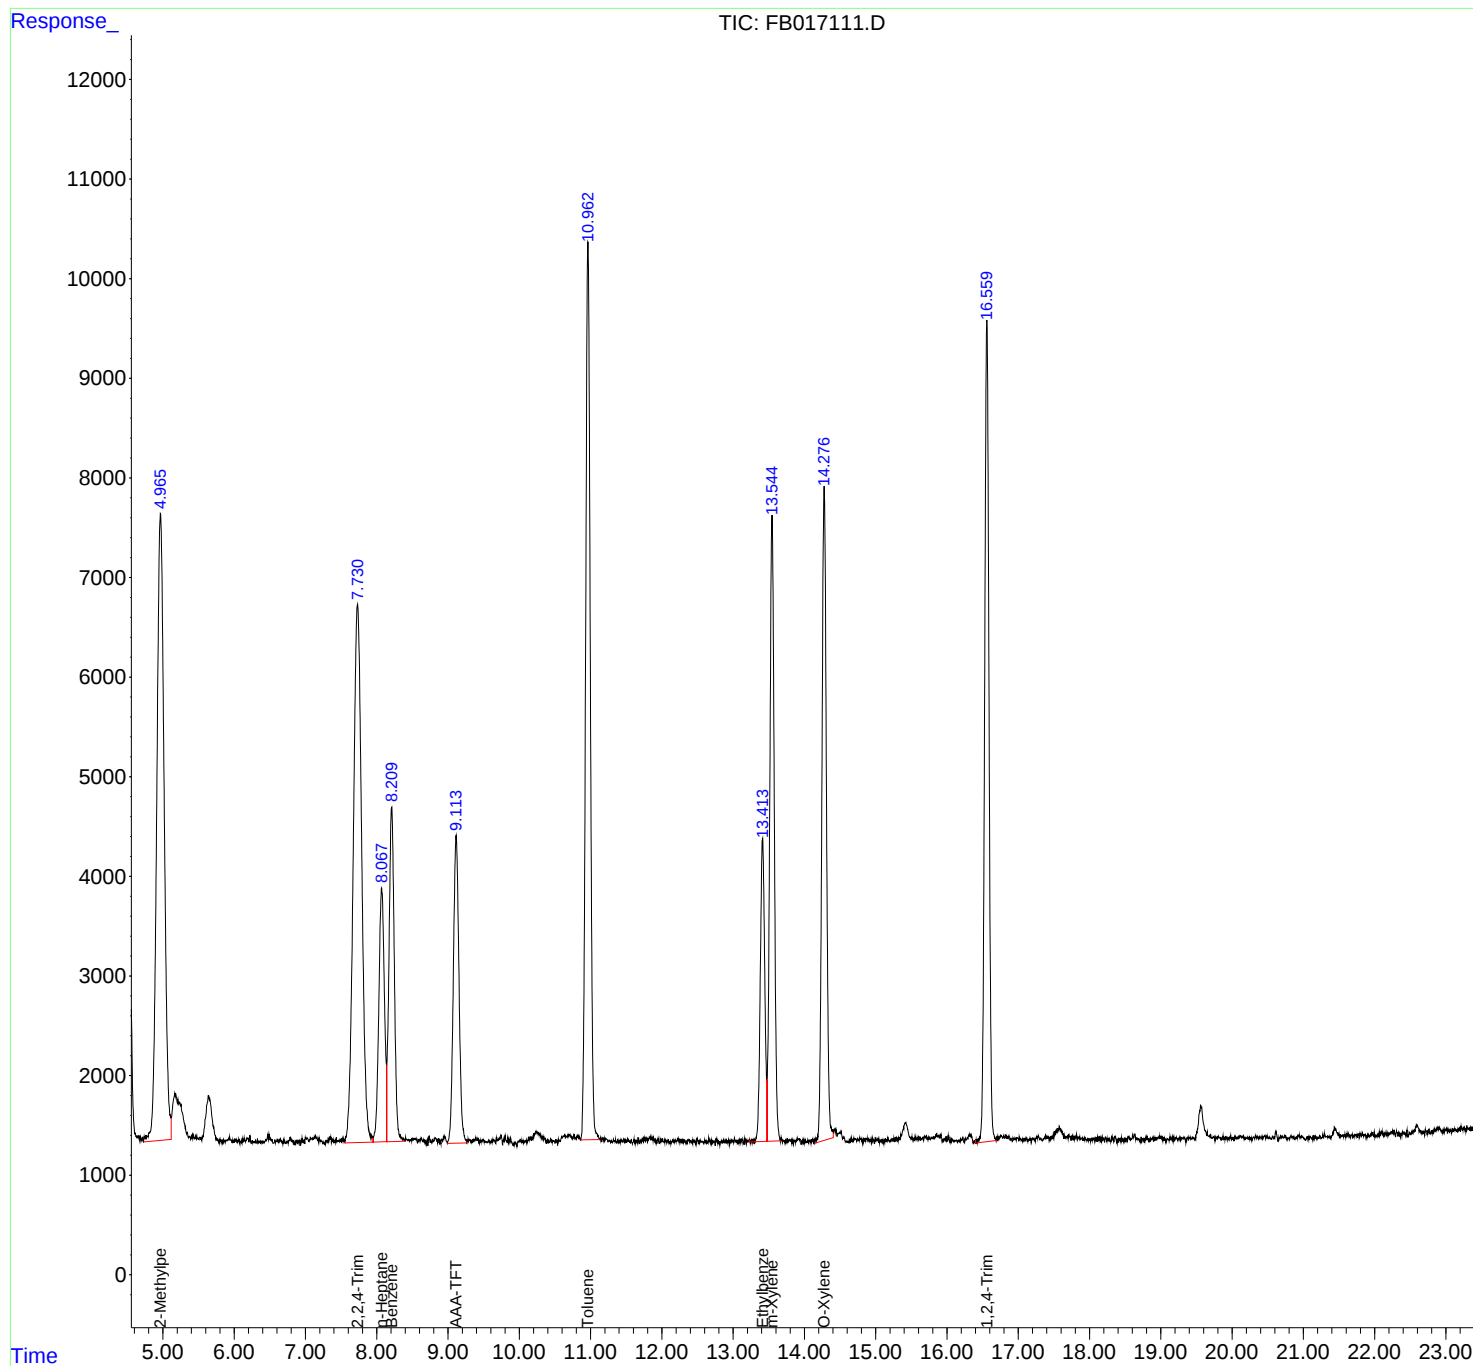

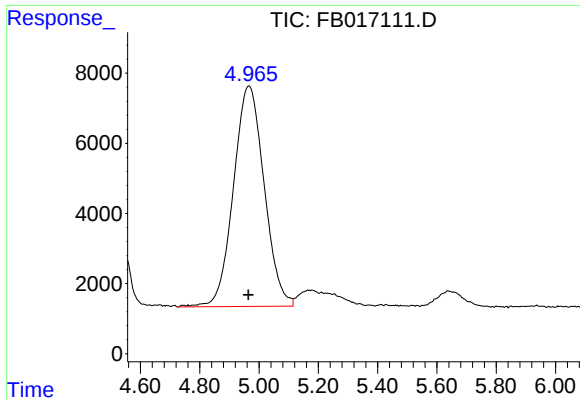


#1 2-Methylpentane

R.T.: 4.966 min
Delta R.T.: 0.002 min
Response: 452520
Conc: 31.35 ng/ml

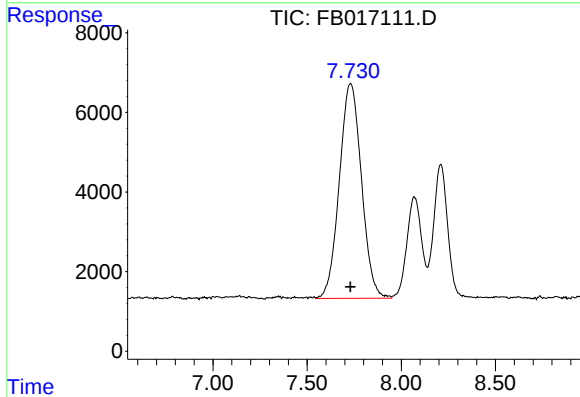


#2 2,2,4-Trimethylpentane

R.T.: 7.731 min
Delta R.T.: 0.000 min
Response: 440828
Conc: 31.51 ng/ml

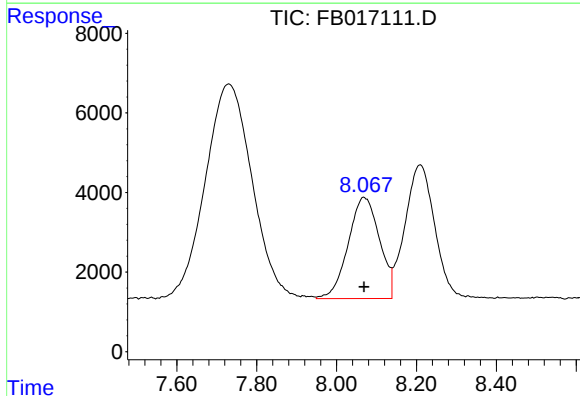


#3 n-Heptane

R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 138328
Conc: 9.84 ng/ml

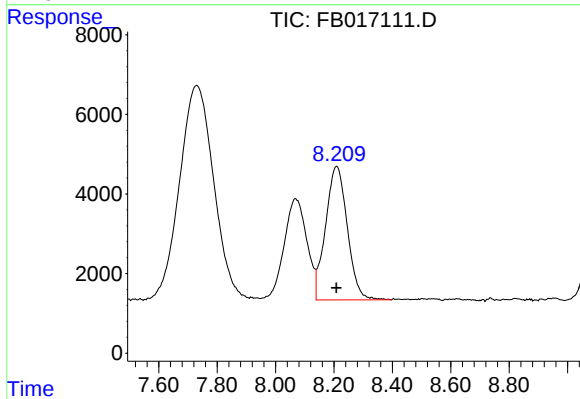


#4 Benzene

R.T.: 8.210 min
Delta R.T.: 0.001 min
Response: 174125
Conc: 9.91 ng/ml

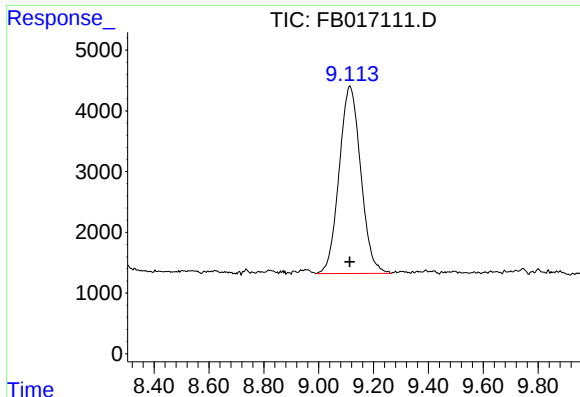


#5 AAA-TFT

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 168515
Conc: 21.29 ng/ml

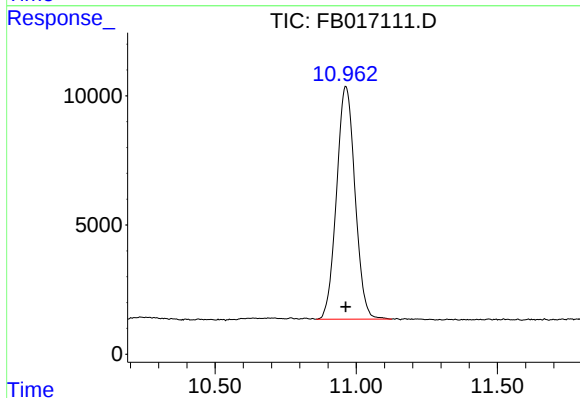


#6 Toluene

R.T.: 10.964 min
Delta R.T.: 0.001 min
Response: 409015
Conc: 29.78 ng/ml

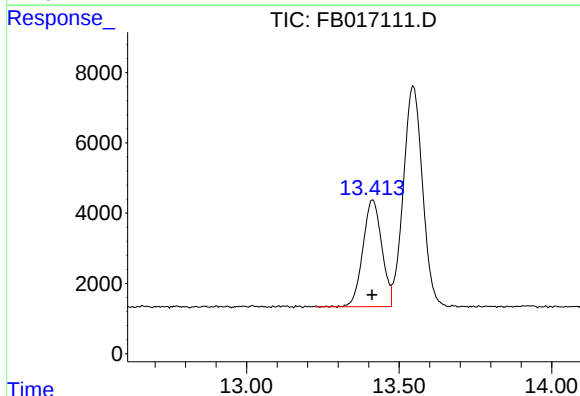


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 130874
Conc: 9.60 ng/ml

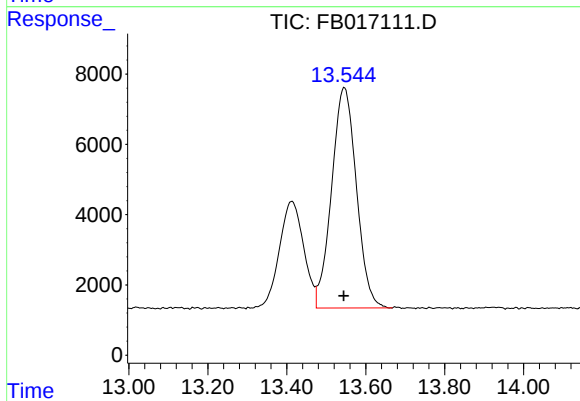

#8 m-Xylene

R.T.: 13.546 min
Delta R.T.: 0.002 min
Response: 274187
Conc: 19.06 ng/ml

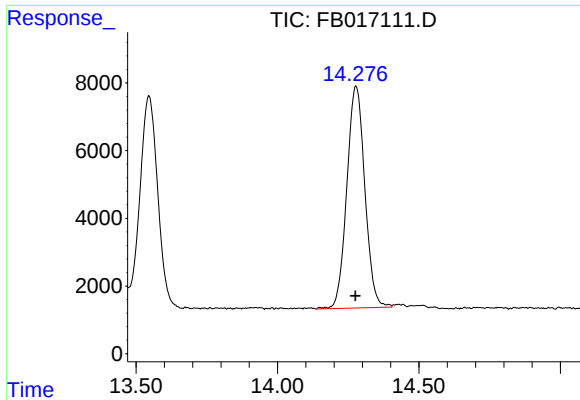


#9 O-Xylene

R.T.: 14.278 min

Delta R.T.: 0.002 min

Response: 290054

Conc: 19.02 ng/ml

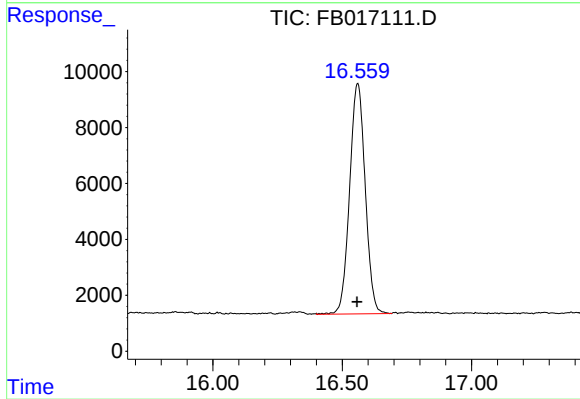

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min

Delta R.T.: 0.002 min

Response: 345293

Conc: 18.71 ng/ml