

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080320\
 Data File : FB024709.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2020 14:51
 Operator : DD/AJ
 Sample : BSF0803S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 04 02:16:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	510880	22.178 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	970274	32.787 ng/ml
2) t	2,2,4-Trimethylpentane	7.420	1067020	34.083 ng/ml
3) t	n-Heptane	7.760	348625	11.213 ng/ml
4) t	Benzene	7.894	419832	11.014 ng/ml
6) t	Toluene	10.632	1205031	32.956 ng/ml
7) t	Ethylbenzene	13.072	367699	10.765 ng/ml
8) t	m-Xylene	13.204	724717	21.475 ng/ml
9) t	O-Xylene	13.932	713537	21.710 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	598818	22.199 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080320\
Data File : FB024709.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2020 14:51
Operator : DD/AJ
Sample : BSF0803S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 04 02:16:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

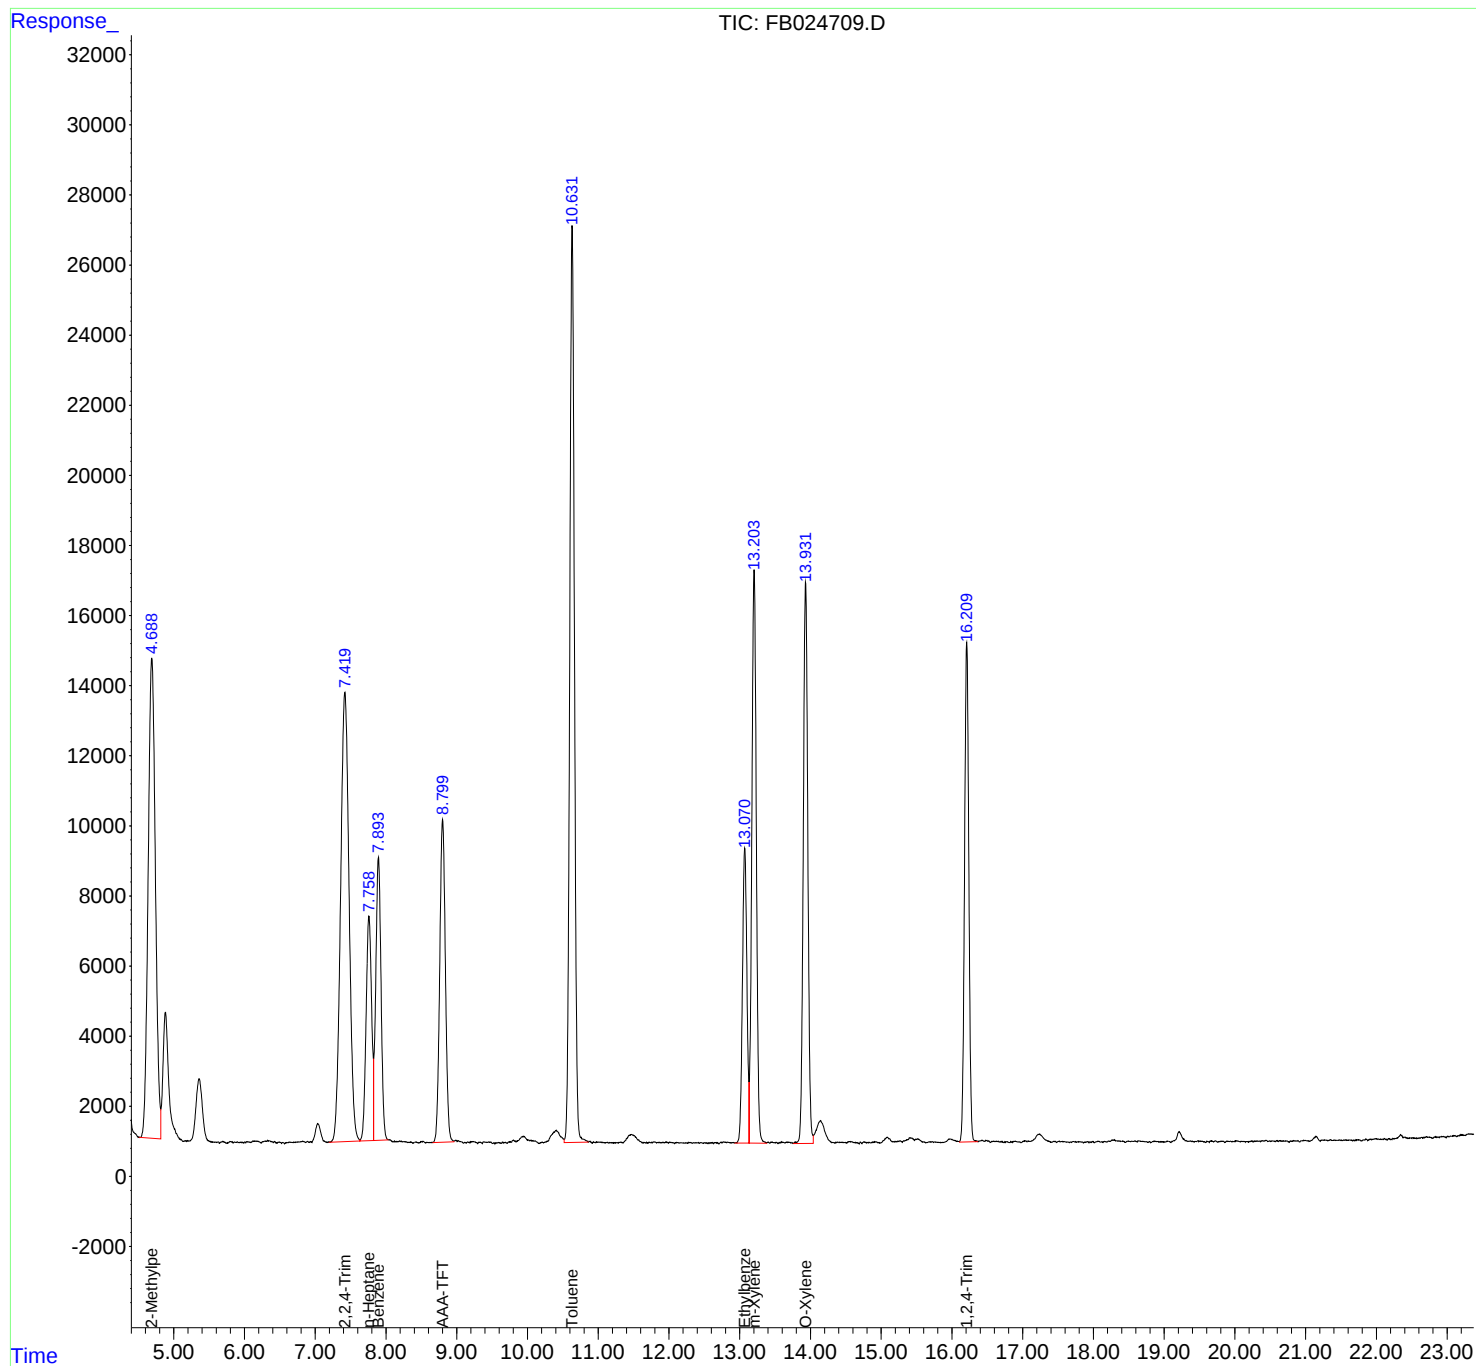

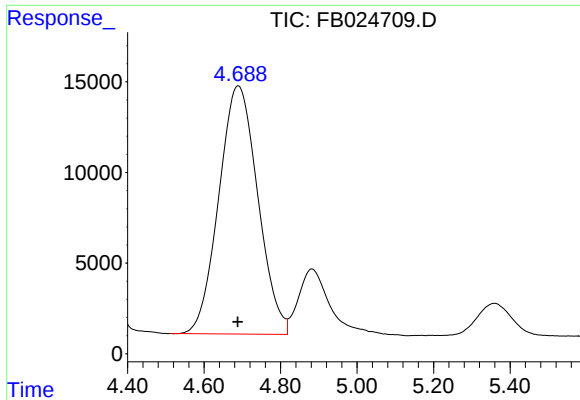


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.002 min
Response: 970274
Conc: 32.79 ng/ml

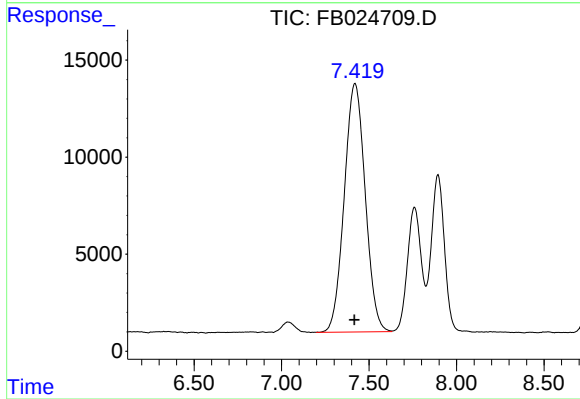


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.004 min
Response: 1067020
Conc: 34.08 ng/ml

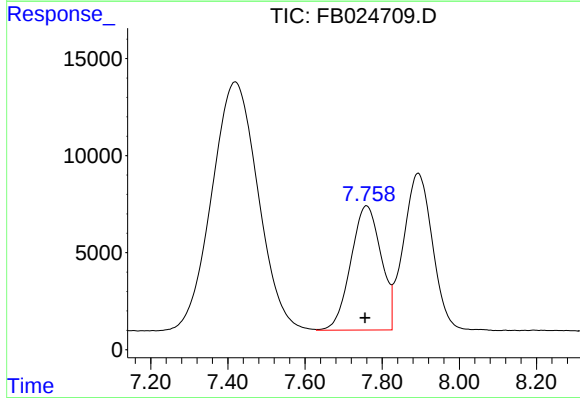


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.004 min
Response: 348625
Conc: 11.21 ng/ml

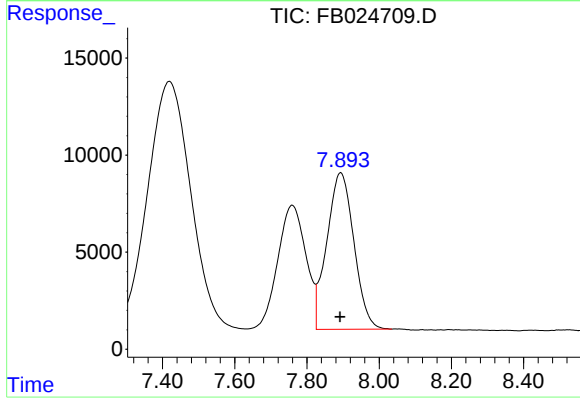


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 419832
Conc: 11.01 ng/ml

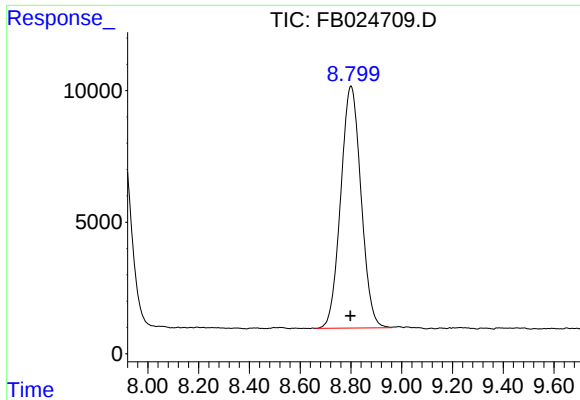


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 510880
Conc: 22.18 ng/ml

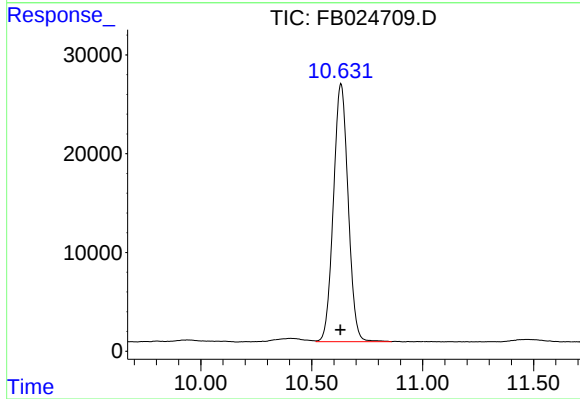


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.003 min
Response: 1205031
Conc: 32.96 ng/ml

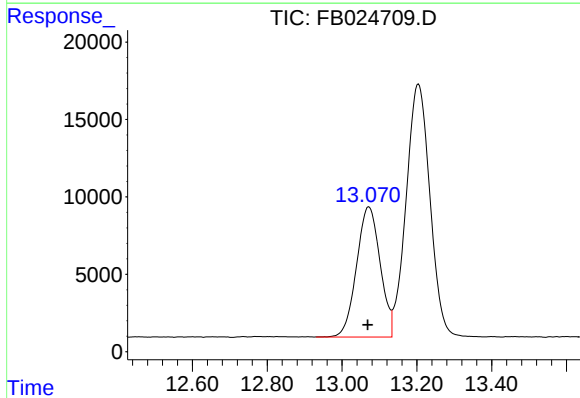


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.003 min
Response: 367699
Conc: 10.77 ng/ml

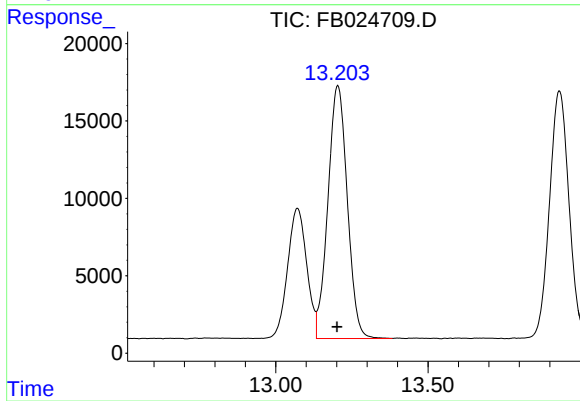


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 724717
Conc: 21.48 ng/ml

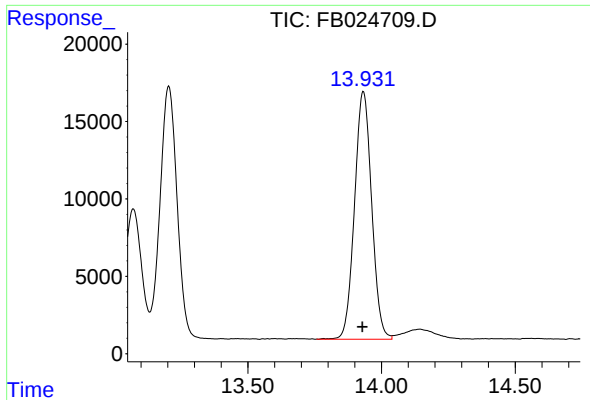

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.003 min
Response: 713537
Conc: 21.71 ng/ml

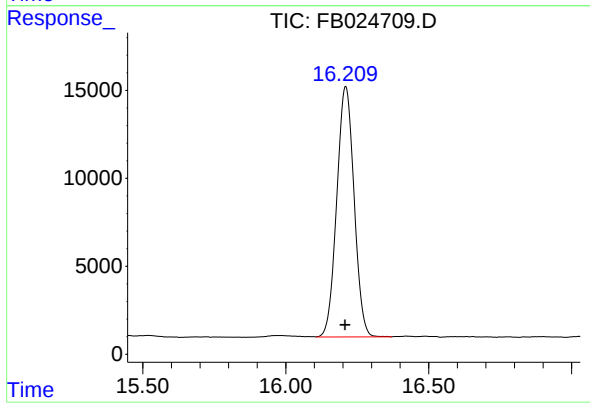

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 598818
Conc: 22.20 ng/ml