

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080320\
Data File : FB024711.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2020 15:53
Operator : DD/AJ
Sample : L3507-02MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 04 02:16:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.810	50507	2.193 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.697	79289	2.679 ng/ml
2) t	2,2,4-Trimethylpentane	7.424	44708	1.428 ng/ml
3) t	n-Heptane	7.758	12194	0.392 ng/ml
4) t	Benzene	7.898	37286	0.978 ng/ml
6) t	Toluene	10.634	86846	2.375 ng/ml
7) t	Ethylbenzene	13.075	19993	0.585 ng/ml
8) t	m-Xylene	13.209	35257	1.045 ng/ml
9) t	O-Xylene	13.936	35825	1.090 ng/ml
10) t	1,2,4-Trimethylbenzene	16.213	15361	0.569 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080320\
Data File : FB024711.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2020 15:53
Operator : DD/AJ
Sample : L3507-02MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 04 02:16:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

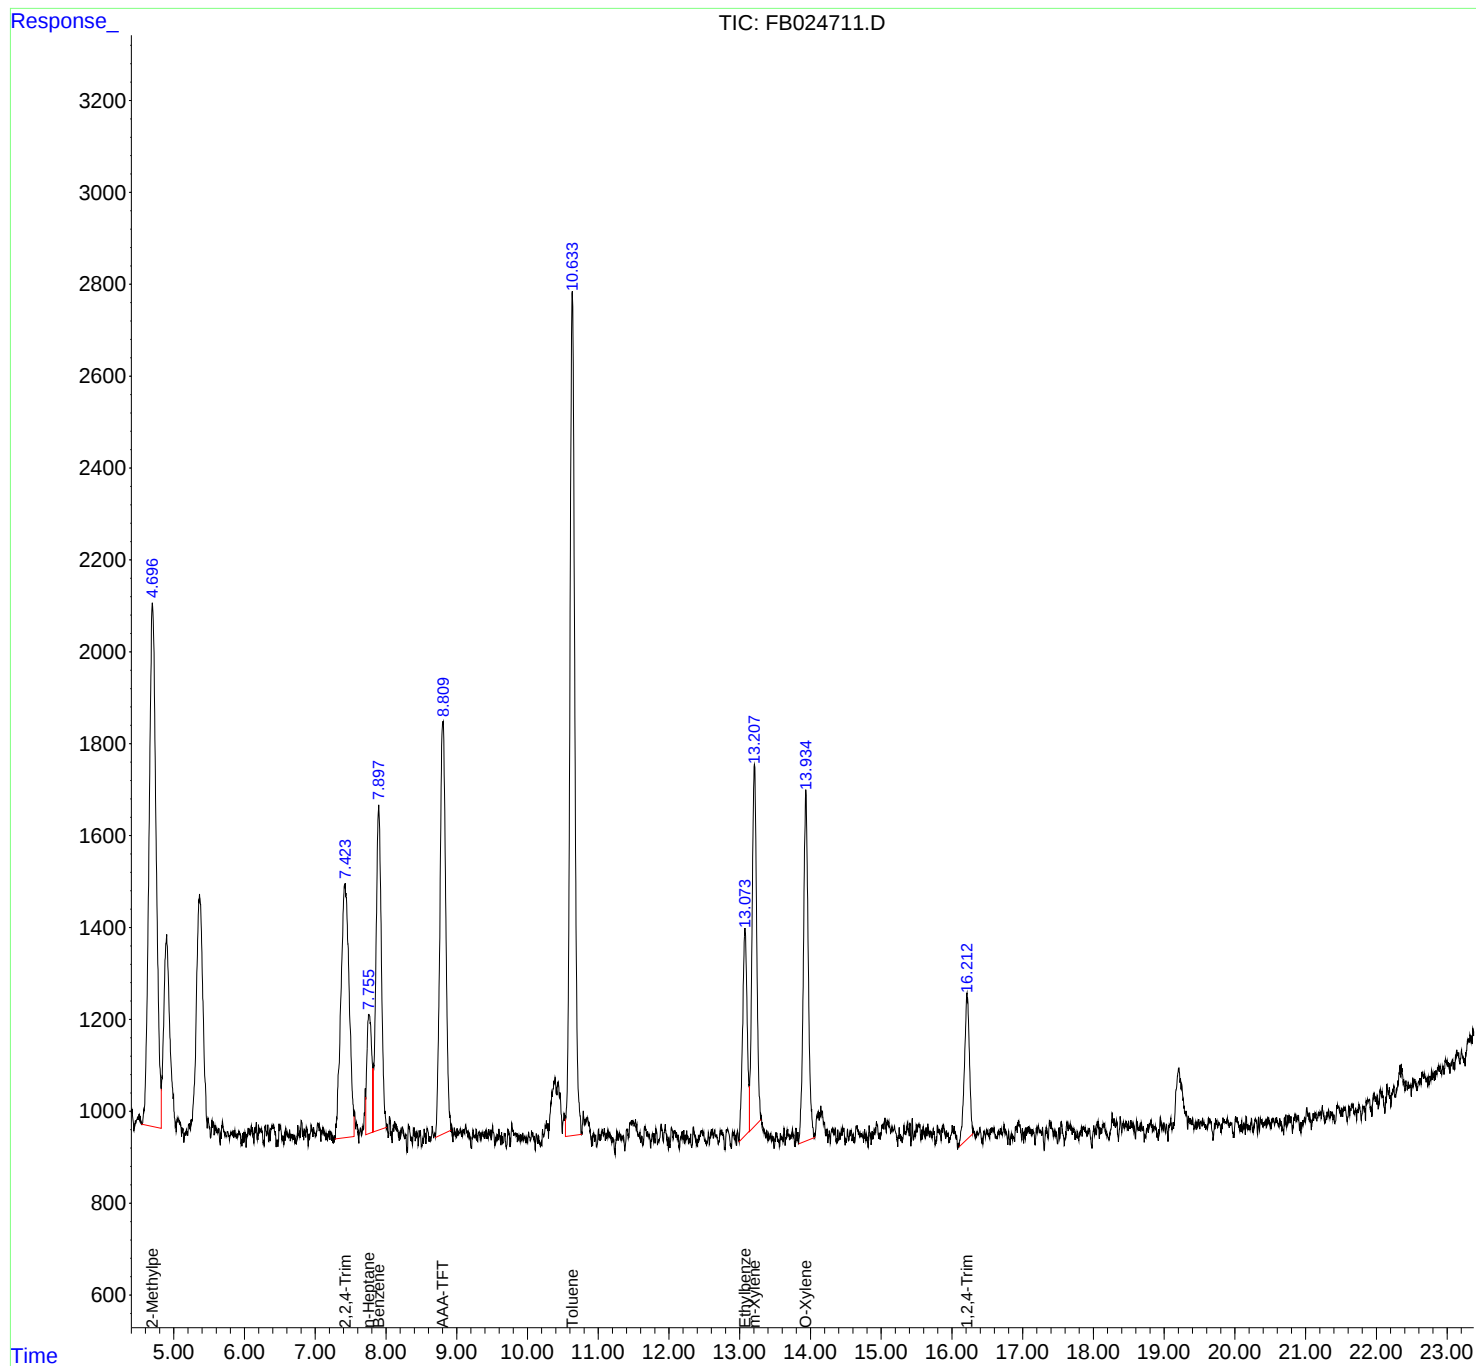

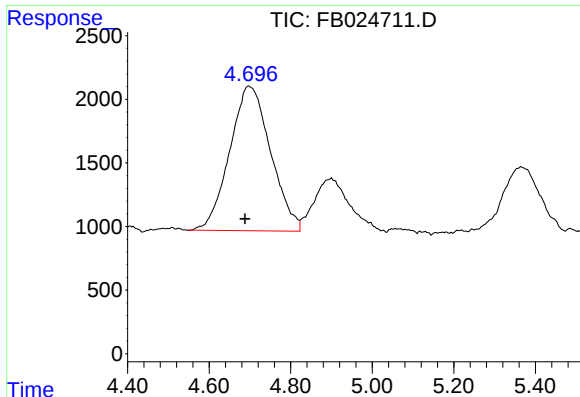


#1 2-Methylpentane

R.T.: 4.697 min
Delta R.T.: 0.009 min
Response: 79289
Conc: 2.68 ng/ml

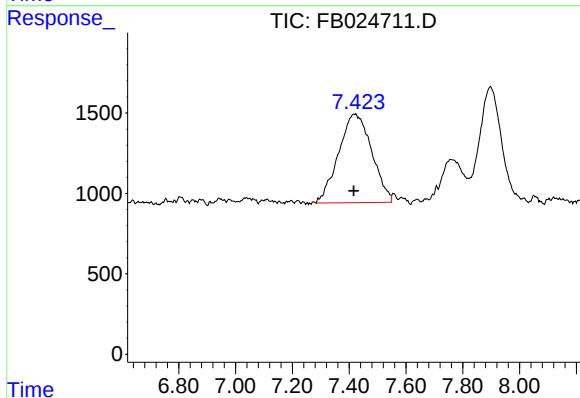


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.008 min
Response: 44708
Conc: 1.43 ng/ml

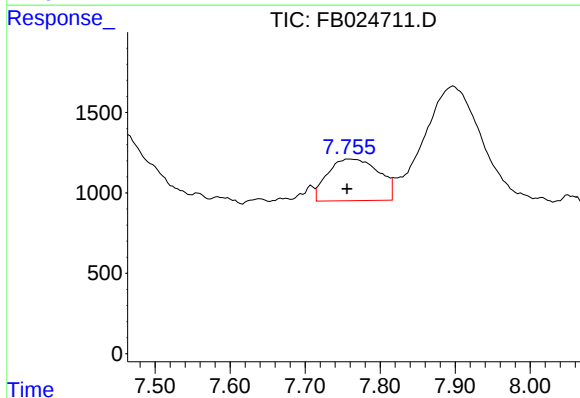


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.002 min
Response: 12194
Conc: 0.39 ng/ml

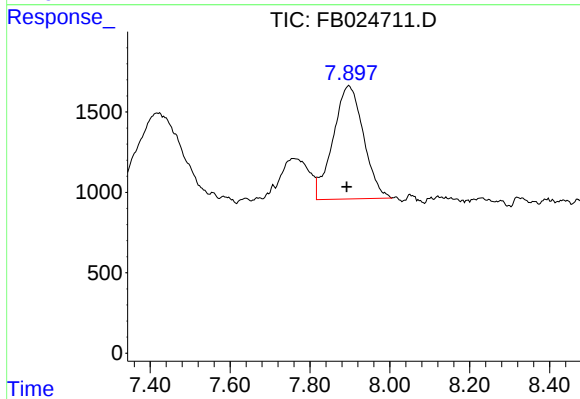


#4 Benzene

R.T.: 7.898 min
Delta R.T.: 0.006 min
Response: 37286
Conc: 0.98 ng/ml

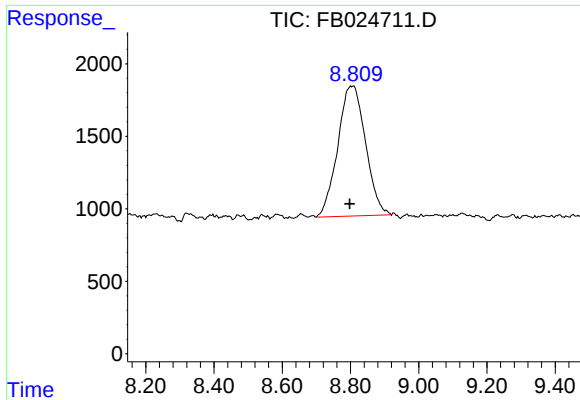


#5 AAA-TFT

R.T.: 8.810 min
Delta R.T.: 0.012 min
Response: 50507
Conc: 2.19 ng/ml

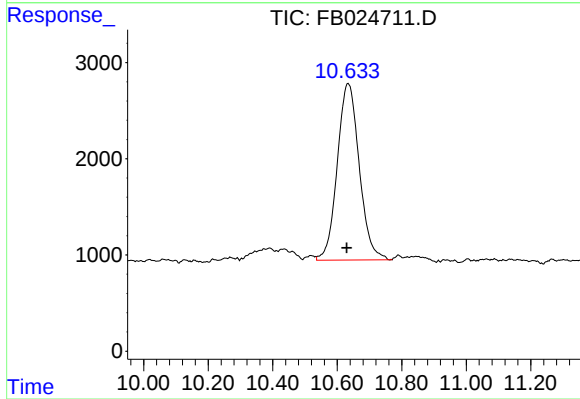


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.005 min
Response: 86846
Conc: 2.38 ng/ml

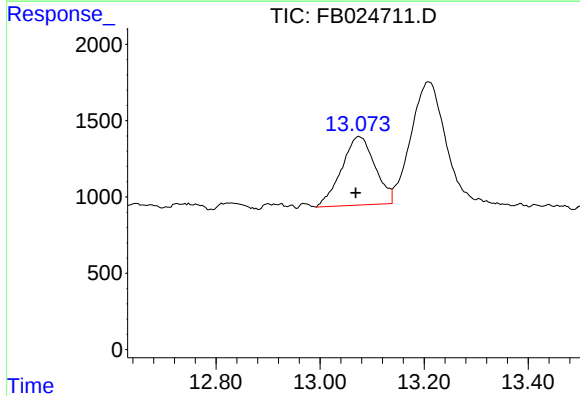


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: 0.006 min
Response: 19993
Conc: 0.59 ng/ml

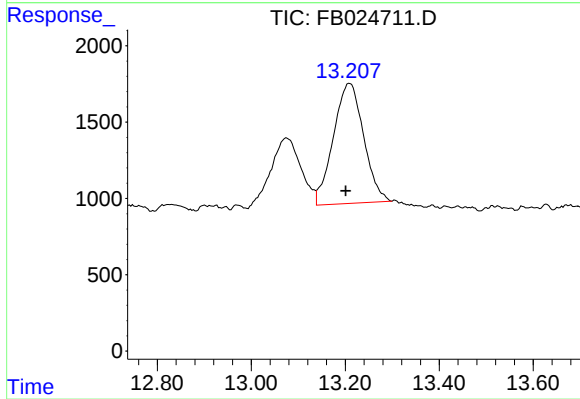


#8 m-Xylene

R.T.: 13.209 min
Delta R.T.: 0.008 min
Response: 35257
Conc: 1.04 ng/ml

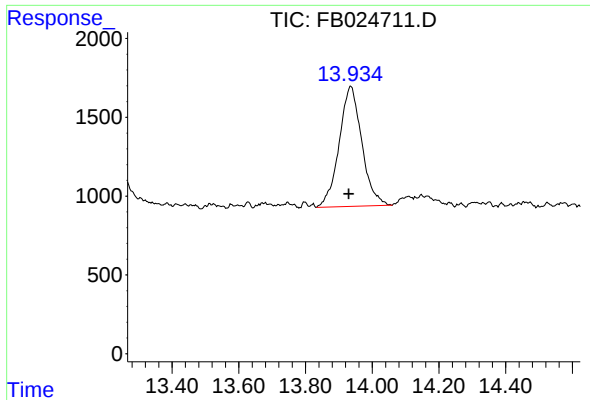

#9 O-Xylene

R.T.: 13.936 min
Delta R.T.: 0.007 min
Response: 35825
Conc: 1.09 ng/ml

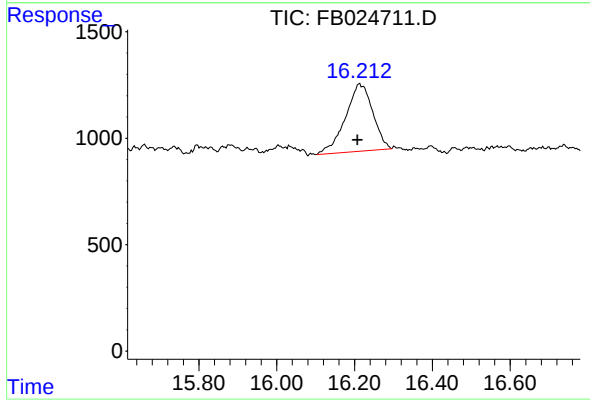

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.006 min
Response: 15361
Conc: 0.57 ng/ml