

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
 Data File : FB027798.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2022 11:56
 Operator : AJ/MA
 Sample : BSF0803W2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 23:33:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.795	194312	16.696 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.719	565946	26.873 ng/ml
2) t	2,2,4-Trimethylpentane	7.433	656672	31.644 ng/ml
3) t	n-Heptane	7.753	175155	8.520 ng/ml
4) t	Benzene	7.889	223535	9.526 ng/ml
6) t	Toluene	10.623	642940	28.793 ng/ml
7) t	Ethylbenzene	13.060	212091	10.122 ng/ml
8) t	m-Xylene	13.193	432340	20.649 ng/ml
9) t	O-Xylene	13.920	432609	21.142 ng/ml
10) t	1,2,4-Trimethylbenzene	16.195	471909	22.708 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
Data File : FB027798.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2022 11:56
Operator : AJ/MA
Sample : BSF0803W2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 23:33:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

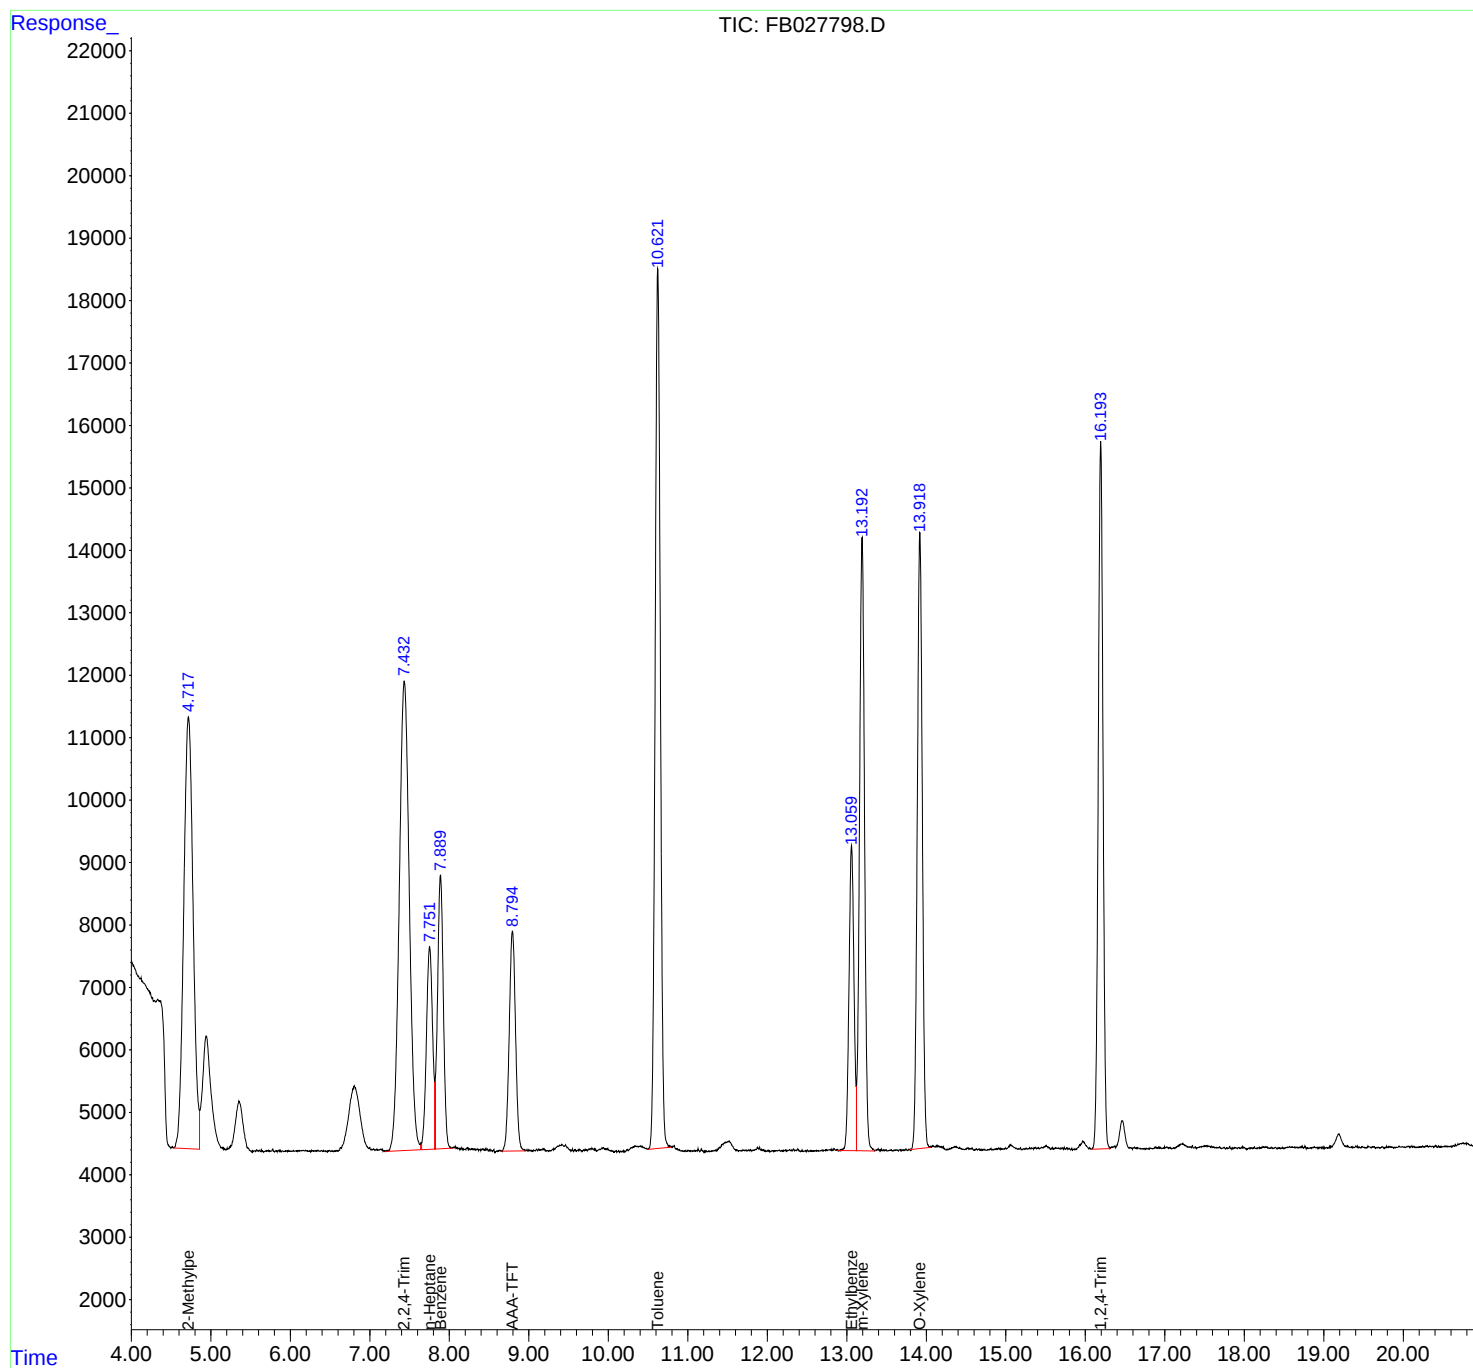

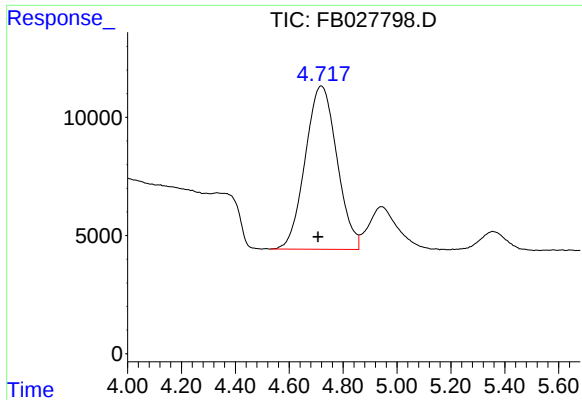


#1 2-Methylpentane

R.T.: 4.719 min
Delta R.T.: 0.012 min
Response: 565946
Conc: 26.87 ng/ml

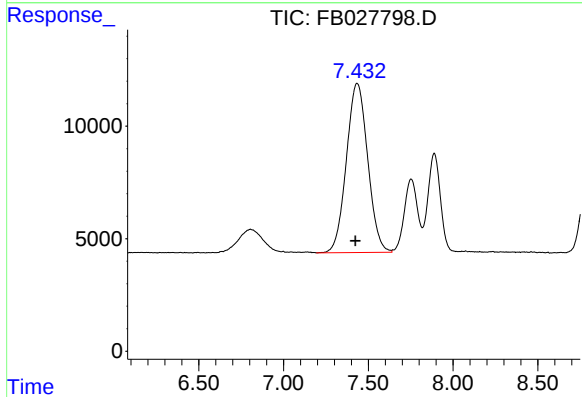


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.009 min
Response: 656672
Conc: 31.64 ng/ml

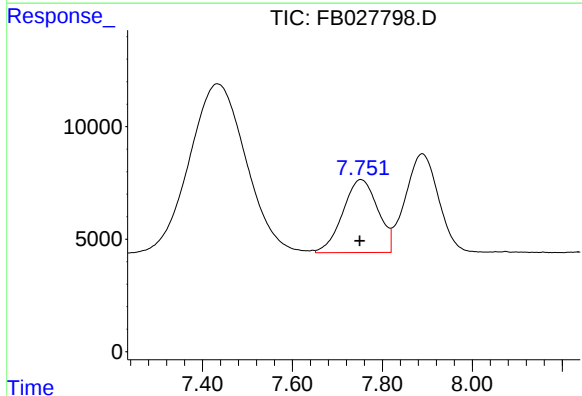


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 175155
Conc: 8.52 ng/ml

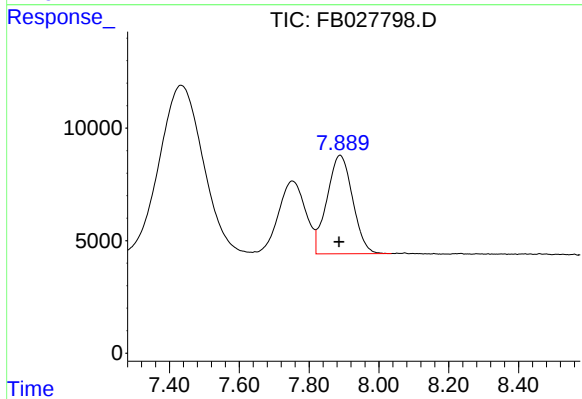


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 223535
Conc: 9.53 ng/ml

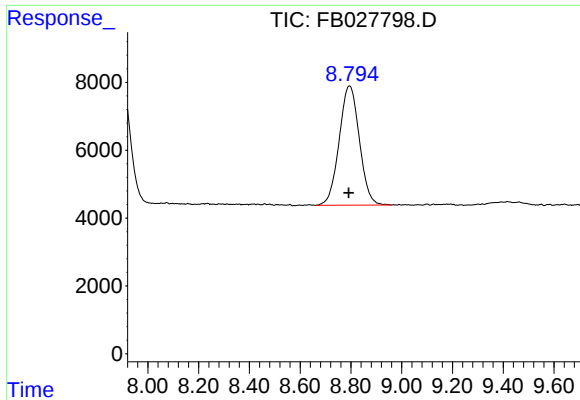


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 194312
Conc: 16.70 ng/ml

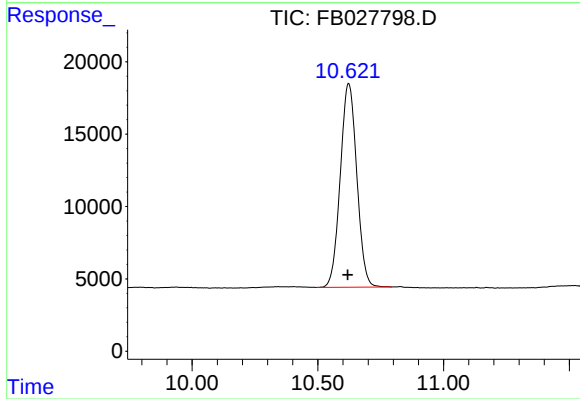


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 642940
Conc: 28.79 ng/ml

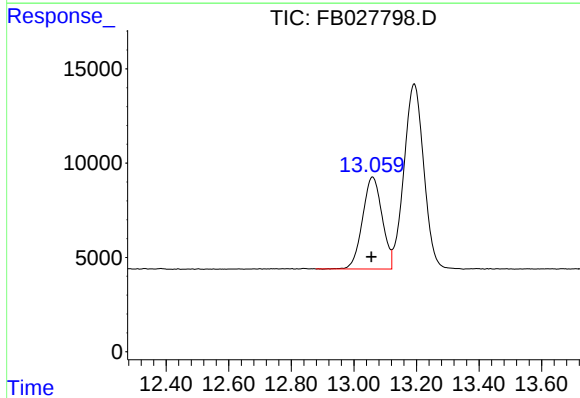


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 212091
Conc: 10.12 ng/ml

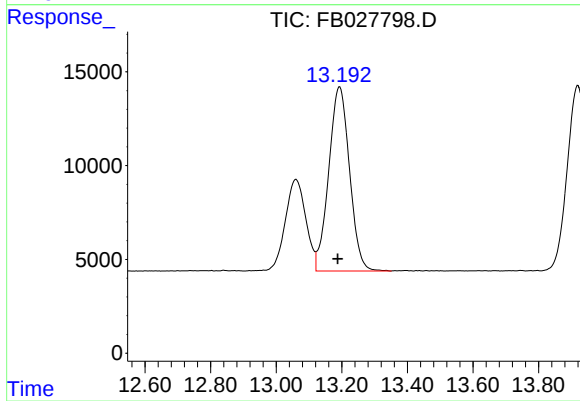

#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.005 min
Response: 432340
Conc: 20.65 ng/ml

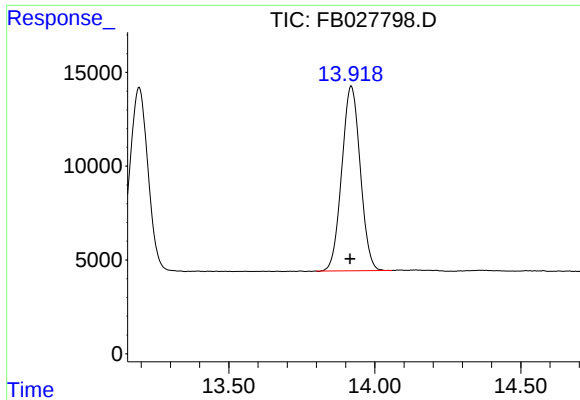


#9 O-Xylene

R.T.: 13.920 min

Delta R.T.: 0.004 min

Response: 432609

Conc: 21.14 ng/ml

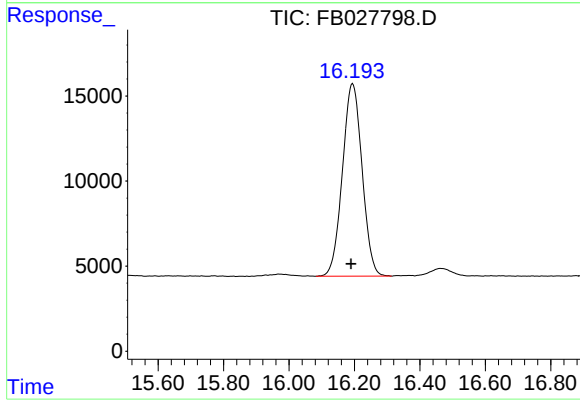

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min

Delta R.T.: 0.004 min

Response: 471909

Conc: 22.71 ng/ml