

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
 Data File : FB027808.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2022 18:17
 Operator : AJ/MA
 Sample : N4017-10MS
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 23:35:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	240244	20.642 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	636912	30.243 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	674393	32.498 ng/ml
3) t n-Heptane	7.756	223554	10.874 ng/ml
4) t Benzene	7.893	254955	10.864 ng/ml
6) t Toluene	10.626	734482	32.892 ng/ml
7) t Ethylbenzene	13.063	231419	11.044 ng/ml
8) t m-Xylene	13.196	459675	21.954 ng/ml
9) t O-Xylene	13.923	443688	21.683 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	434531	20.909 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
Data File : FB027808.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2022 18:17
Operator : AJ/MA
Sample : N4017-10MS
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 23:35:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

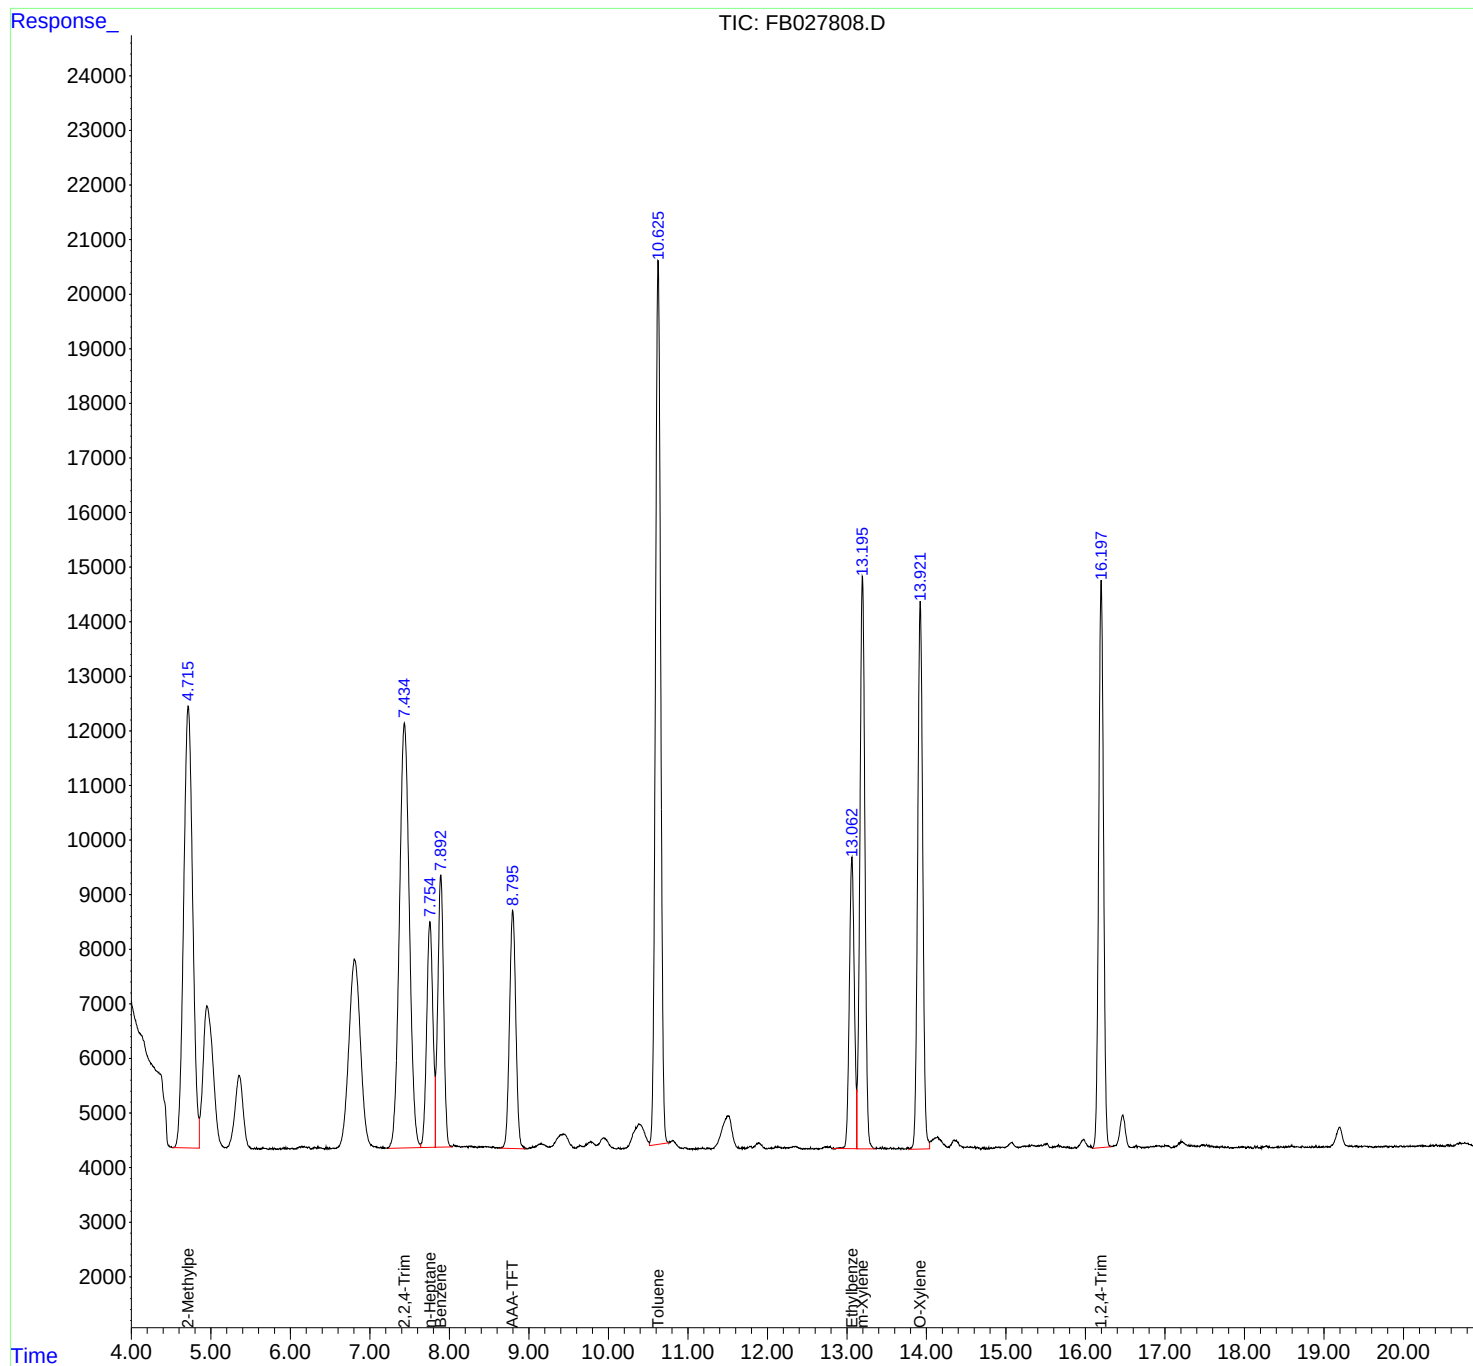

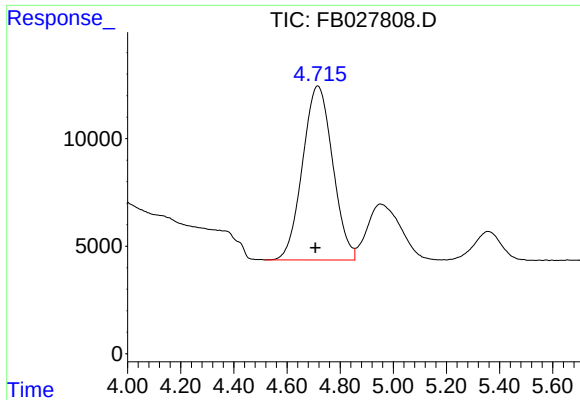


#1 2-Methylpentane

R.T.: 4.716 min
Delta R.T.: 0.009 min
Response: 636912
Conc: 30.24 ng/ml

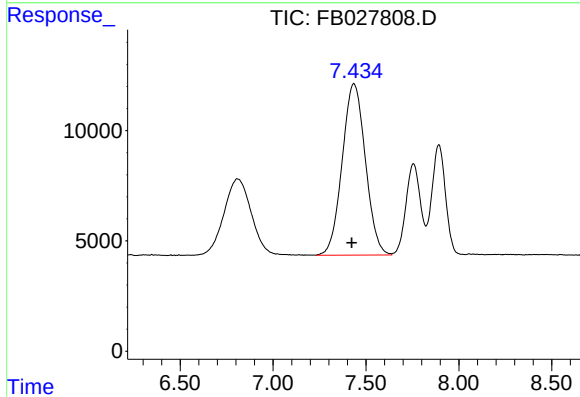


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.011 min
Response: 674393
Conc: 32.50 ng/ml

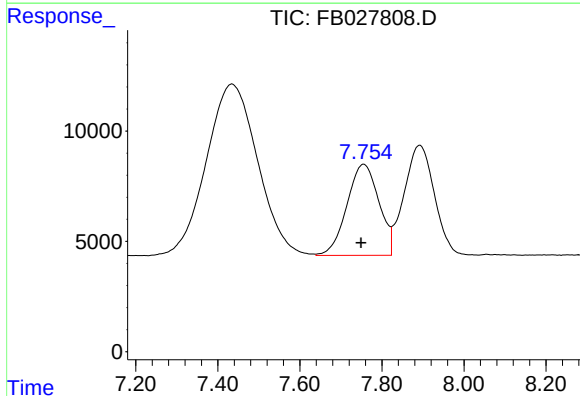


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 223554
Conc: 10.87 ng/ml

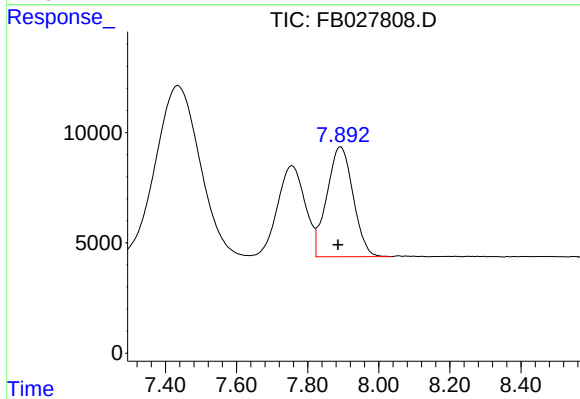


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.007 min
Response: 254955
Conc: 10.86 ng/ml

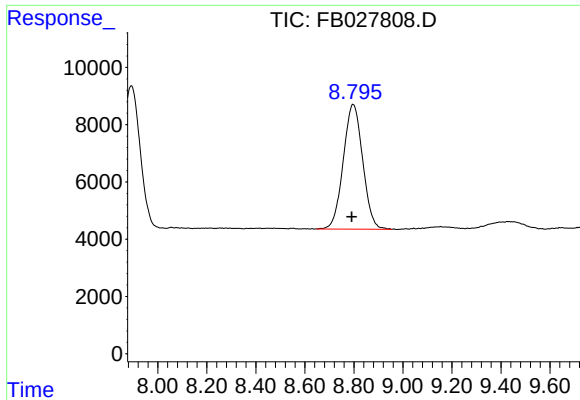


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 240244
Conc: 20.64 ng/ml

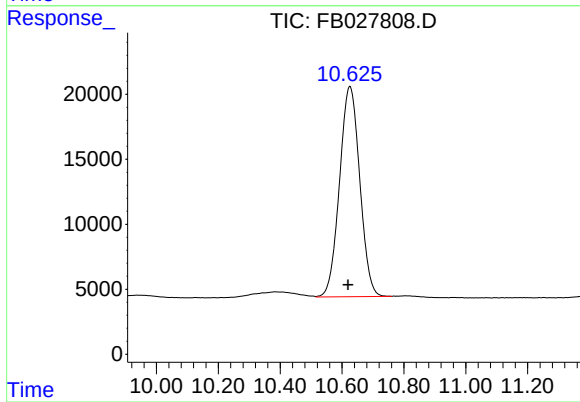


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.007 min
Response: 734482
Conc: 32.89 ng/ml

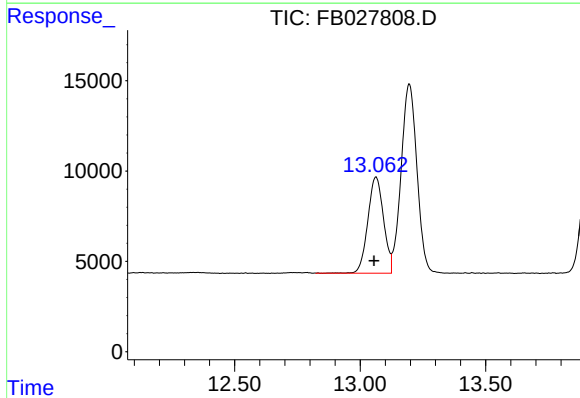


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.007 min
Response: 231419
Conc: 11.04 ng/ml

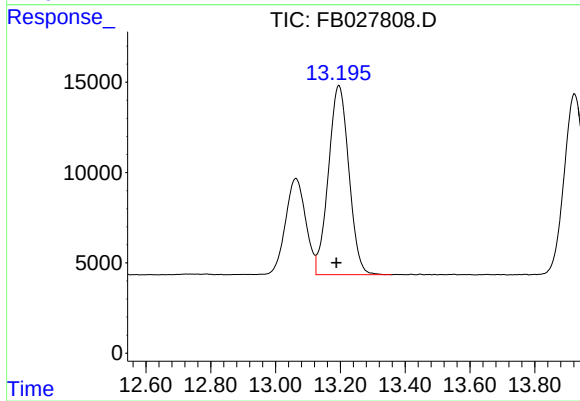


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: 0.008 min
Response: 459675
Conc: 21.95 ng/ml

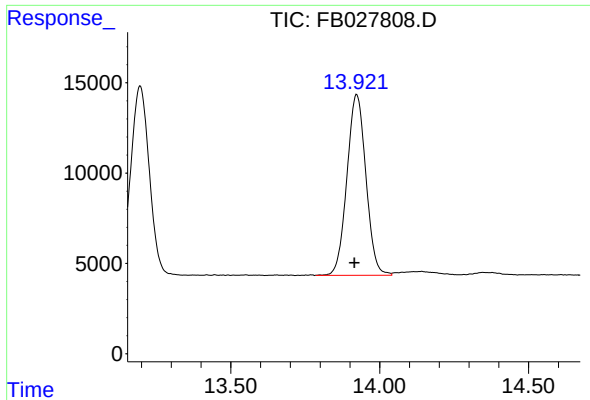

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.008 min
Response: 443688
Conc: 21.68 ng/ml

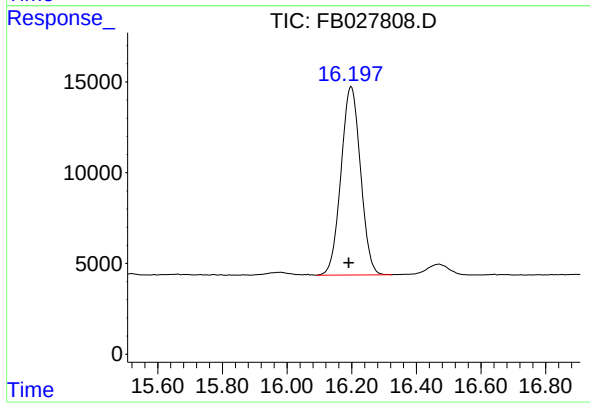

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.008 min
Response: 434531
Conc: 20.91 ng/ml