

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
 Data File : FB027799.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2022 12:34
 Operator : AJ/MA
 Sample : N3980-09
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 23:33:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	181990	15.637 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.729	22902	1.087 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	19937	0.961 ng/mlm
3) t n-Heptane	7.756	4468	0.217 ng/ml
4) t Benzene	7.888	5744	0.245 ng/ml
6) t Toluene	10.627	19462	0.872 ng/ml
7) t Ethylbenzene	13.063	7678	0.366 ng/ml
8) t m-Xylene	13.197	14964	0.715 ng/ml
9) t O-Xylene	13.924	16302	0.797 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	17870	0.860 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
Data File : FB027799.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2022 12:34
Operator : AJ/MA
Sample : N3980-09
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 23:33:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

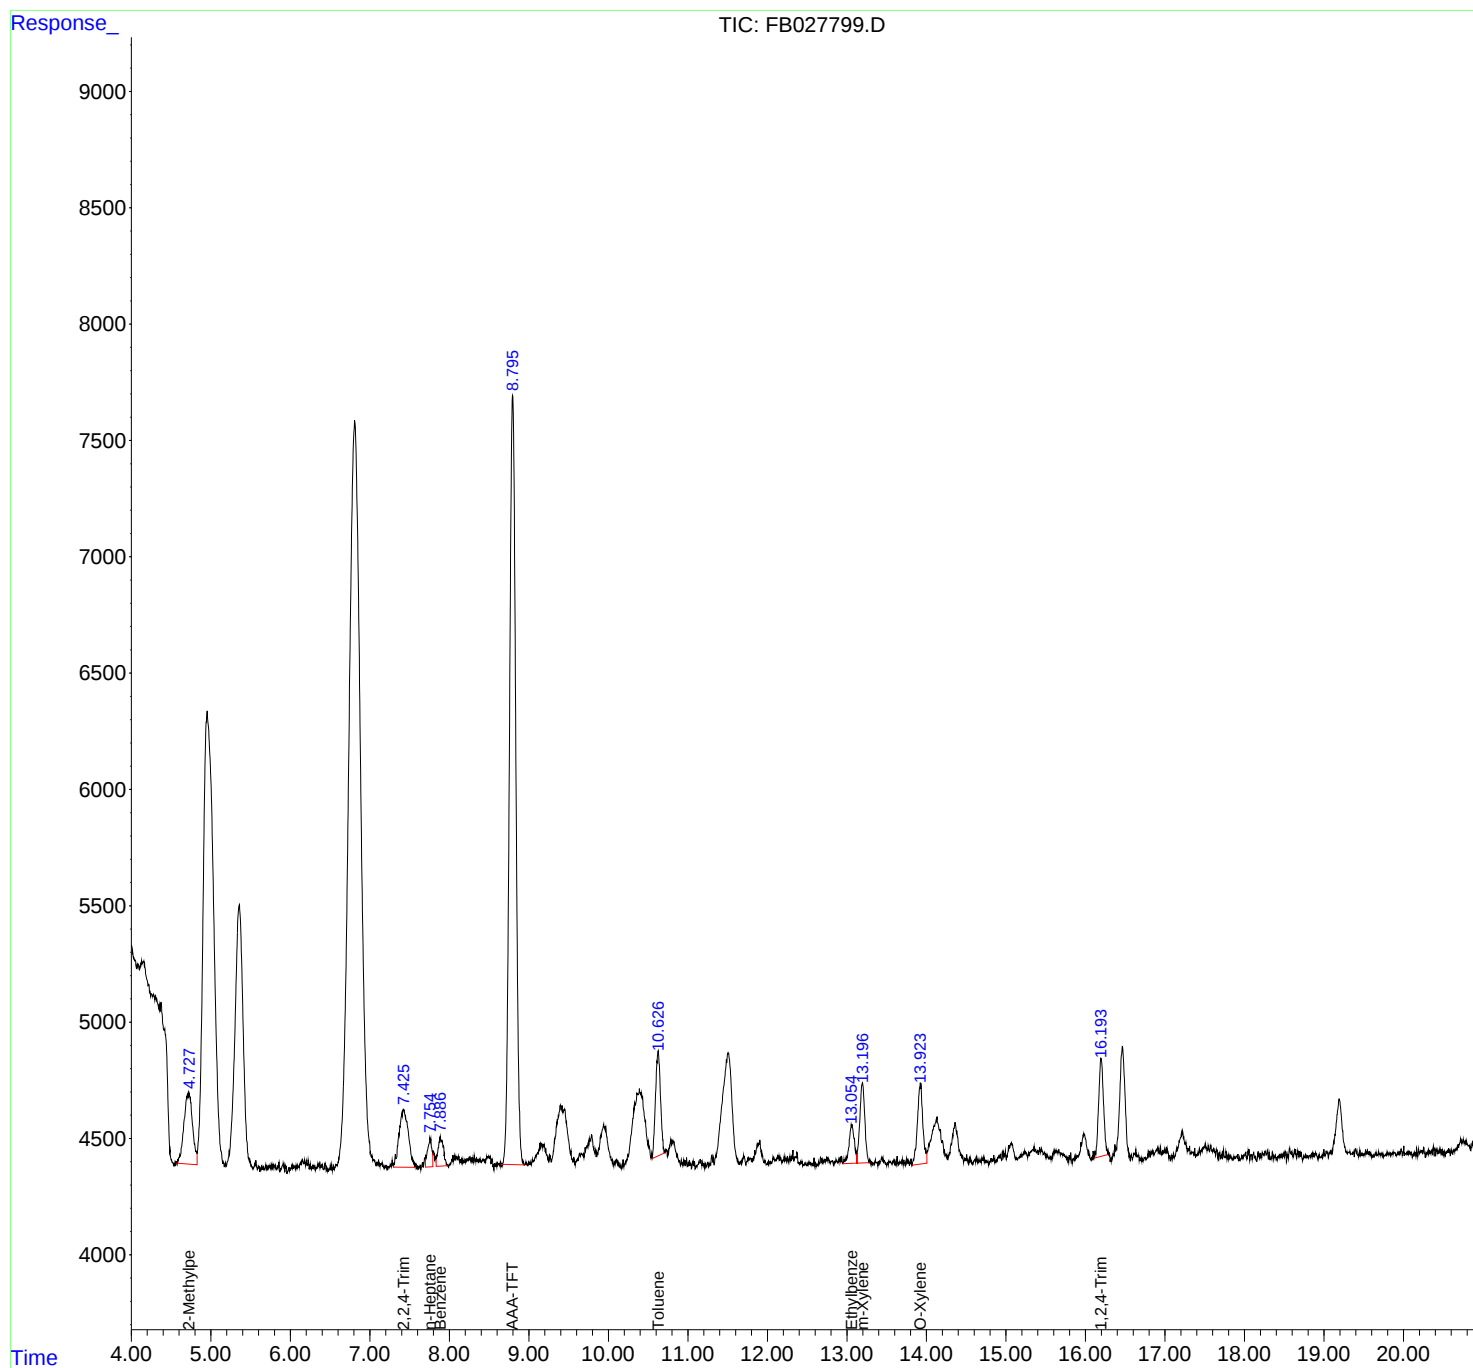

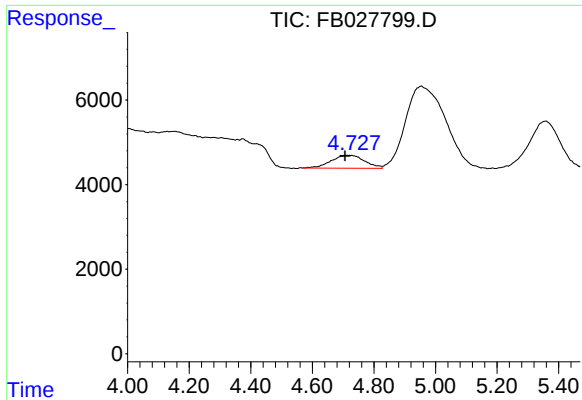


#1 2-Methylpentane

R.T.: 4.729 min
Delta R.T.: 0.022 min
Response: 22902
Conc: 1.09 ng/ml

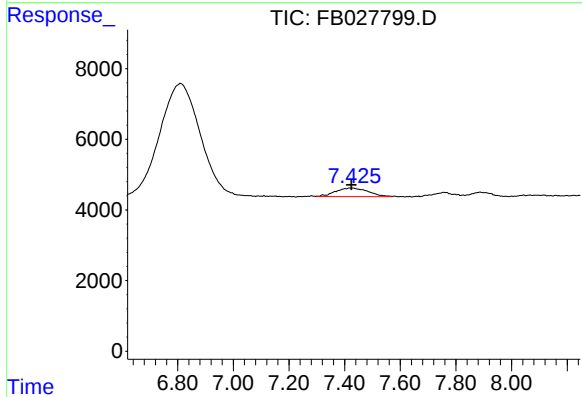


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 19937
Conc: 0.96 ng/ml m

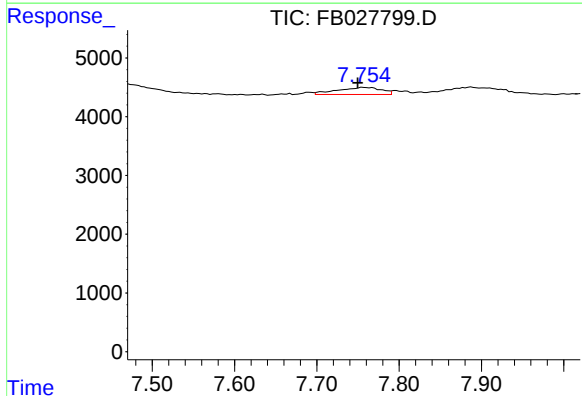


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 4468
Conc: 0.22 ng/ml

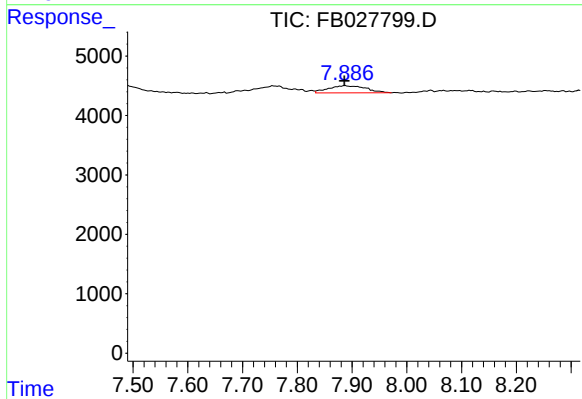


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 5744
Conc: 0.24 ng/ml

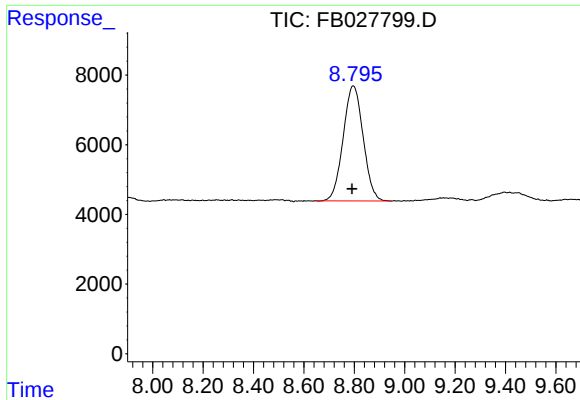


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 181990
Conc: 15.64 ng/ml

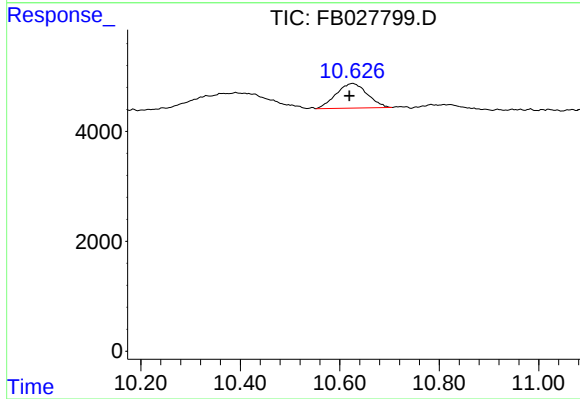


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.008 min
Response: 19462
Conc: 0.87 ng/ml

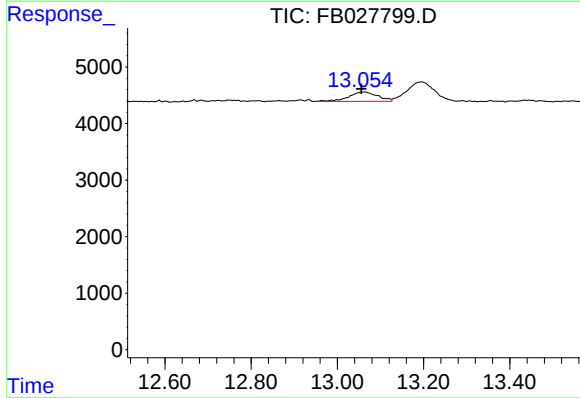


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.008 min
Response: 7678
Conc: 0.37 ng/ml

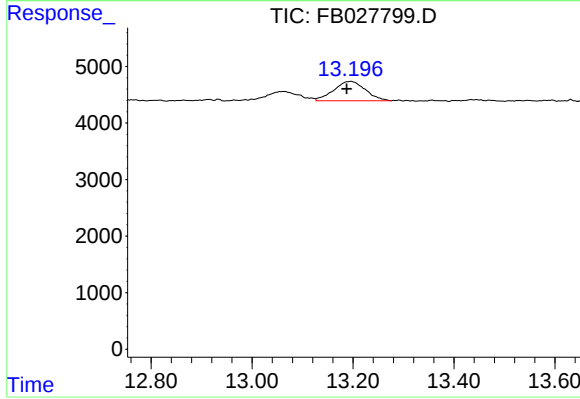


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: 0.009 min
Response: 14964
Conc: 0.71 ng/ml

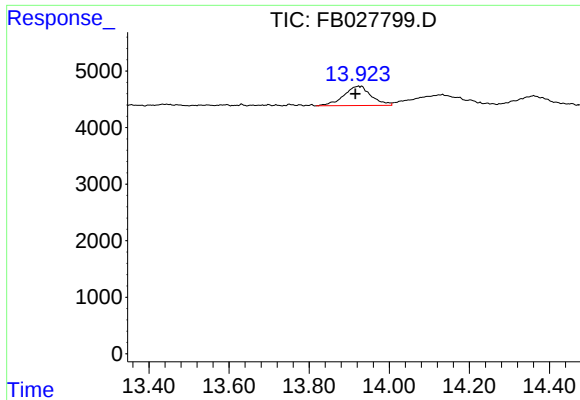

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.009 min
Response: 16302
Conc: 0.80 ng/ml

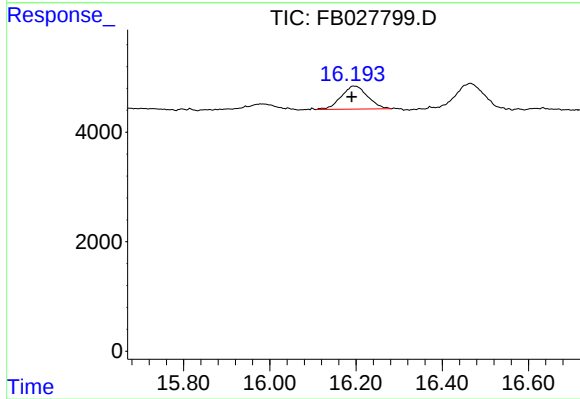

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.005 min
Response: 17870
Conc: 0.86 ng/ml