

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
 Data File : FB027804.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2022 15:48
 Operator : AJ/MA
 Sample : N3980-03
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 23:34:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	212172	18.230 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	20108	0.955 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	18665	0.899 ng/mlm
3) t n-Heptane	7.749	4167	0.203 ng/ml
4) t Benzene	7.886	4505	0.192 ng/mlm
6) t Toluene	10.627	20494	0.918 ng/ml
7) t Ethylbenzene	13.061	6434	0.307 ng/ml
8) t m-Xylene	13.195	13330	0.637 ng/ml
9) t O-Xylene	13.931	11213	0.548 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	16752	0.806 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
Data File : FB027804.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2022 15:48
Operator : AJ/MA
Sample : N3980-03
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 23:34:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

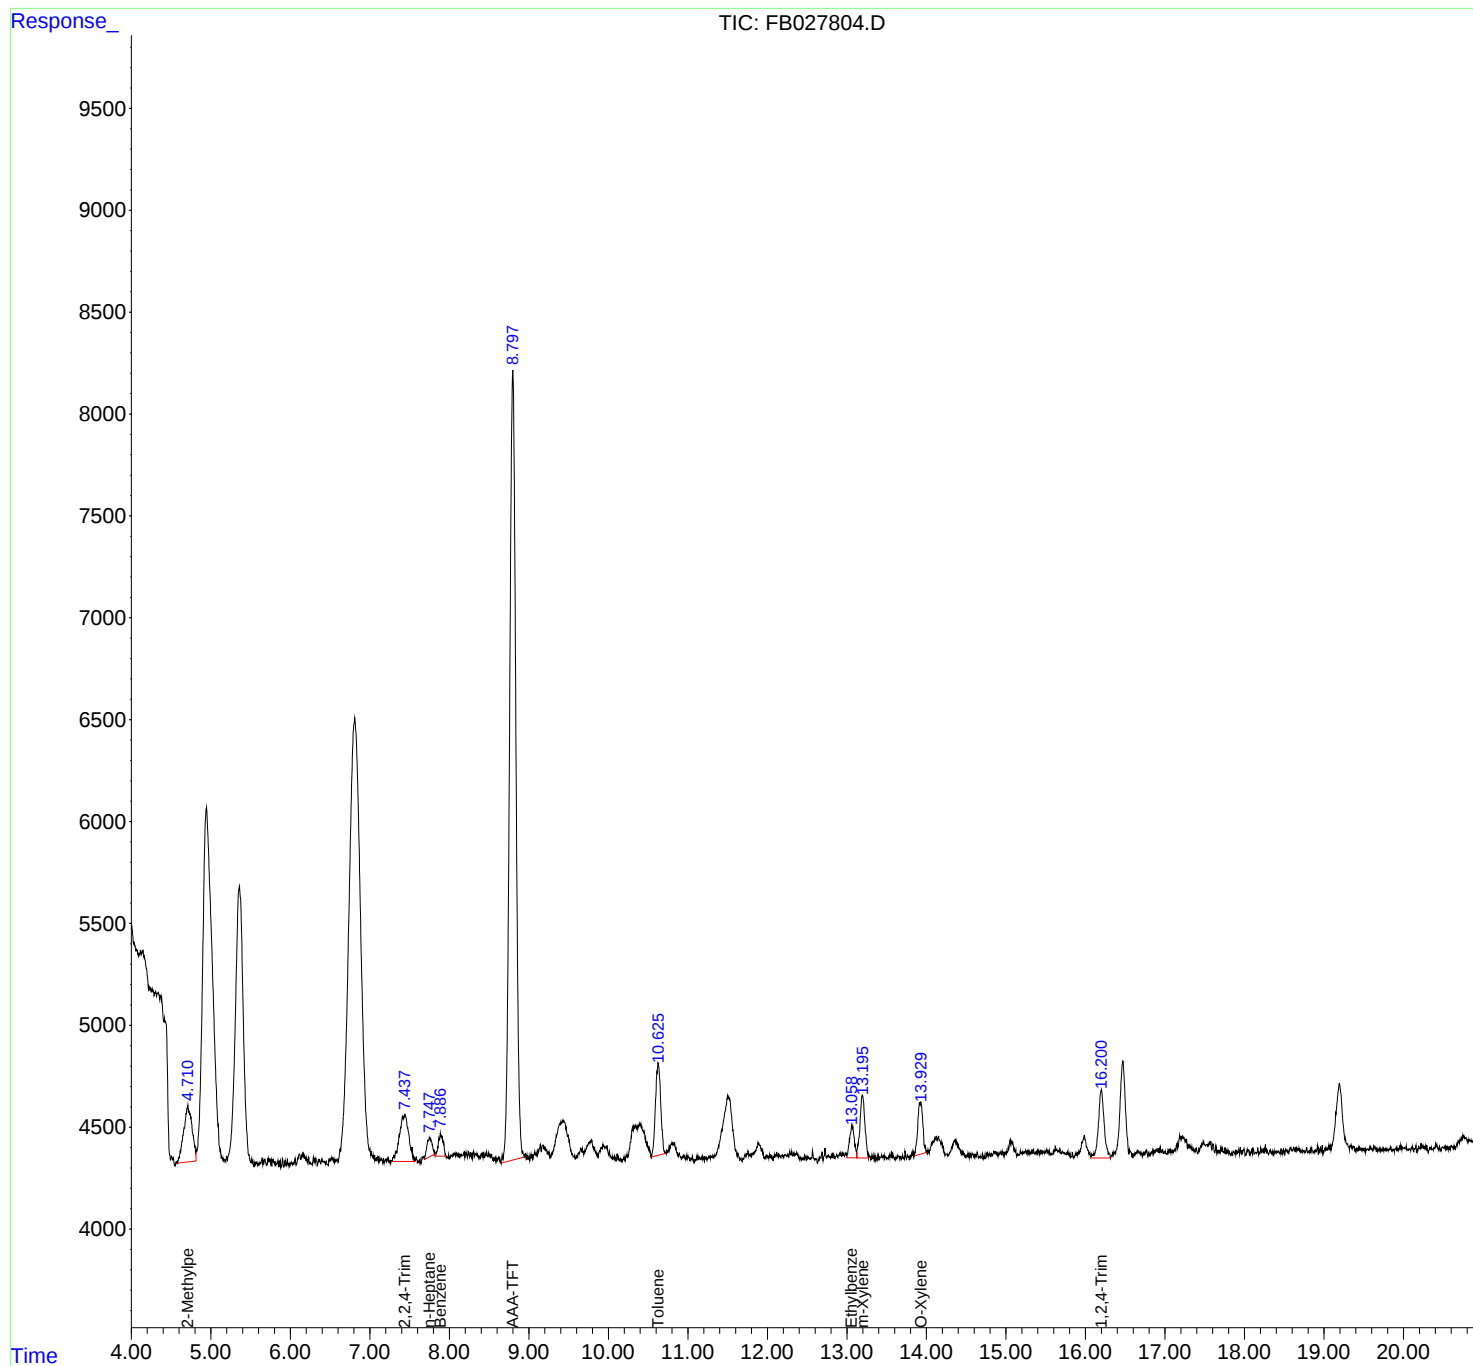

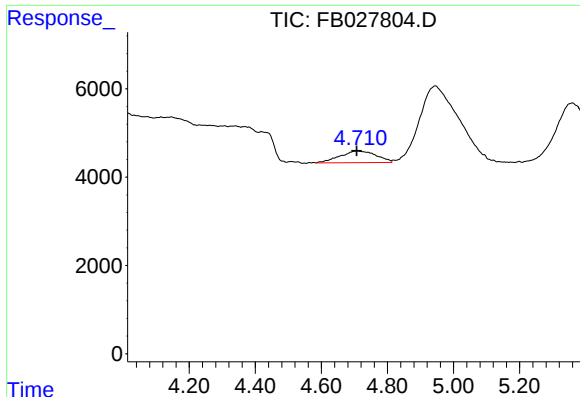


#1 2-Methylpentane

R.T.: 4.711 min
Delta R.T.: 0.004 min
Response: 20108
Conc: 0.95 ng/ml

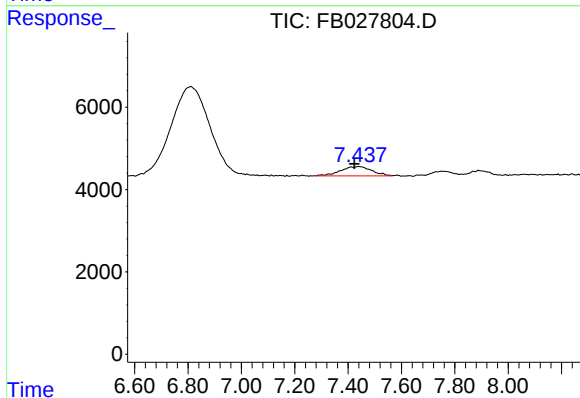


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.012 min
Response: 18665
Conc: 0.90 ng/ml m

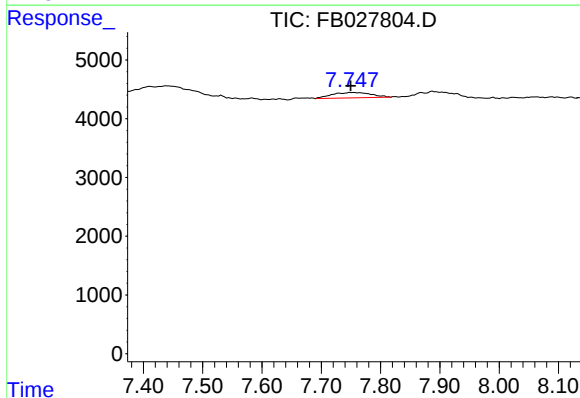


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 4167
Conc: 0.20 ng/ml

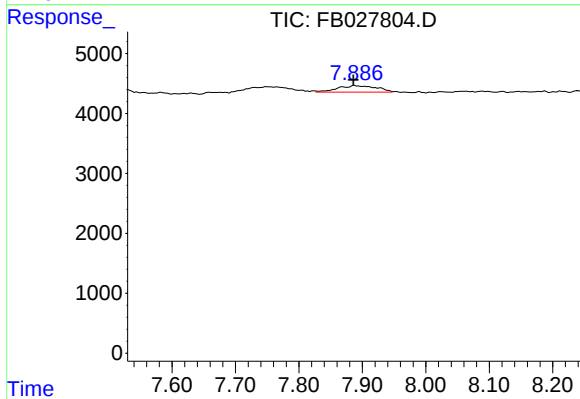


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 4505
Conc: 0.19 ng/ml m

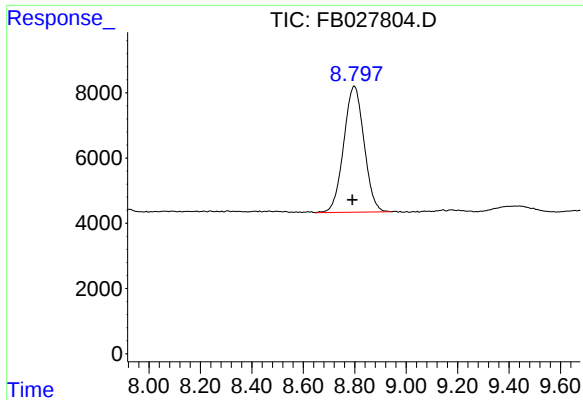


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.008 min
Response: 212172
Conc: 18.23 ng/ml

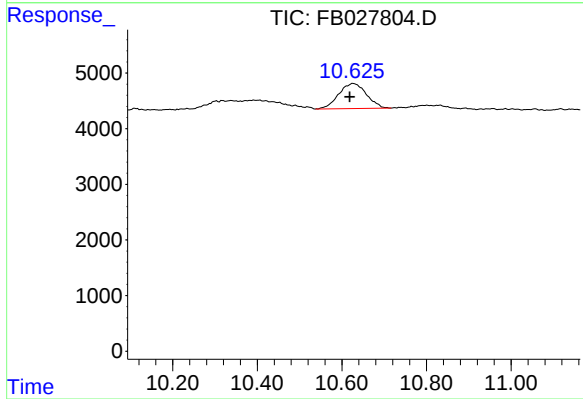


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.008 min
Response: 20494
Conc: 0.92 ng/ml

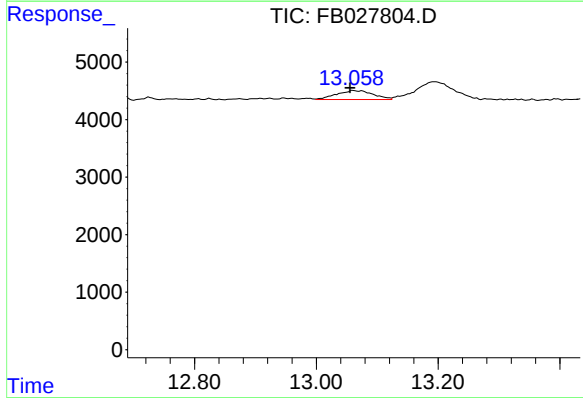


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.005 min
Response: 6434
Conc: 0.31 ng/ml

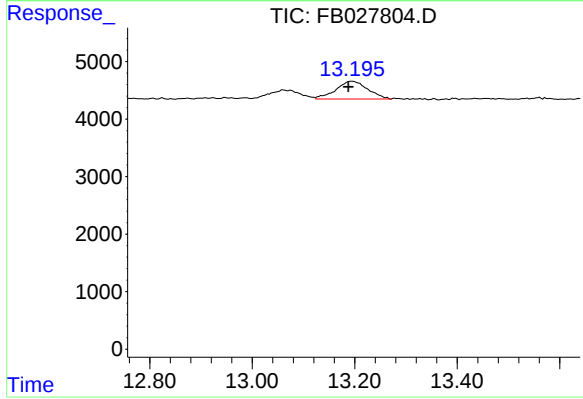


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: 0.007 min
Response: 13330
Conc: 0.64 ng/ml

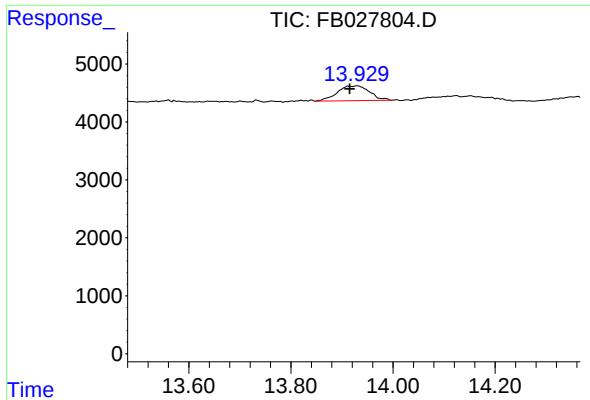

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.015 min
Response: 11213
Conc: 0.55 ng/ml

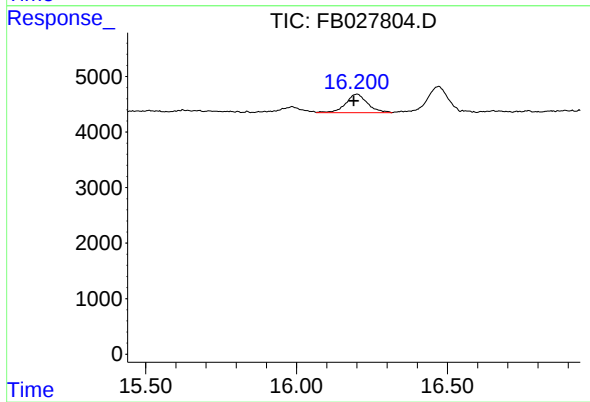

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.011 min
Response: 16752
Conc: 0.81 ng/ml