

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
 Data File : FB027809.D
 Signal(s) : FID2B.CH
 Acq On : 3 Aug 2022 18:54
 Operator : AJ/MA
 Sample : N4017-10MSD
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 03 23:35:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	266989	22.940 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	600822	28.530 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	634926	30.596 ng/ml
3) t n-Heptane	7.756	207157	10.076 ng/ml
4) t Benzene	7.893	248250	10.579 ng/ml
6) t Toluene	10.626	700892	31.388 ng/ml
7) t Ethylbenzene	13.063	218679	10.436 ng/ml
8) t m-Xylene	13.196	435907	20.819 ng/ml
9) t O-Xylene	13.923	428397	20.936 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	415245	19.981 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080322\
Data File : FB027809.D
Signal(s) : FID2B.CH
Acq On : 3 Aug 2022 18:54
Operator : AJ/MA
Sample : N4017-10MSD
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 03 23:35:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

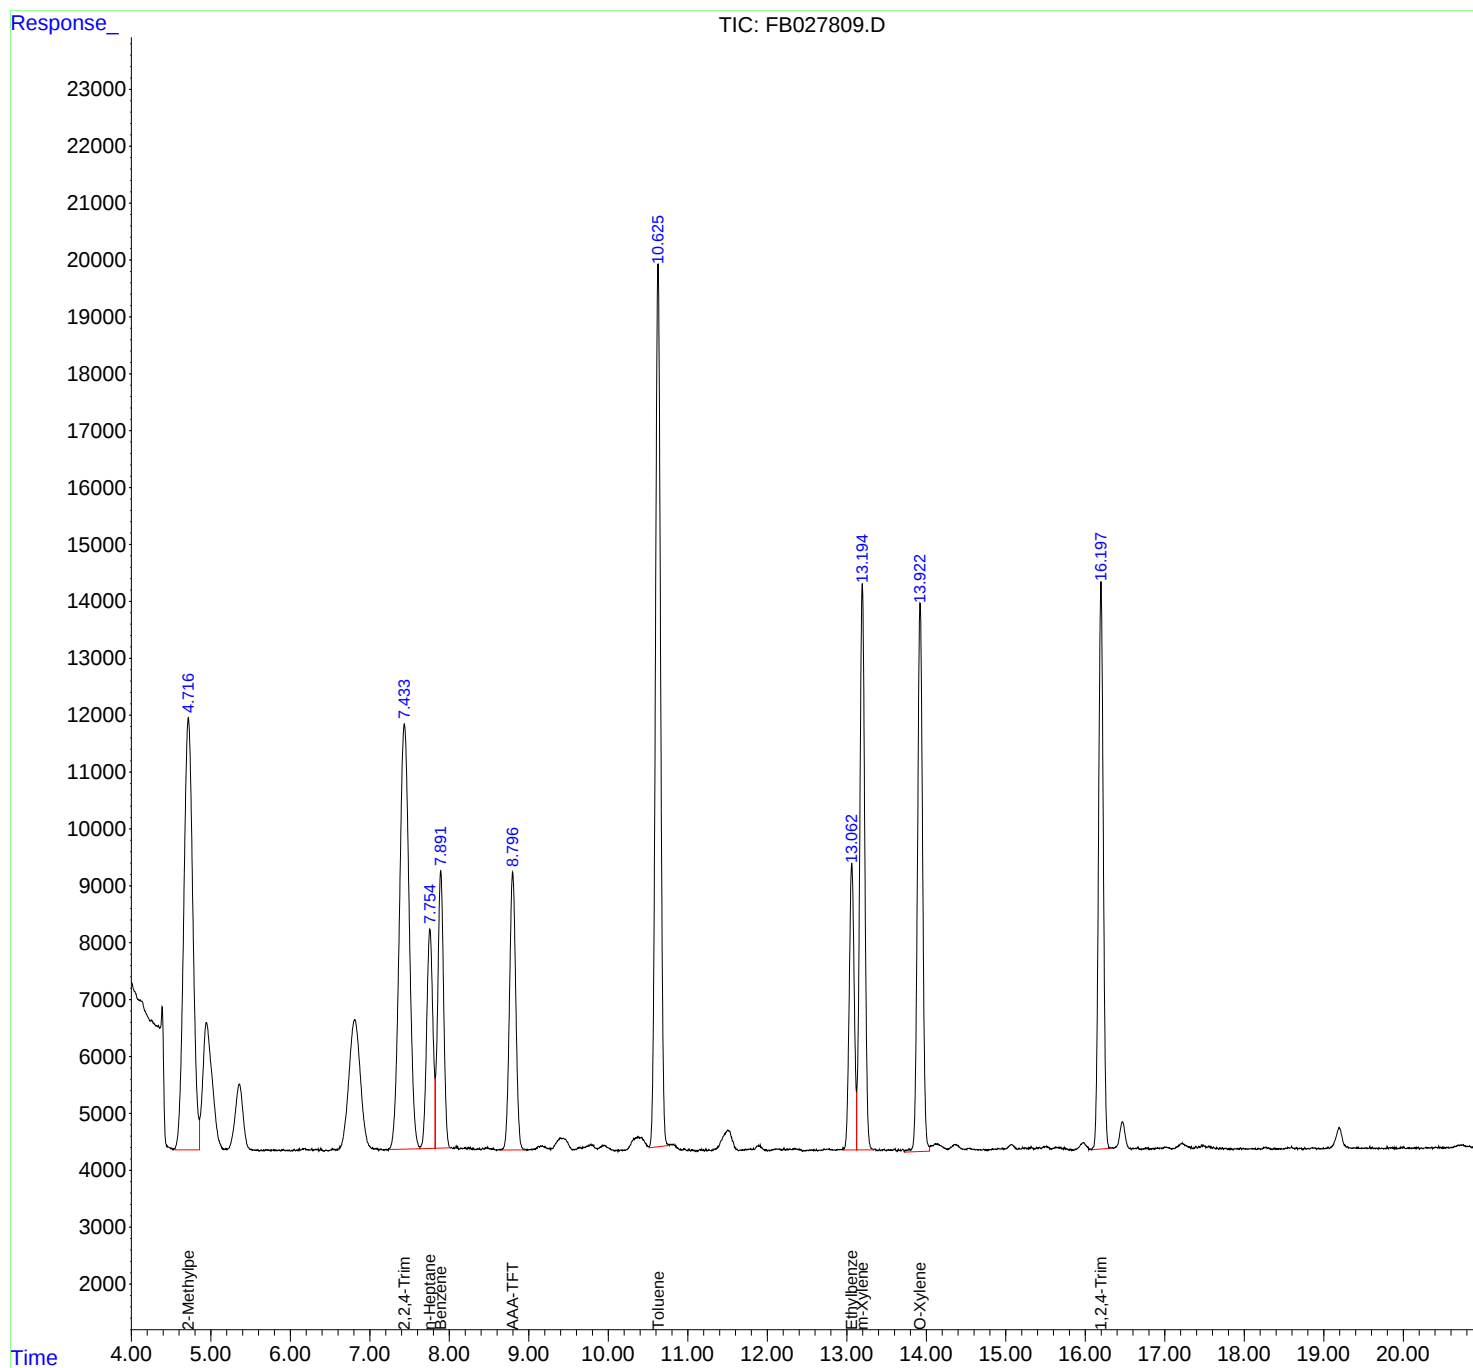

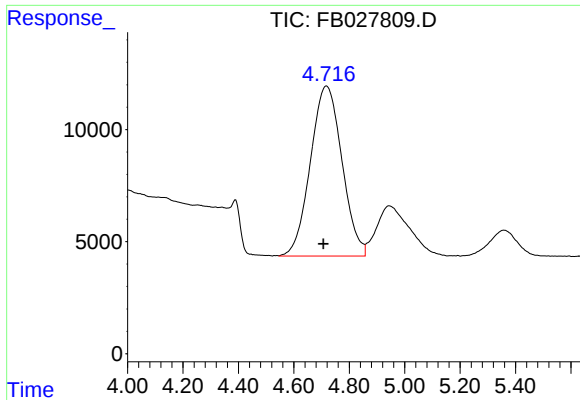


#1 2-Methylpentane

R.T.: 4.718 min
Delta R.T.: 0.011 min
Response: 600822
Conc: 28.53 ng/ml

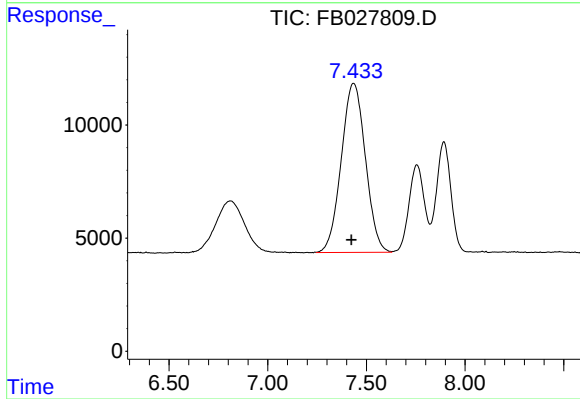


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.010 min
Response: 634926
Conc: 30.60 ng/ml

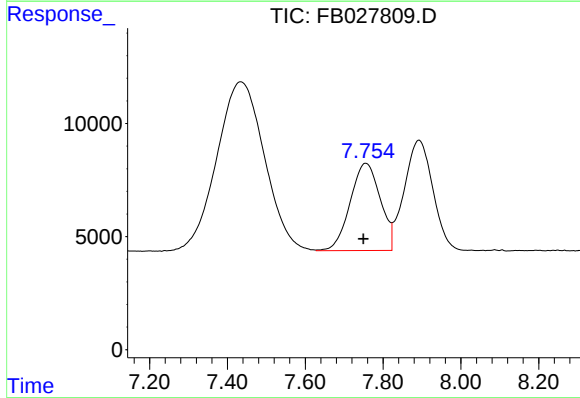


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 207157
Conc: 10.08 ng/ml

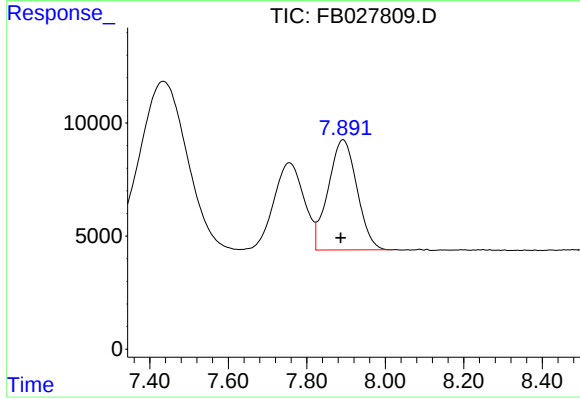


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.007 min
Response: 248250
Conc: 10.58 ng/ml

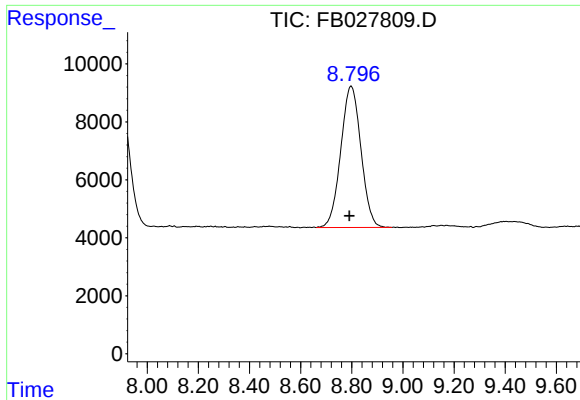


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 266989
Conc: 22.94 ng/ml

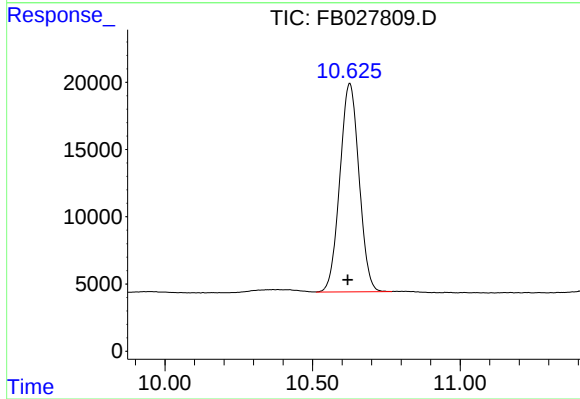


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.007 min
Response: 700892
Conc: 31.39 ng/ml

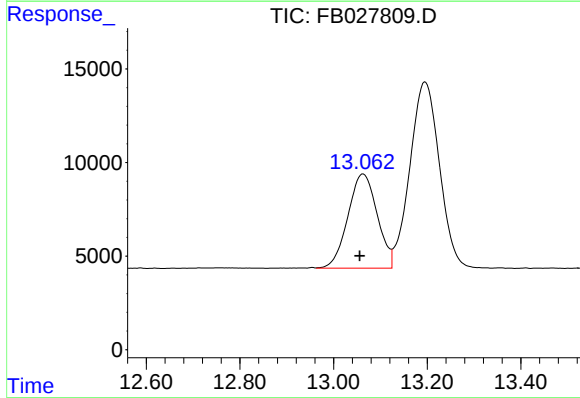


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.007 min
Response: 218679
Conc: 10.44 ng/ml

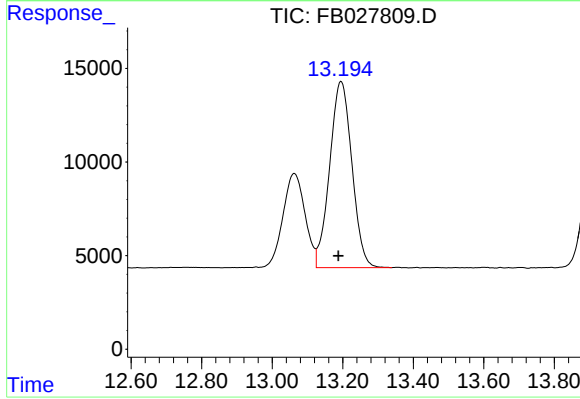

#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: 0.008 min
Response: 435907
Conc: 20.82 ng/ml

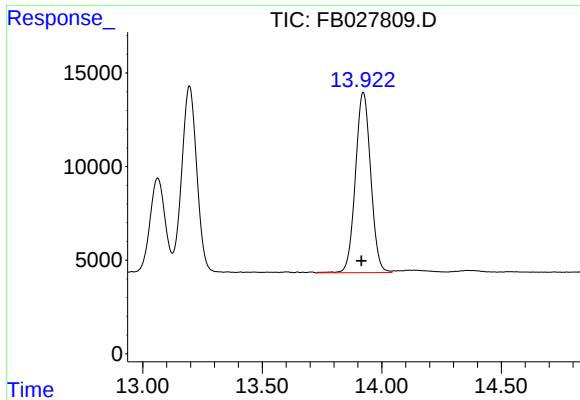


#9 O-Xylene

R.T.: 13.923 min

Delta R.T.: 0.008 min

Response: 428397

Conc: 20.94 ng/ml

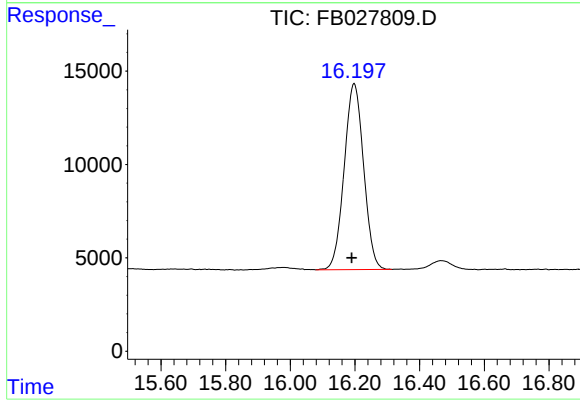

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min

Delta R.T.: 0.008 min

Response: 415245

Conc: 19.98 ng/ml