

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080519\
 Data File : FB021909.D
 Signal(s) : FID2B.CH
 Acq On : 5 Aug 2019 9:39
 Operator : DD/AJ
 Sample : BSF0805S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 00:56:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	262559	19.240 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	860240	31.195 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	831395	31.451 ng/ml
3) t n-Heptane	7.951	263081	10.610 ng/ml
4) t Benzene	8.087	292182	10.001 ng/ml
6) t Toluene	10.834	610239	29.657 ng/ml
7) t Ethylbenzene	13.280	205061	9.857 ng/ml
8) t m-Xylene	13.412	440876	19.846 ng/ml
9) t O-Xylene	14.141	455408	19.798 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	473768	20.095 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080519\
Data File : FB021909.D
Signal(s) : FID2B.CH
Acq On : 5 Aug 2019 9:39
Operator : DD/AJ
Sample : BSF0805S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 00:56:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

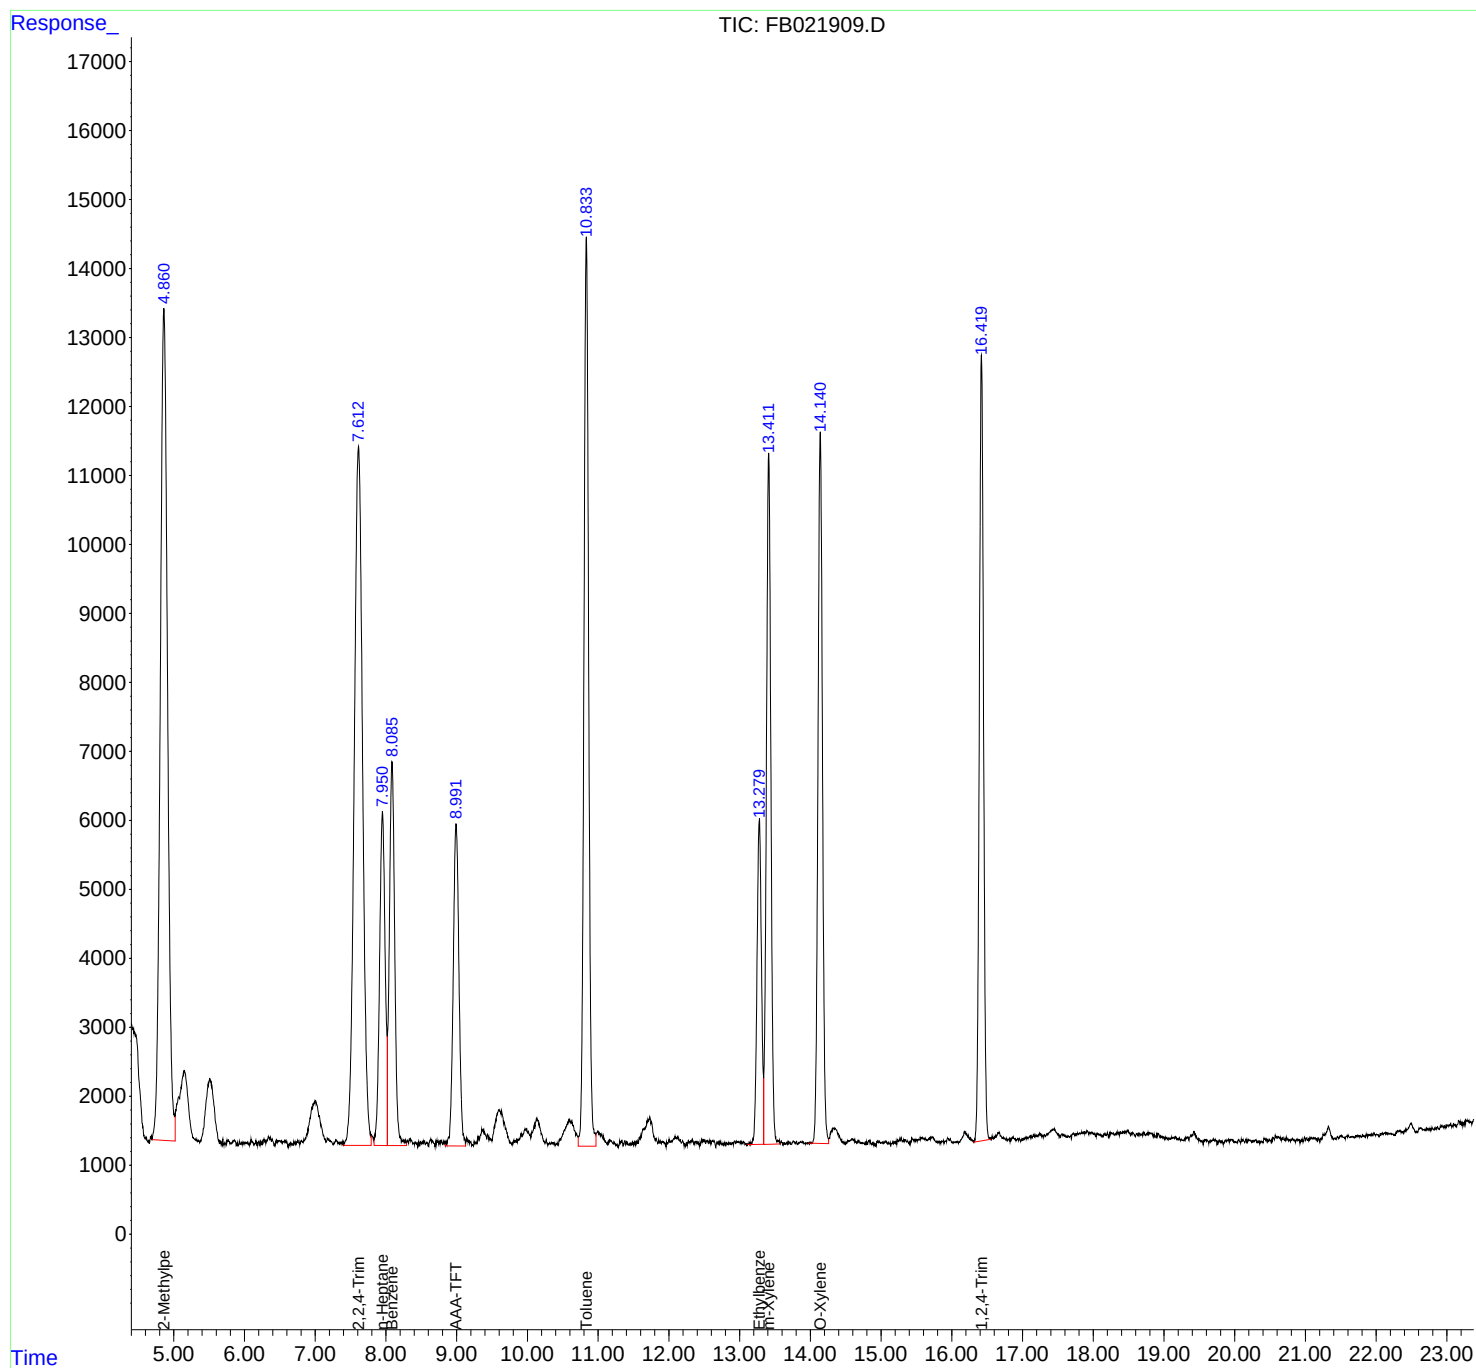

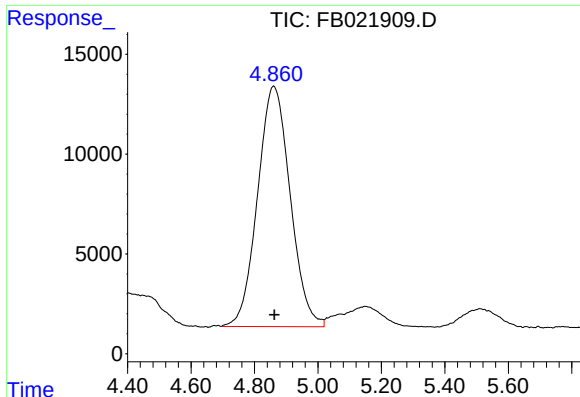


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 860240
Conc: 31.20 ng/ml

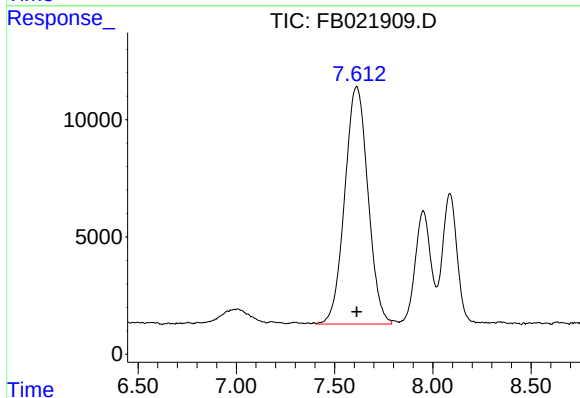


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.001 min
Response: 831395
Conc: 31.45 ng/ml

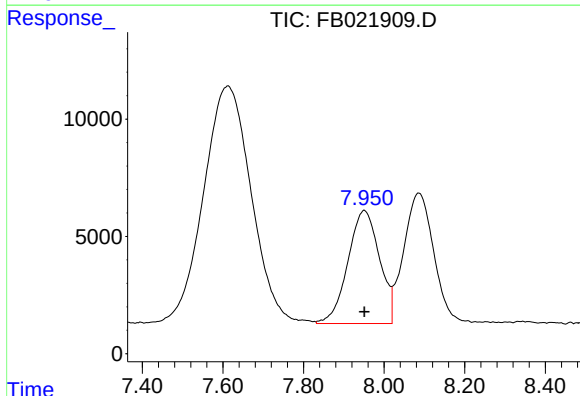


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 263081
Conc: 10.61 ng/ml

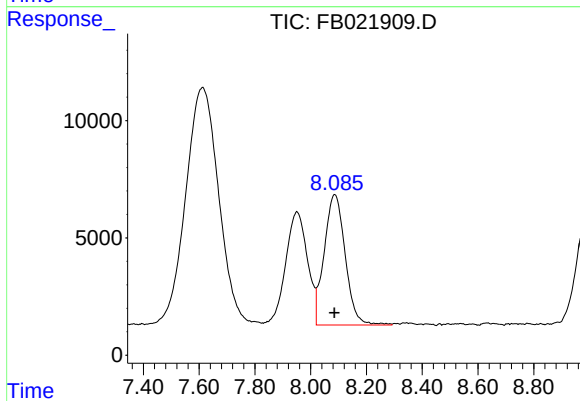


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.001 min
Response: 292182
Conc: 10.00 ng/ml

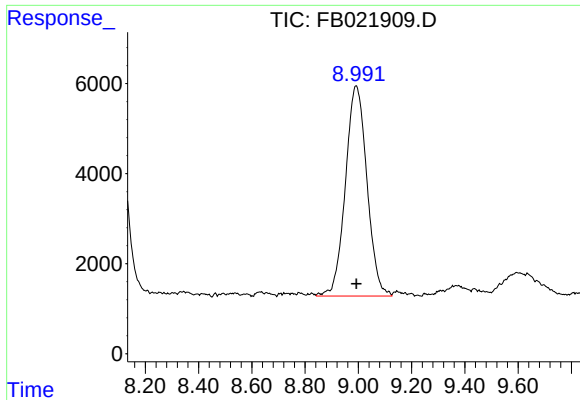


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 262559
Conc: 19.24 ng/ml

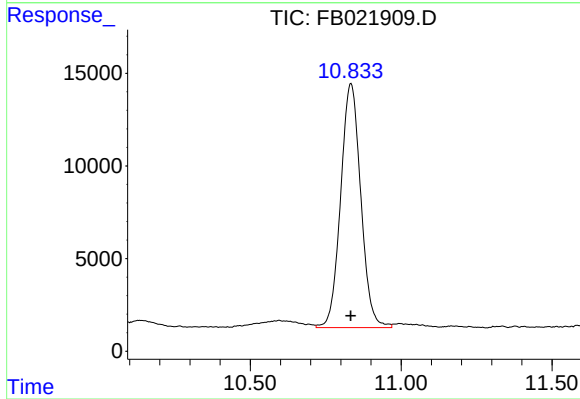


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 610239
Conc: 29.66 ng/ml

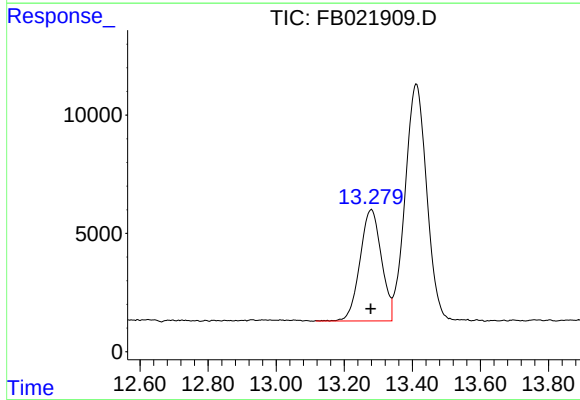


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 205061
Conc: 9.86 ng/ml

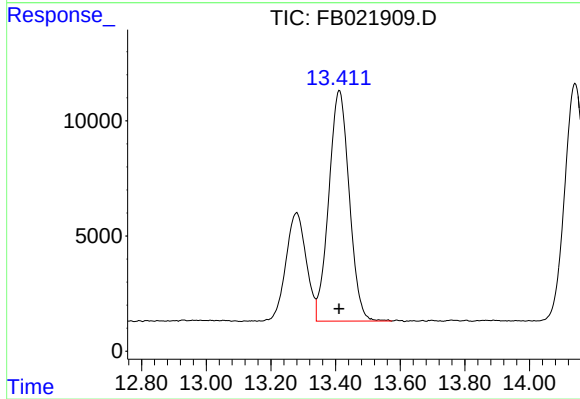

#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.001 min
Response: 440876
Conc: 19.85 ng/ml

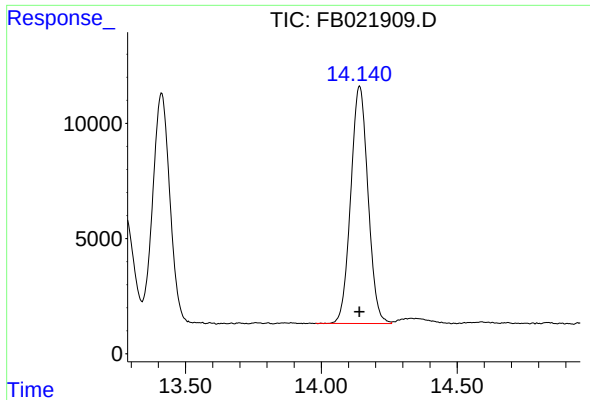


#9 O-Xylene

R.T.: 14.141 min

Delta R.T.: 0.000 min

Response: 455408

Conc: 19.80 ng/ml

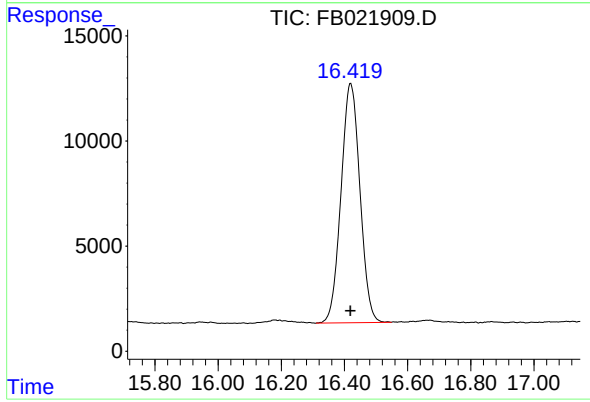

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min

Delta R.T.: 0.000 min

Response: 473768

Conc: 20.09 ng/ml