

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080519\
 Data File : FB021911.D
 Signal(s) : FID2B.CH
 Acq On : 5 Aug 2019 10:41
 Operator : DD/AJ
 Sample : K4090-01MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 00:56:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	296062	21.695 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	697694	25.301 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	697015	26.368 ng/ml
3) t n-Heptane	7.952	197052	7.947 ng/ml
4) t Benzene	8.087	274301	9.389 ng/ml
6) t Toluene	10.834	583861	28.375 ng/ml
7) t Ethylbenzene	13.280	199557	9.592 ng/ml
8) t m-Xylene	13.412	424338	19.101 ng/ml
9) t O-Xylene	14.142	443796	19.293 ng/ml
10) t 1,2,4-Trimethylbenzene	16.421	443622	18.816 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080519\
Data File : FB021911.D
Signal(s) : FID2B.CH
Acq On : 5 Aug 2019 10:41
Operator : DD/AJ
Sample : K4090-01MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 00:56:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

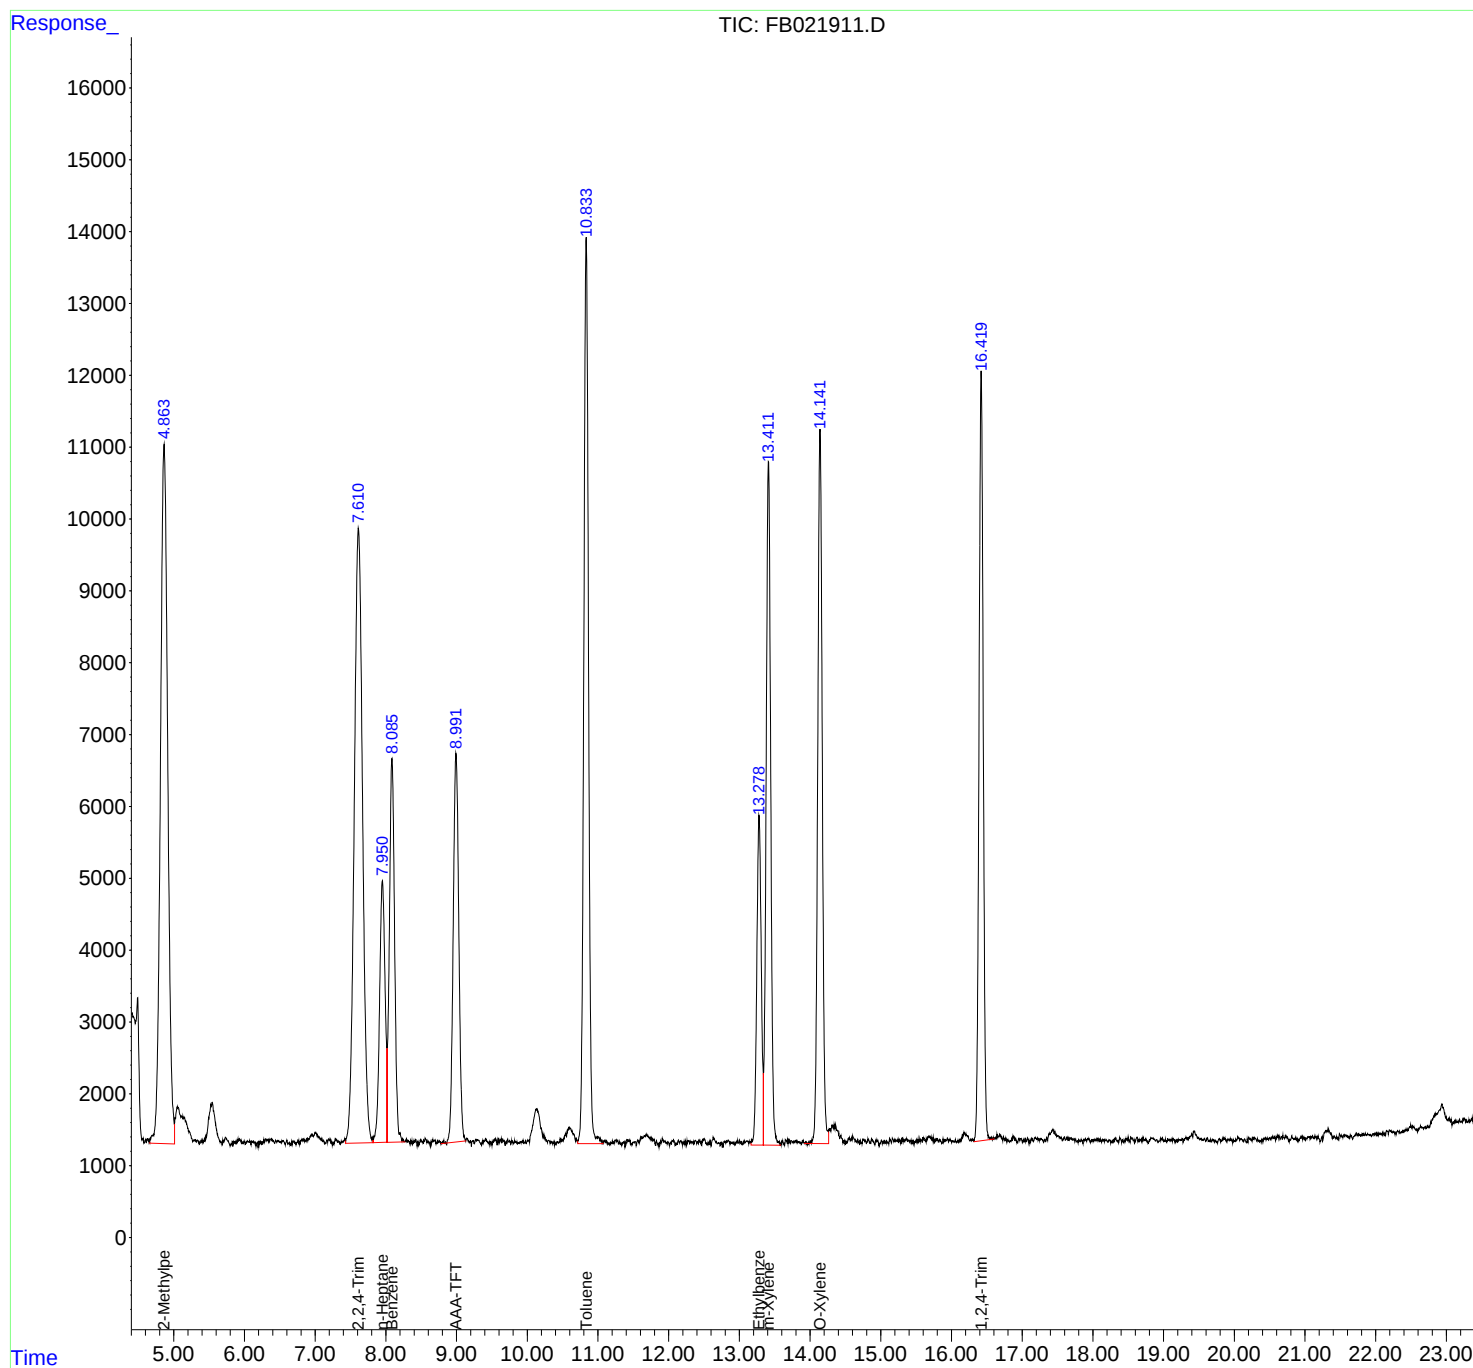

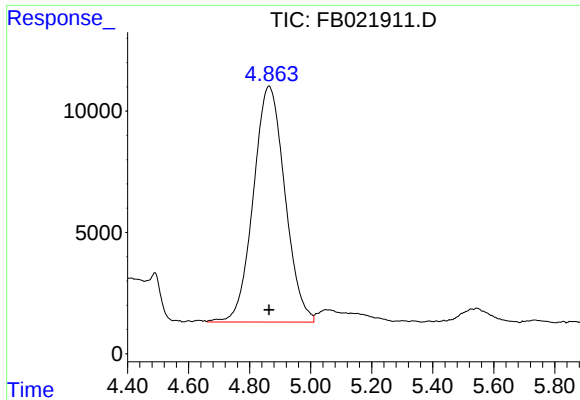


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 697694
Conc: 25.30 ng/ml

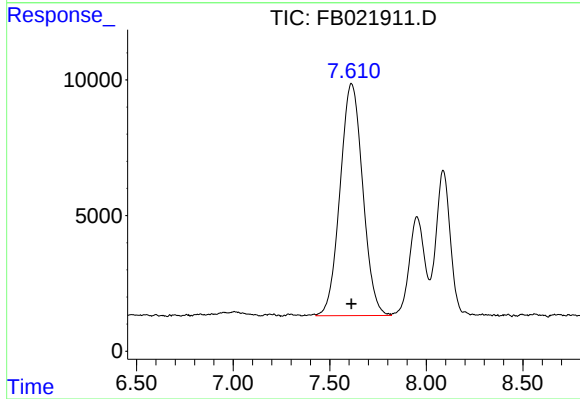


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 697015
Conc: 26.37 ng/ml

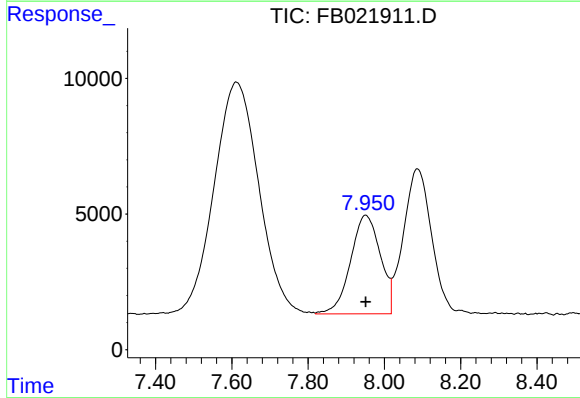


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 197052
Conc: 7.95 ng/ml

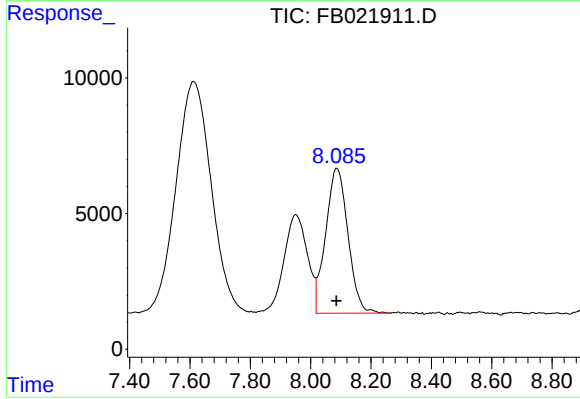


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.001 min
Response: 274301
Conc: 9.39 ng/ml

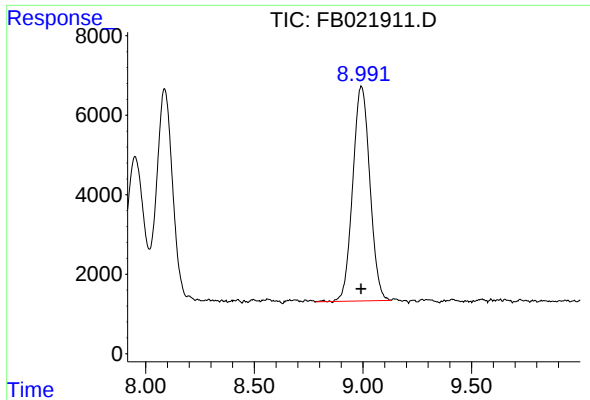


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 296062
Conc: 21.69 ng/ml

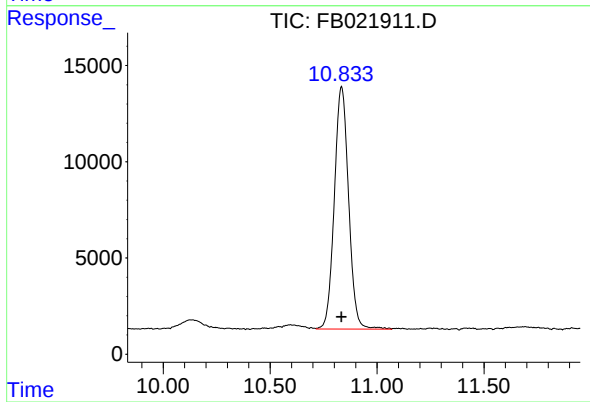


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.001 min
Response: 583861
Conc: 28.38 ng/ml

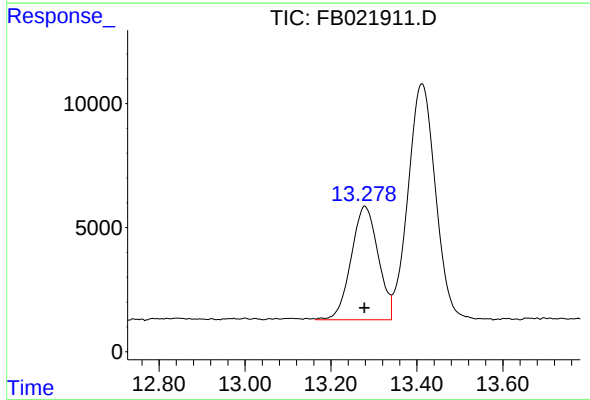


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 199557
Conc: 9.59 ng/ml

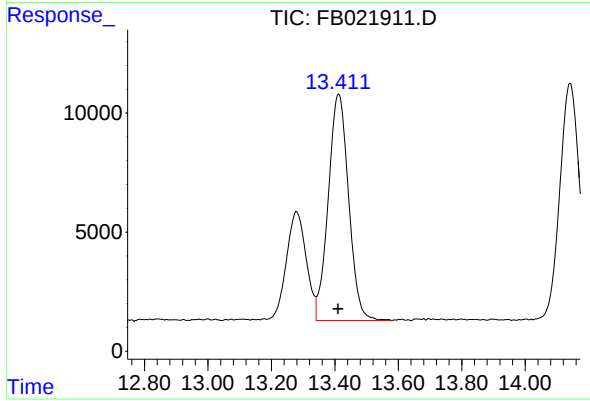


#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.002 min
Response: 424338
Conc: 19.10 ng/ml

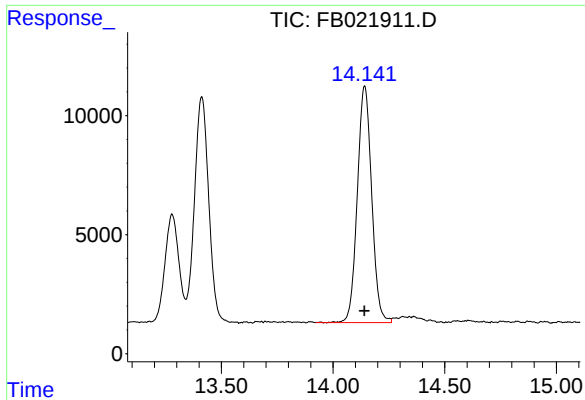

#9 O-Xylene

R.T.: 14.142 min
Delta R.T.: 0.001 min
Response: 443796
Conc: 19.29 ng/ml

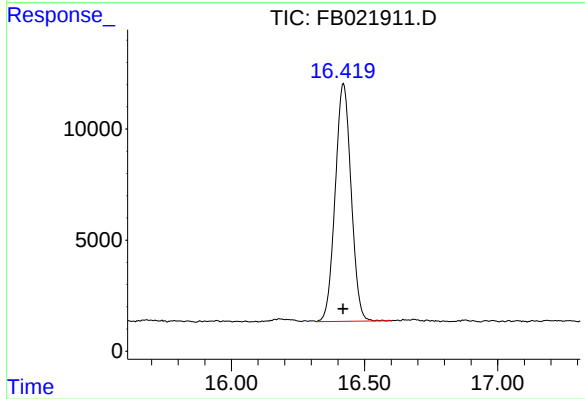

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: 0.002 min
Response: 443622
Conc: 18.82 ng/ml