

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080521\
 Data File : FB026124.D
 Signal(s) : FID2B.CH
 Acq On : 5 Aug 2021 14:08
 Operator : AJ/MA
 Sample : M3281-01MSD
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 05 22:18:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
 Quant Title :
 QLast Update : Tue Jul 27 12:01:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
1) t 2-Methylpentane	4.847	200955	6.123 ng/ml
2) t 2,2,4-Trimethylpentane	7.502	436231	13.401 ng/ml
3) t n-Heptane	7.837	218676	4.728 ng/ml
4) t Benzene	7.954	347238	7.147 ng/ml
6) t Toluene	10.654	601415	13.213 ng/ml
7) t Ethylbenzene	13.037	4759328	124.740 ng/ml
9) t O-Xylene	13.944	768501	24.787 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	312174	12.169 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080521\
Data File : FB026124.D
Signal(s) : FID2B.CH
Acq On : 5 Aug 2021 14:08
Operator : AJ/MA
Sample : M3281-01MSD
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 05 22:18:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
Quant Title :
QLast Update : Tue Jul 27 12:01:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

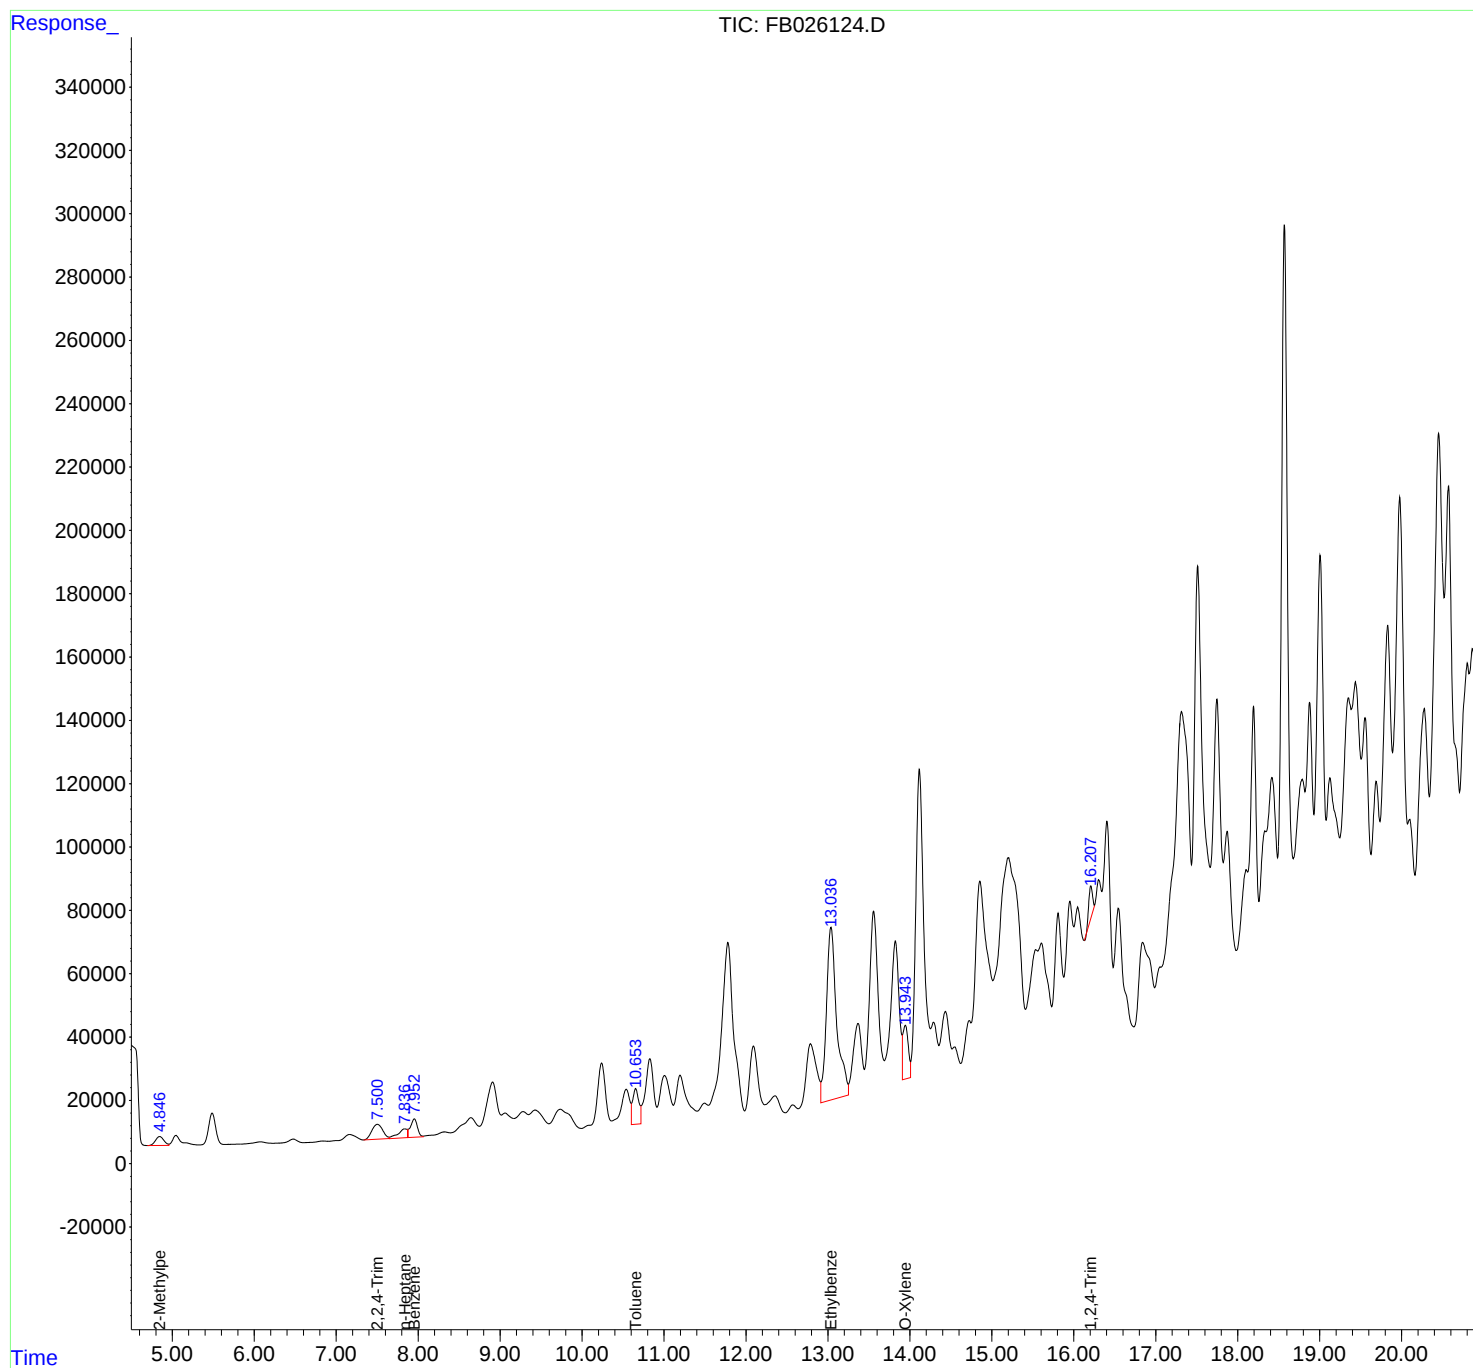


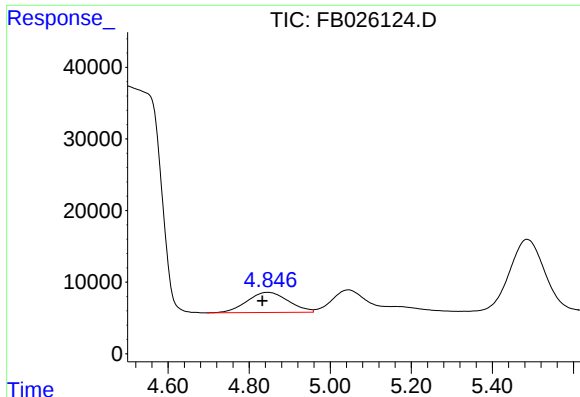

#1 2-Methylpentane


R.T.: 4.847 min
Delta R.T.: 0.014 min
Response: 200955
Conc: 6.12 ng/ml

Instrument :
FID_B
ClientSampleId :

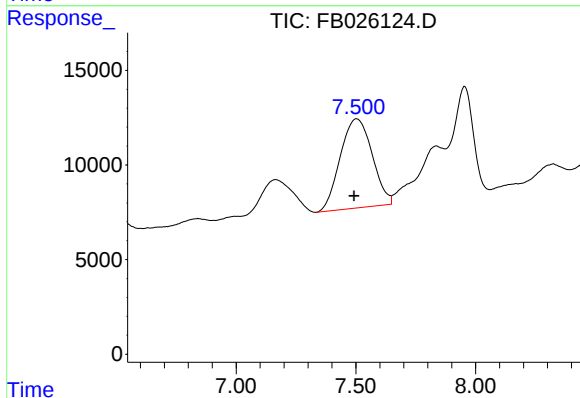


#2 2,2,4-Trimethylpentane

R.T.: 7.502 min
Delta R.T.: 0.008 min
Response: 436231
Conc: 13.40 ng/ml

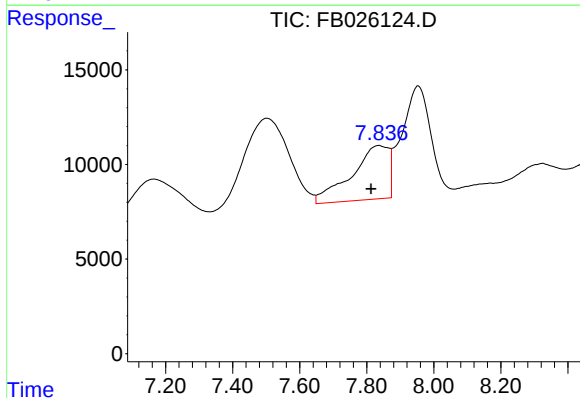


#3 n-Heptane

R.T.: 7.837 min
Delta R.T.: 0.024 min
Response: 218676
Conc: 4.73 ng/ml

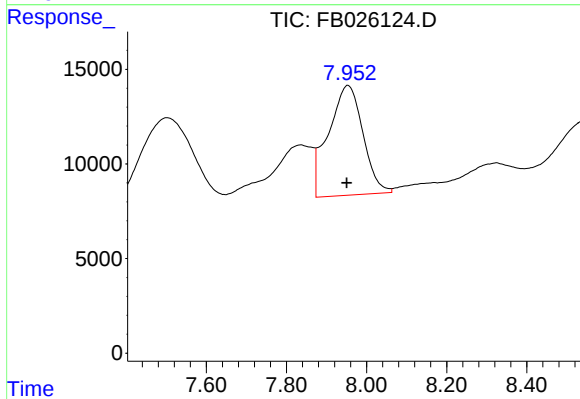

#4 Benzene


R.T.: 7.954 min
Delta R.T.: 0.003 min
Response: 347238
Conc: 7.15 ng/ml

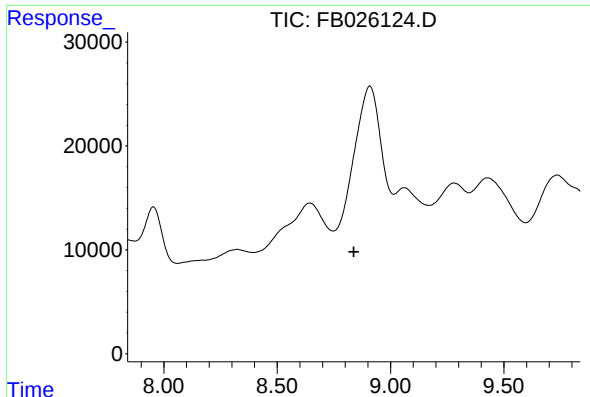

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.837 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :

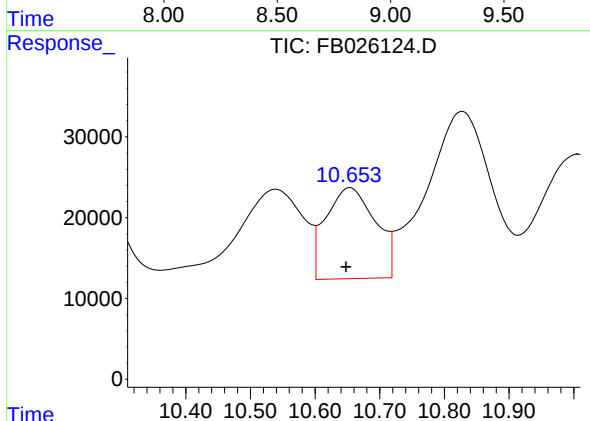


#6 Toluene

R.T.: 10.654 min
Delta R.T.: 0.006 min
Response: 601415
Conc: 13.21 ng/ml

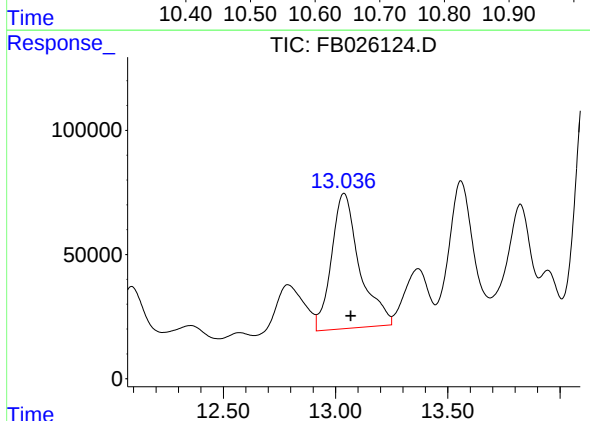


#7 Ethylbenzene

R.T.: 13.037 min
Delta R.T.: -0.031 min
Response: 4759328
Conc: 124.74 ng/ml

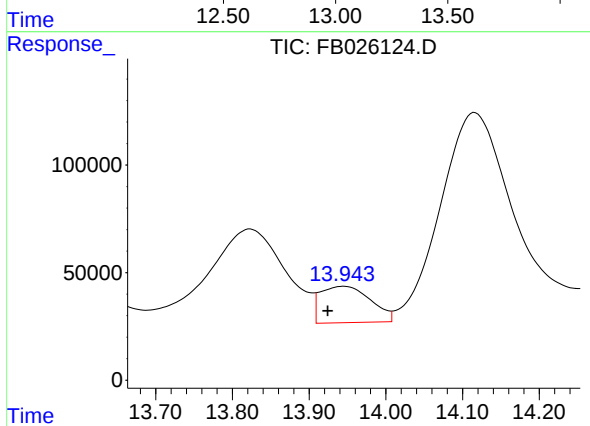

#9 O-Xylene

R.T.: 13.944 min
Delta R.T.: 0.020 min
Response: 768501
Conc: 24.79 ng/ml

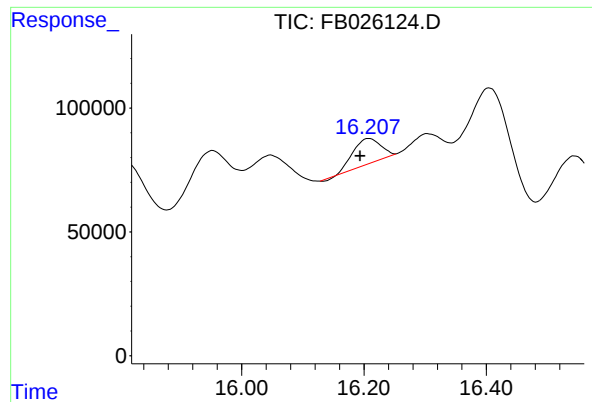

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.016 min
Response: 312174
Conc: 12.17 ng/ml

Instrument :
FID_B
ClientSampleId :