

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080521\
 Data File : FB026121.D
 Signal(s) : FID2B.CH
 Acq On : 5 Aug 2021 11:31
 Operator : AJ/MA
 Sample : BSF0805S1
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0805S1

Integration File: Calibration.e
 Quant Time: Aug 05 22:18:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
 Quant Title :
 QLast Update : Tue Jul 27 12:01:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.834	470649	16.960 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.821	786117	23.951 ng/ml
2) t 2,2,4-Trimethylpentane	7.489	772214	23.722 ng/ml
3) t n-Heptane	7.809	362461	7.837 ng/ml
4) t Benzene	7.947	407429	8.386 ng/ml
6) t Toluene	10.647	1139077	25.025 ng/ml
7) t Ethylbenzene	13.068	320534	8.401 ng/ml
8) t m-Xylene	13.201	609710	16.911 ng/ml
9) t O-Xylene	13.925	532445	17.173 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	367365	14.321 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080521\
Data File : FB026121.D
Signal(s) : FID2B.CH
Acq On : 5 Aug 2021 11:31
Operator : AJ/MA
Sample : BSF0805S1
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0805S1

Integration File: Calibration.e
Quant Time: Aug 05 22:18:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
Quant Title :
QLast Update : Tue Jul 27 12:01:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

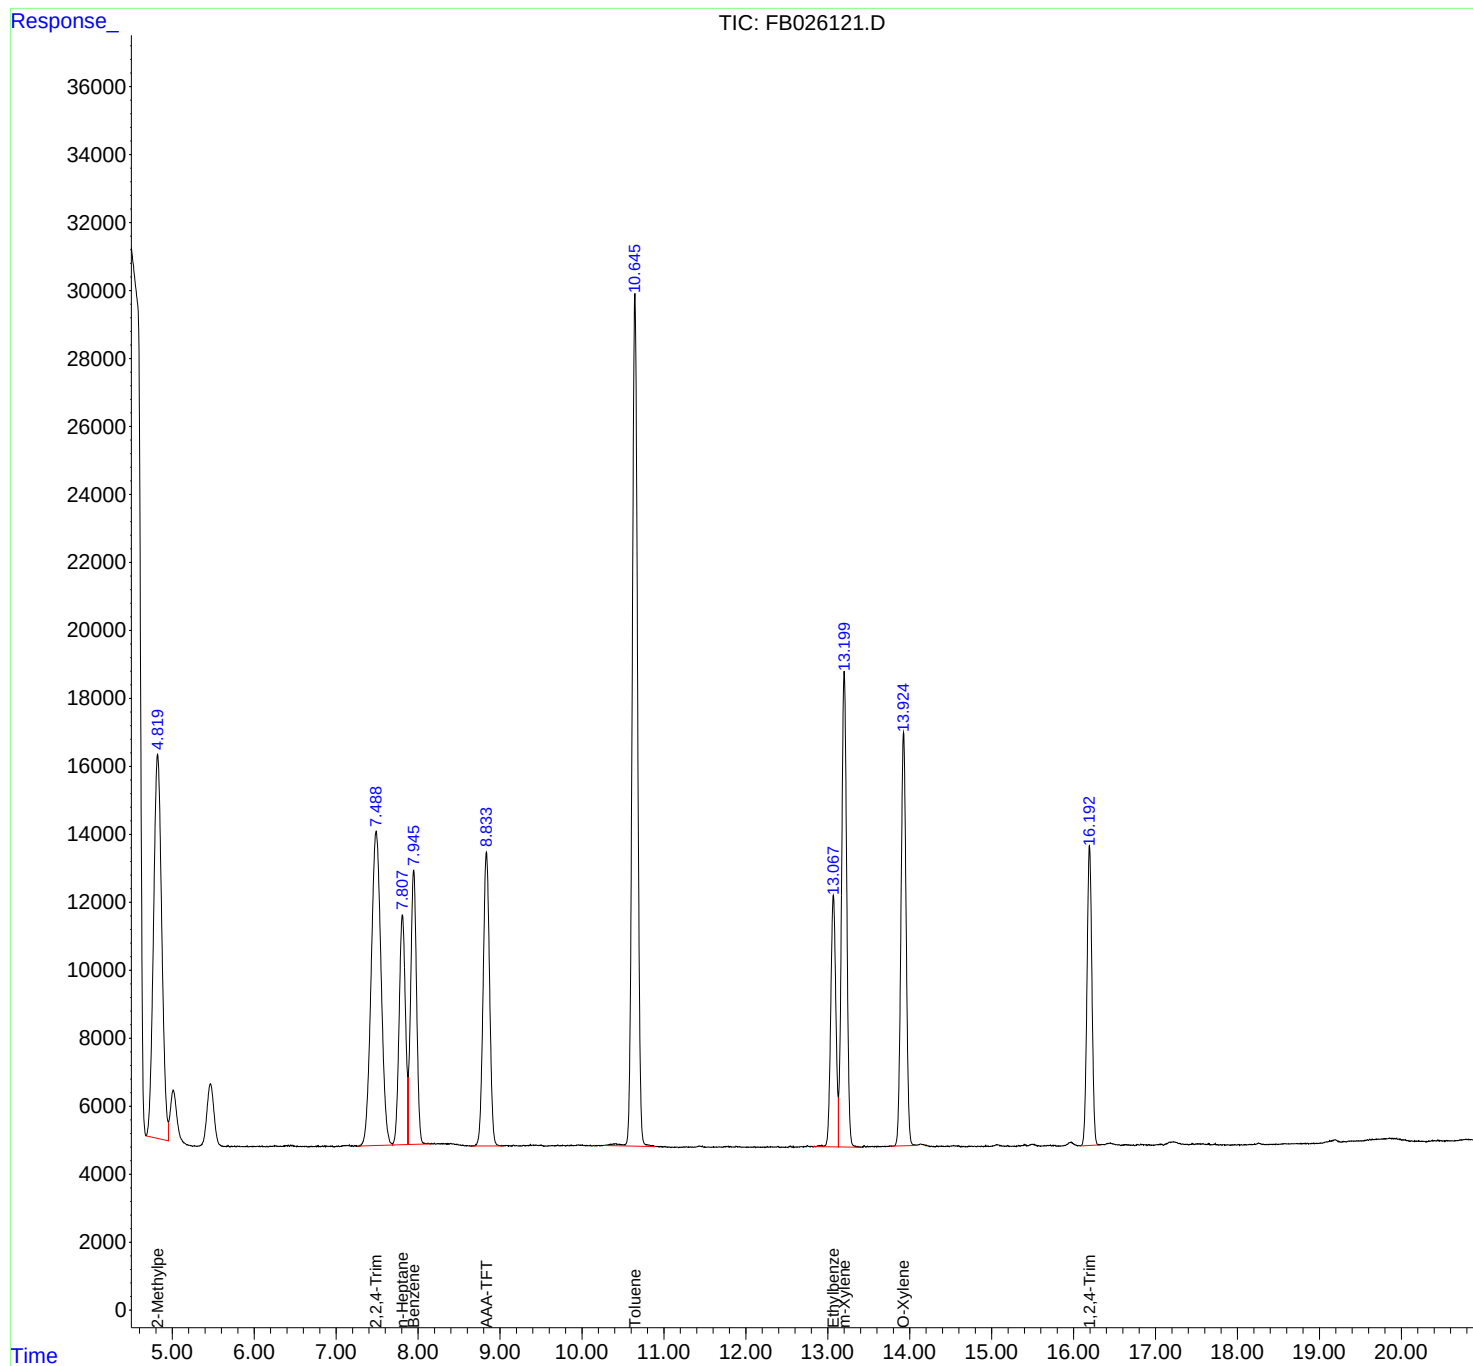


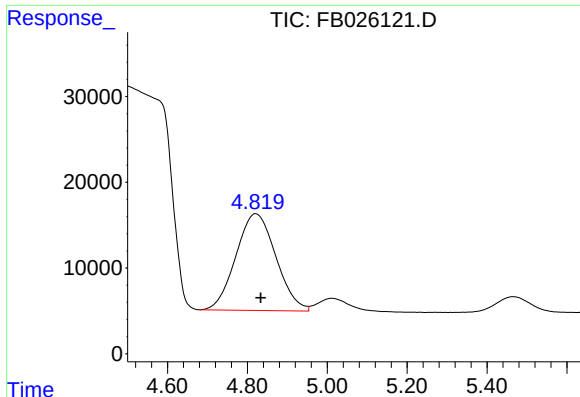

#1 2-Methylpentane


R.T.: 4.821 min
Delta R.T.: -0.012 min
Response: 786117
Conc: 23.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0805S1

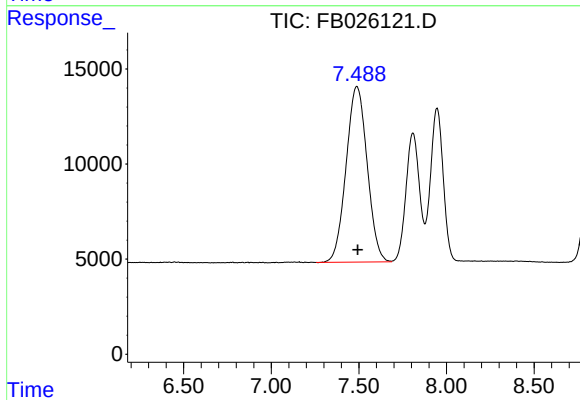


#2 2,2,4-Trimethylpentane

R.T.: 7.489 min
Delta R.T.: -0.005 min
Response: 772214
Conc: 23.72 ng/ml

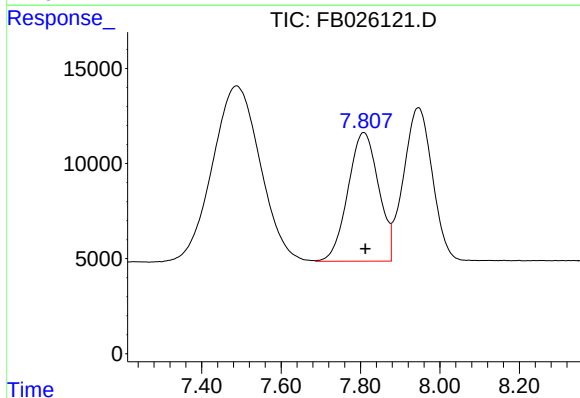


#3 n-Heptane

R.T.: 7.809 min
Delta R.T.: -0.004 min
Response: 362461
Conc: 7.84 ng/ml

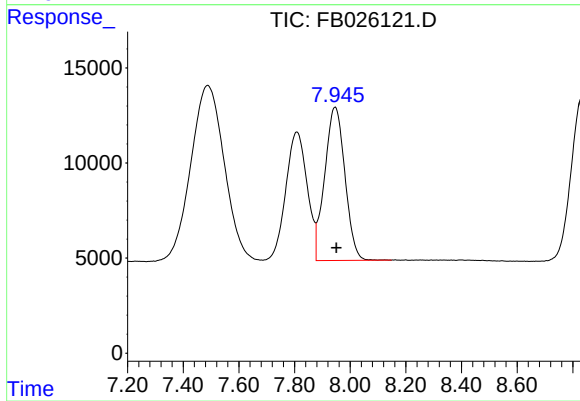

#4 Benzene


R.T.: 7.947 min
Delta R.T.: -0.004 min
Response: 407429
Conc: 8.39 ng/ml

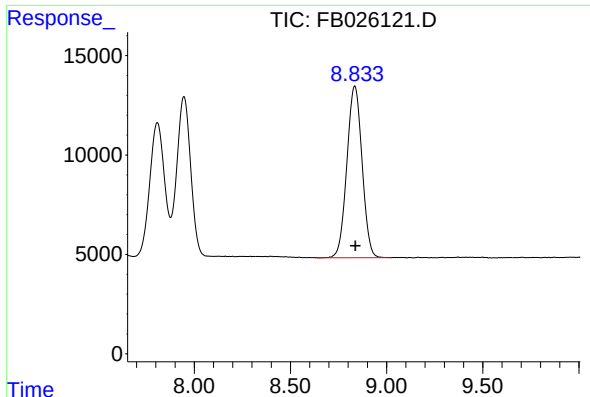

#5 AAA-TFT


R.T.: 8.834 min
Delta R.T.: -0.003 min
Response: 470649
Conc: 16.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0805S1

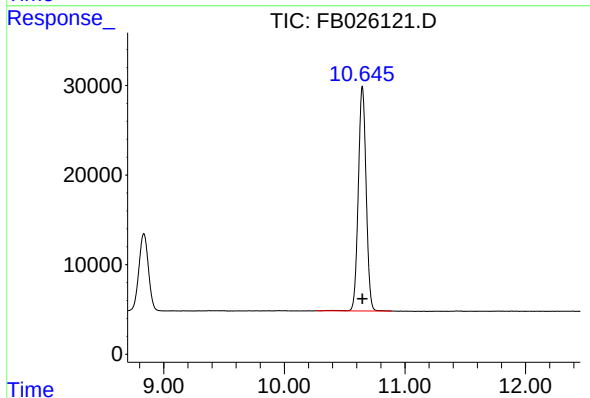


#6 Toluene

R.T.: 10.647 min
Delta R.T.: -0.002 min
Response: 1139077
Conc: 25.02 ng/ml

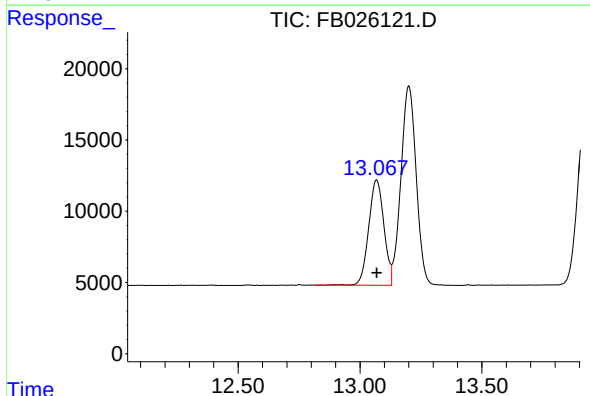


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.000 min
Response: 320534
Conc: 8.40 ng/ml

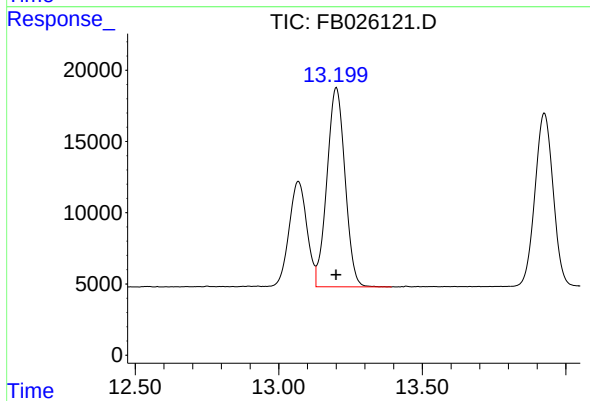

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 609710
Conc: 16.91 ng/ml

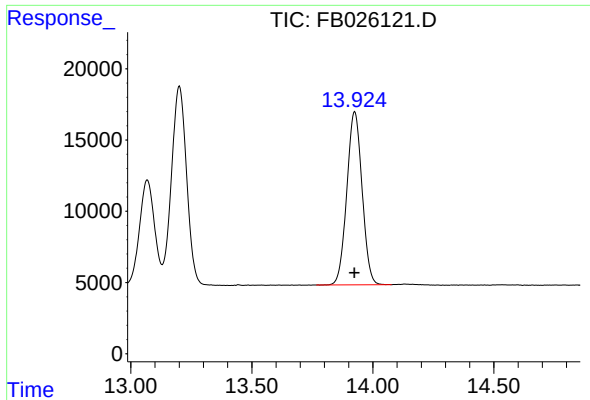

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.000 min
Response: 532445
Conc: 17.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0805S1

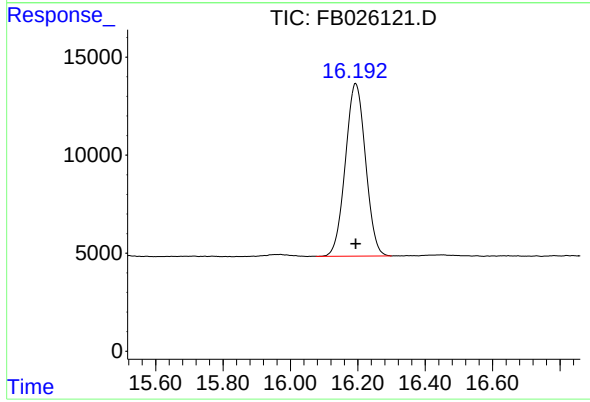

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 367365
Conc: 14.32 ng/ml