

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080522\
 Data File : FB027841.D
 Signal(s) : FID2B.CH
 Acq On : 5 Aug 2022 14:02
 Operator : AJ/MA
 Sample : BSF0805S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0805S1

Integration File: SAMPLE.e
 Quant Time: Aug 08 09:21:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:59:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	261472	22.466 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	593435	28.179 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	629752	30.347 ng/ml
3) t n-Heptane	7.754	209486	10.190 ng/ml
4) t Benzene	7.892	248599	10.594 ng/ml
6) t Toluene	10.624	712307	31.899 ng/ml
7) t Ethylbenzene	13.061	220925	10.543 ng/ml
8) t m-Xylene	13.194	439961	21.013 ng/ml
9) t O-Xylene	13.921	423332	20.688 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	409332	19.697 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080522\
Data File : FB027841.D
Signal(s) : FID2B.CH
Acq On : 5 Aug 2022 14:02
Operator : AJ/MA
Sample : BSF0805S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0805S1

Integration File: SAMPLE.e
Quant Time: Aug 08 09:21:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:59:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

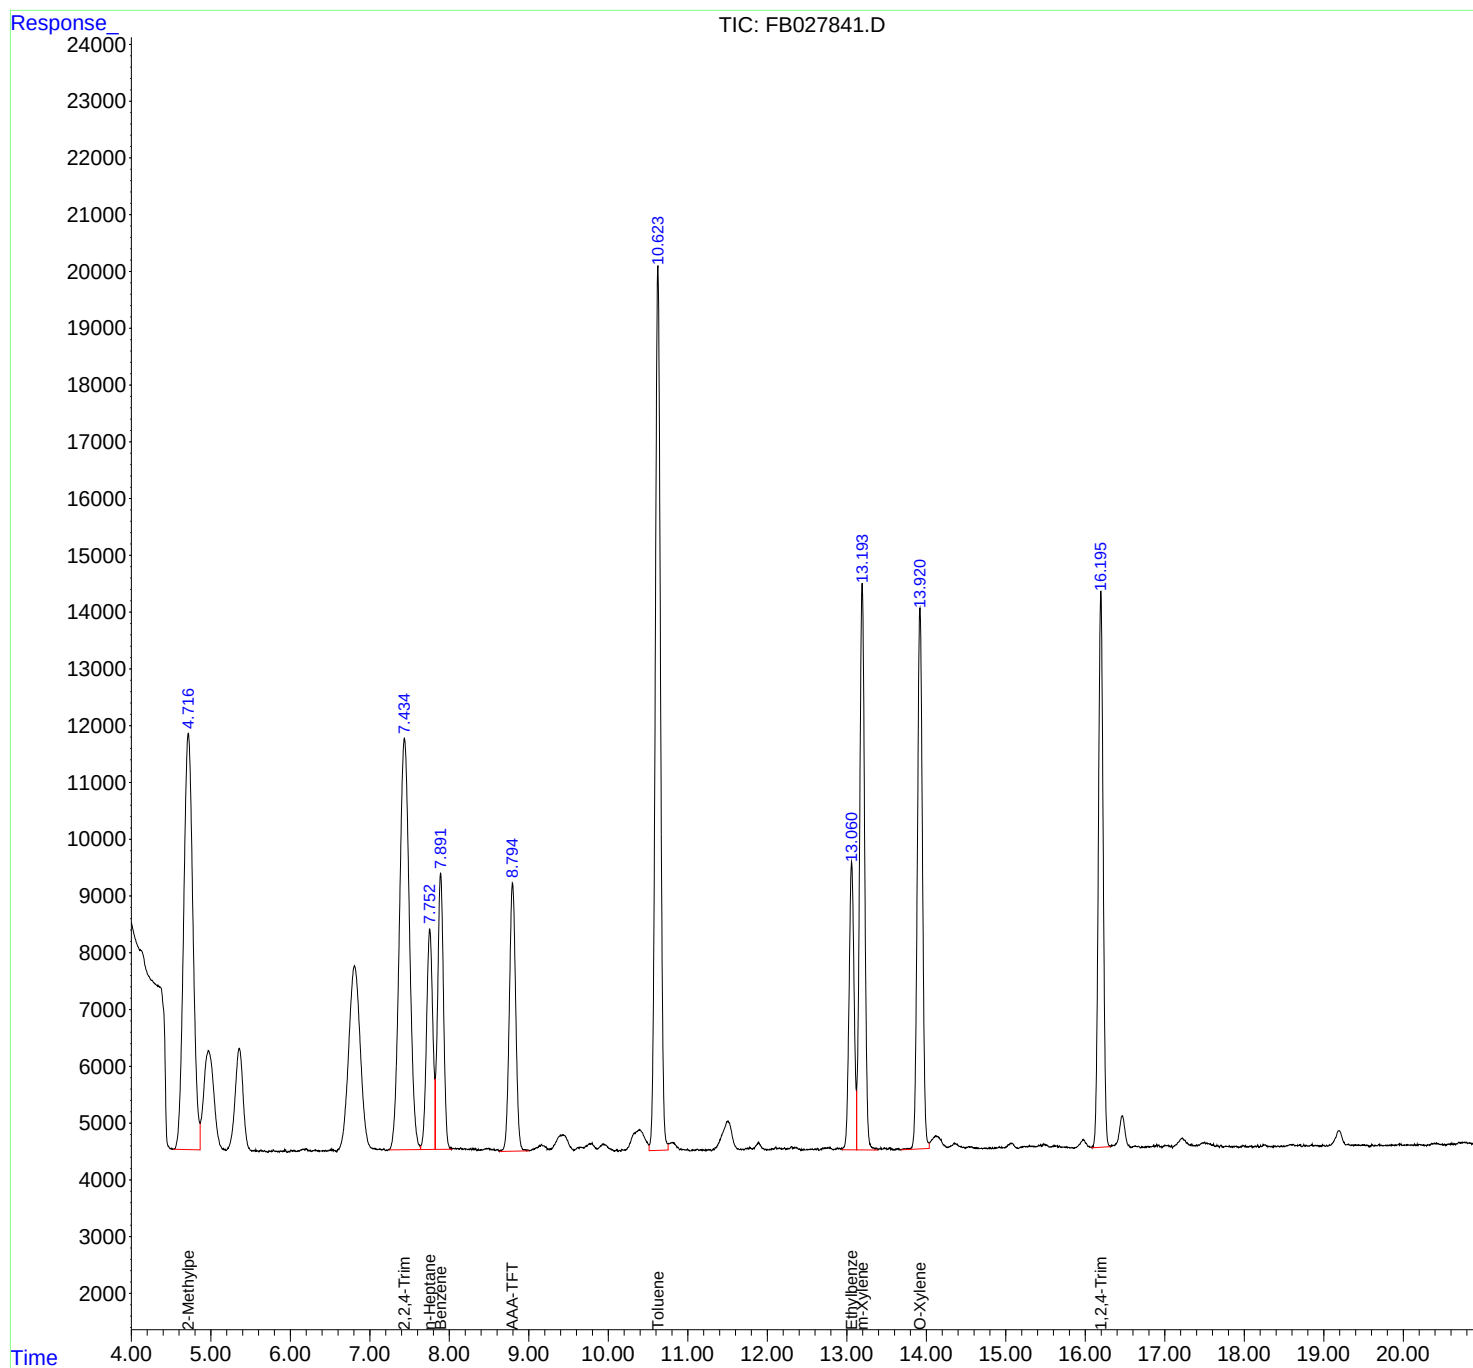


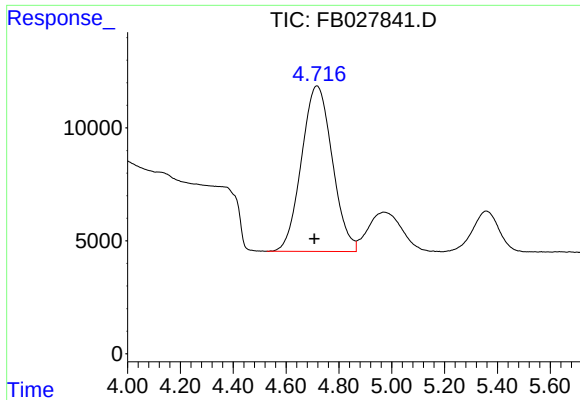

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.010 min
Response: 593435
Conc: 28.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0805S1

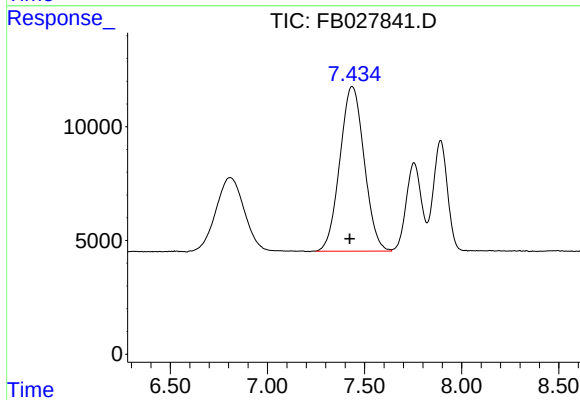


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.012 min
Response: 629752
Conc: 30.35 ng/ml

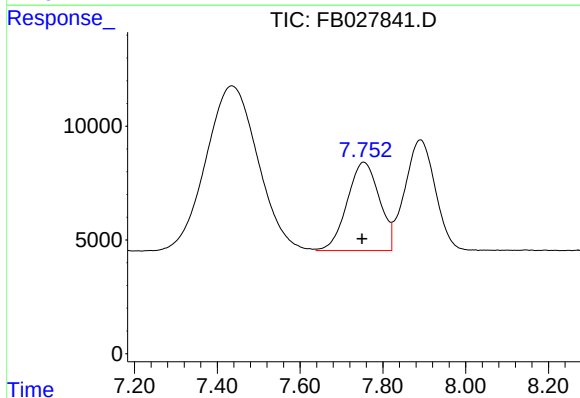


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.004 min
Response: 209486
Conc: 10.19 ng/ml

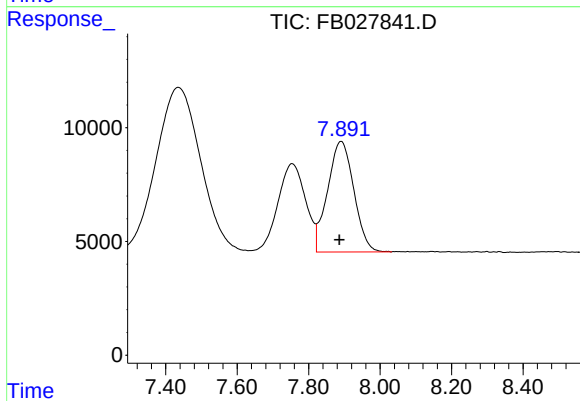

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.005 min
Response: 248599
Conc: 10.59 ng/ml

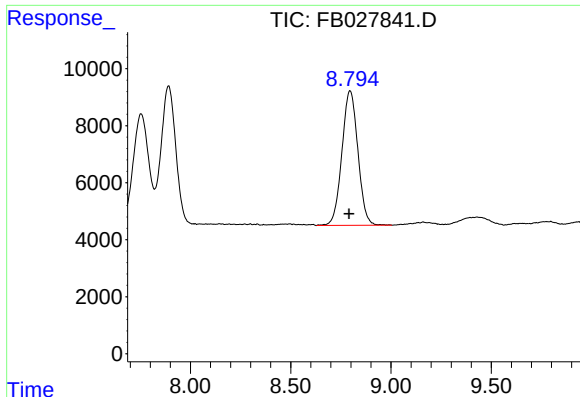

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 261472
Conc: 22.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0805S1

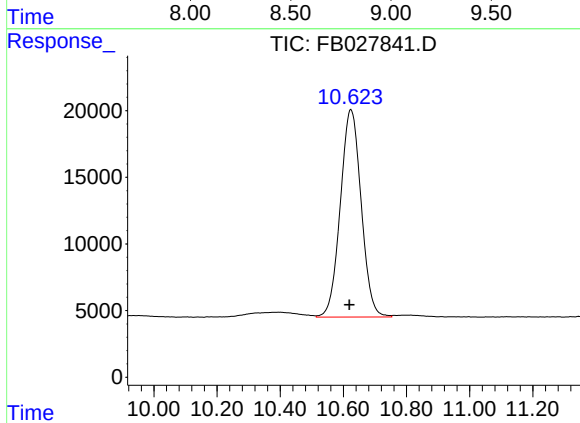


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 712307
Conc: 31.90 ng/ml

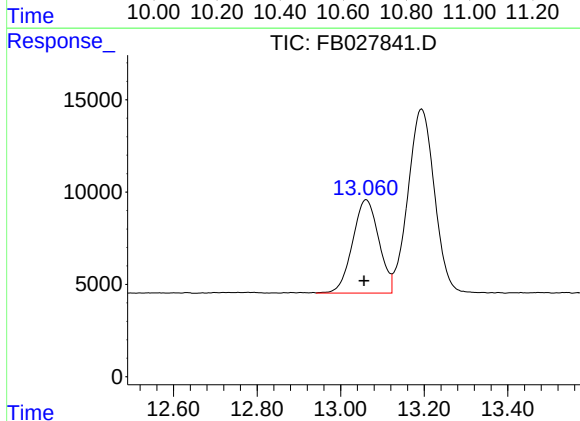


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.006 min
Response: 220925
Conc: 10.54 ng/ml

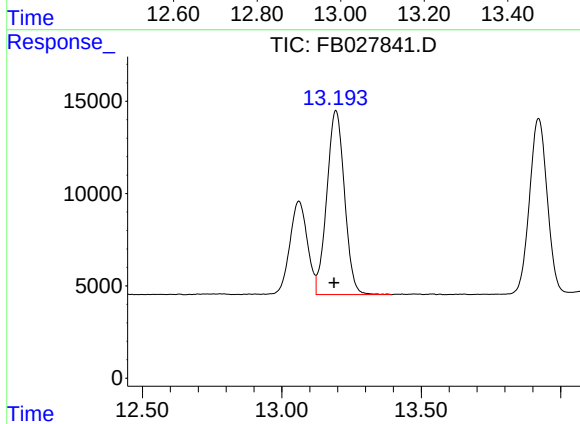

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.006 min
Response: 439961
Conc: 21.01 ng/ml

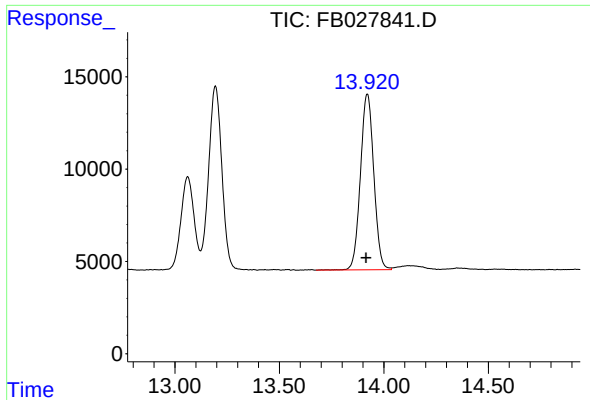

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.006 min
Response: 423332
Conc: 20.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0805S1

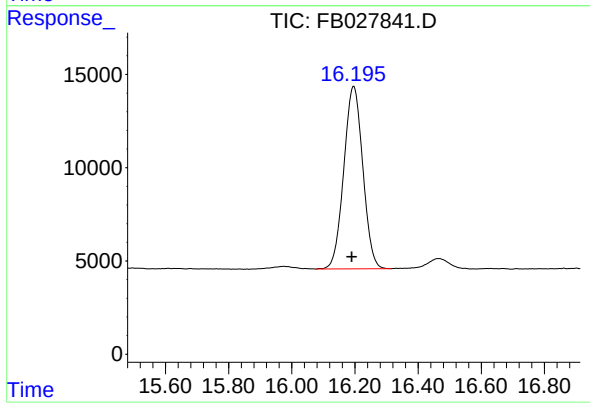

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.006 min
Response: 409332
Conc: 19.70 ng/ml