

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080618\
Data File : FB017163.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2018 13:00
Operator : MJ/SJ
Sample : J4277-01
Misc : 5.01g/5.00ml DI water
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 07 08:31:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.116	192657	24.344 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.666	467	0.033 ng/ml
4) t	Benzene	8.213	15435	0.879 ng/ml
6) t	Toluene	10.972	6946	0.506 ng/ml
7) t	Ethylbenzene	13.413	7429	0.545 ng/ml
8) t	m-Xylene	13.540	11255	0.782 ng/ml
9) t	O-Xylene	14.280	14818	0.972 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080618\
Data File : FB017163.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2018 13:00
Operator : MJ/SJ
Sample : J4277-01
Misc : 5.01g/5.00ml DI water
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 07 08:31:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

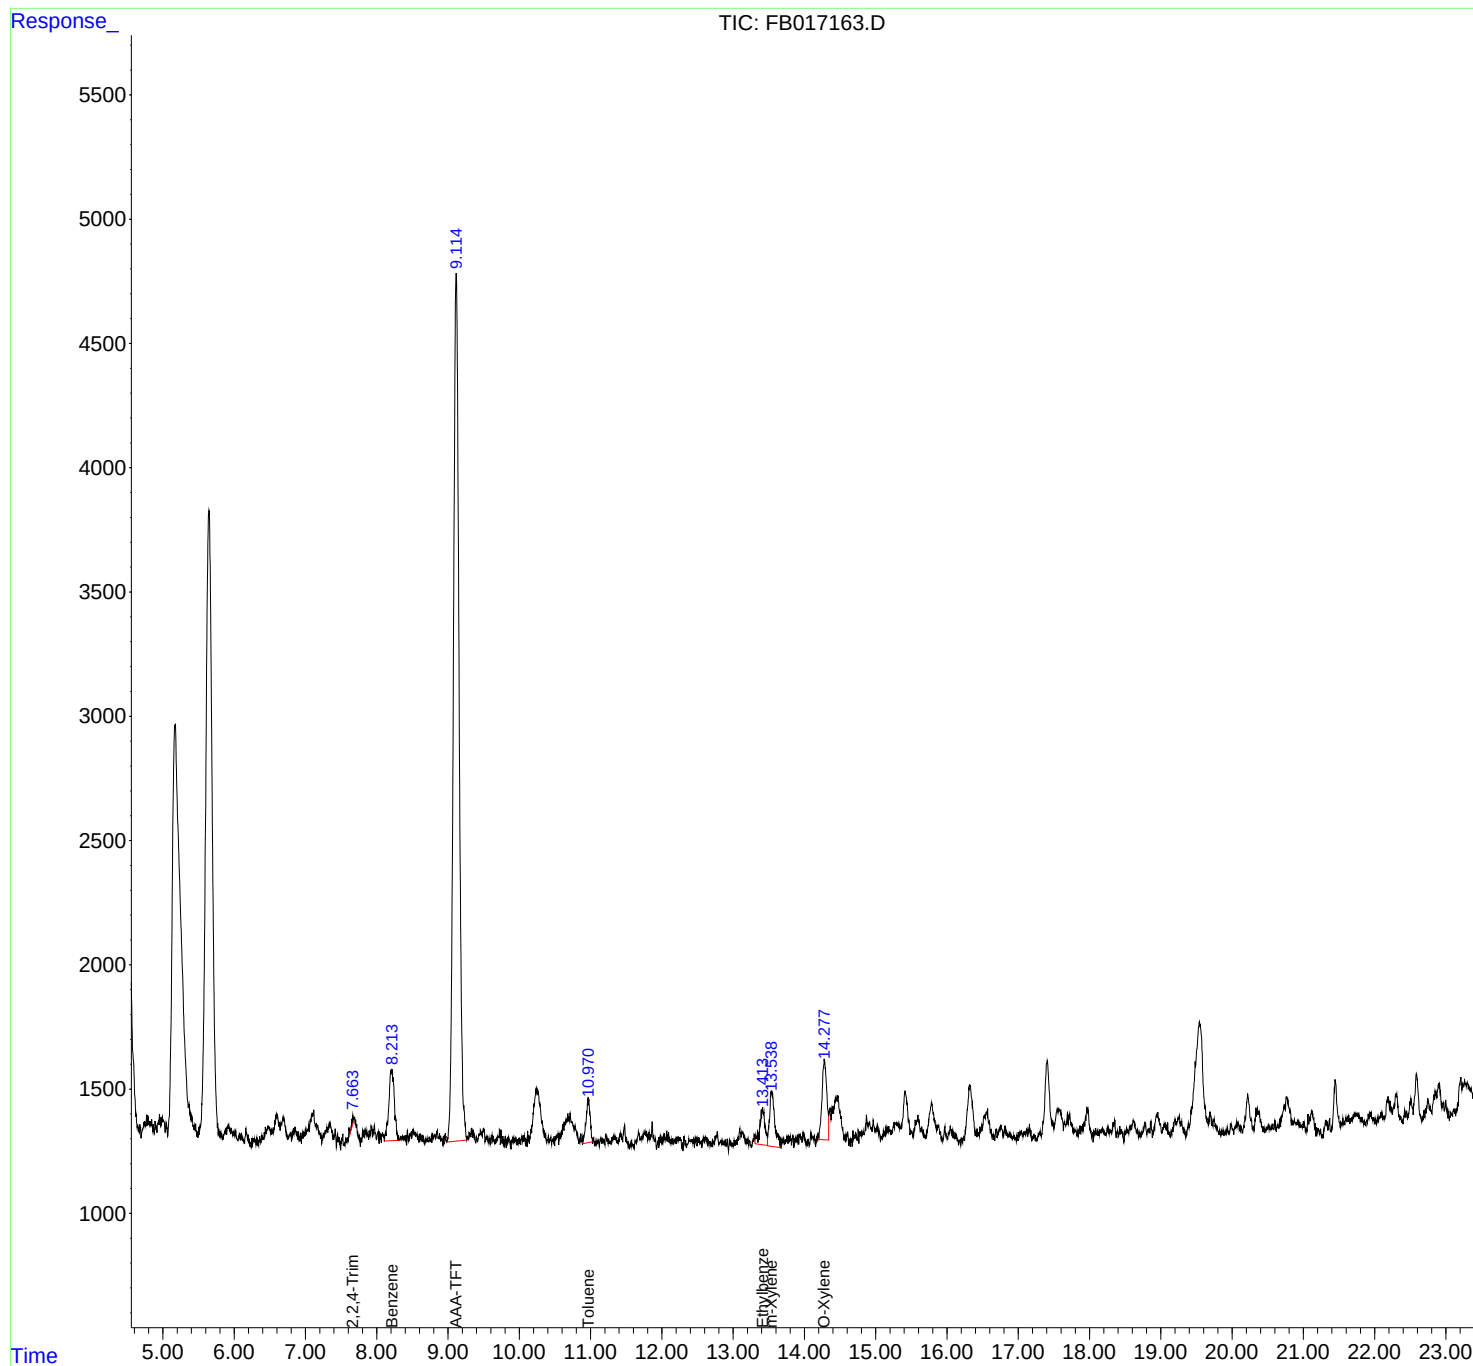

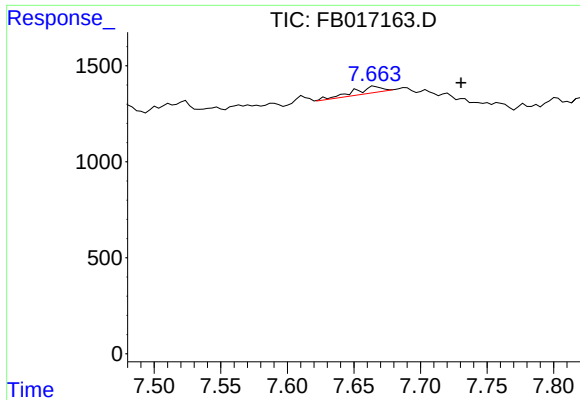


#2 2,2,4-Trimethylpentane

R.T.: 7.666 min
Delta R.T.: -0.064 min
Response: 467
Conc: 0.03 ng/ml

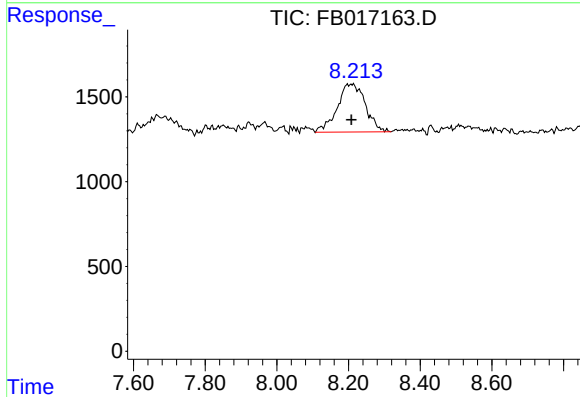


#4 Benzene

R.T.: 8.213 min
Delta R.T.: 0.005 min
Response: 15435
Conc: 0.88 ng/ml

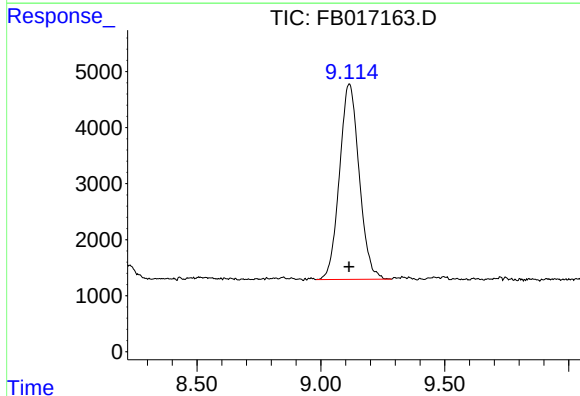


#5 AAA-TFT

R.T.: 9.116 min
Delta R.T.: 0.002 min
Response: 192657
Conc: 24.34 ng/ml

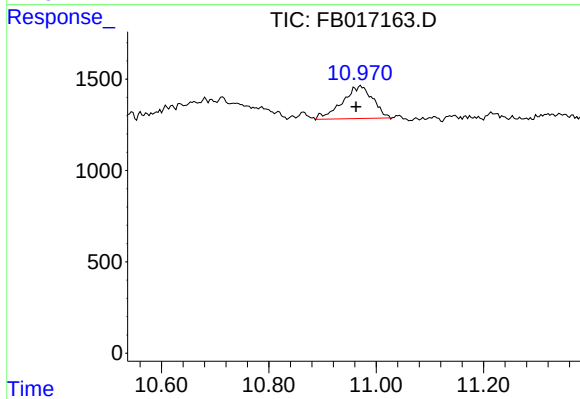


#6 Toluene

R.T.: 10.972 min
Delta R.T.: 0.009 min
Response: 6946
Conc: 0.51 ng/ml

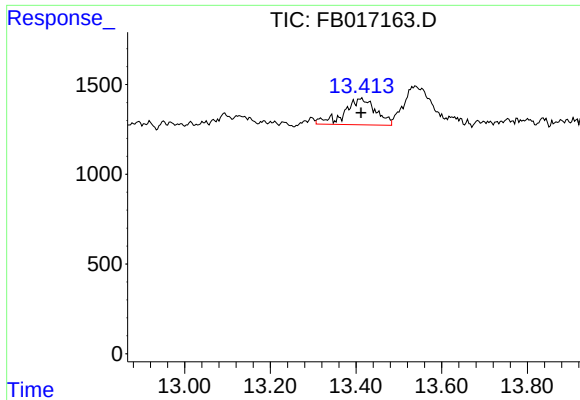


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.000 min
Response: 7429
Conc: 0.54 ng/ml

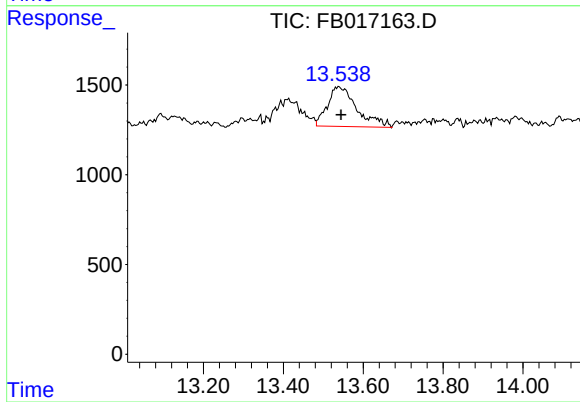

#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.005 min
Response: 11255
Conc: 0.78 ng/ml

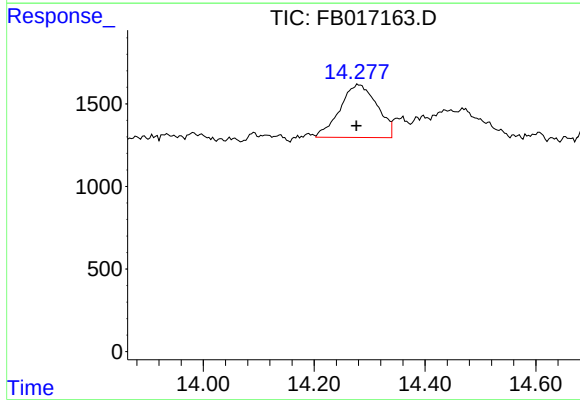

#9 O-Xylene

R.T.: 14.280 min
Delta R.T.: 0.004 min
Response: 14818
Conc: 0.97 ng/ml