

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080618\
Data File : FB017166.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2018 14:31
Operator : MJ/SJ
Sample : J4346-01MSD
Misc : 5.00g/5.00ml DI water
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 07 08:32:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.114	155881	19.697 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.966	336141	23.287 ng/ml
2) t	2,2,4-Trimethylpentane	7.731	241286	17.248 ng/ml
3) t	n-Heptane	8.069	80215	5.704 ng/ml
4) t	Benzene	8.208	152759	8.695 ng/ml
6) t	Toluene	10.964	370471	26.977 ng/ml
7) t	Ethylbenzene	13.414	122391	8.975 ng/ml
8) t	m-Xylene	13.547	258212	17.947 ng/ml
9) t	O-Xylene	14.279	288251	18.901 ng/ml
10) t	1,2,4-Trimethylbenzene	16.560	299493	16.227 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080618\
Data File : FB017166.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2018 14:31
Operator : MJ/SJ
Sample : J4346-01MSD
Misc : 5.00g/5.00ml DI water
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 07 08:32:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

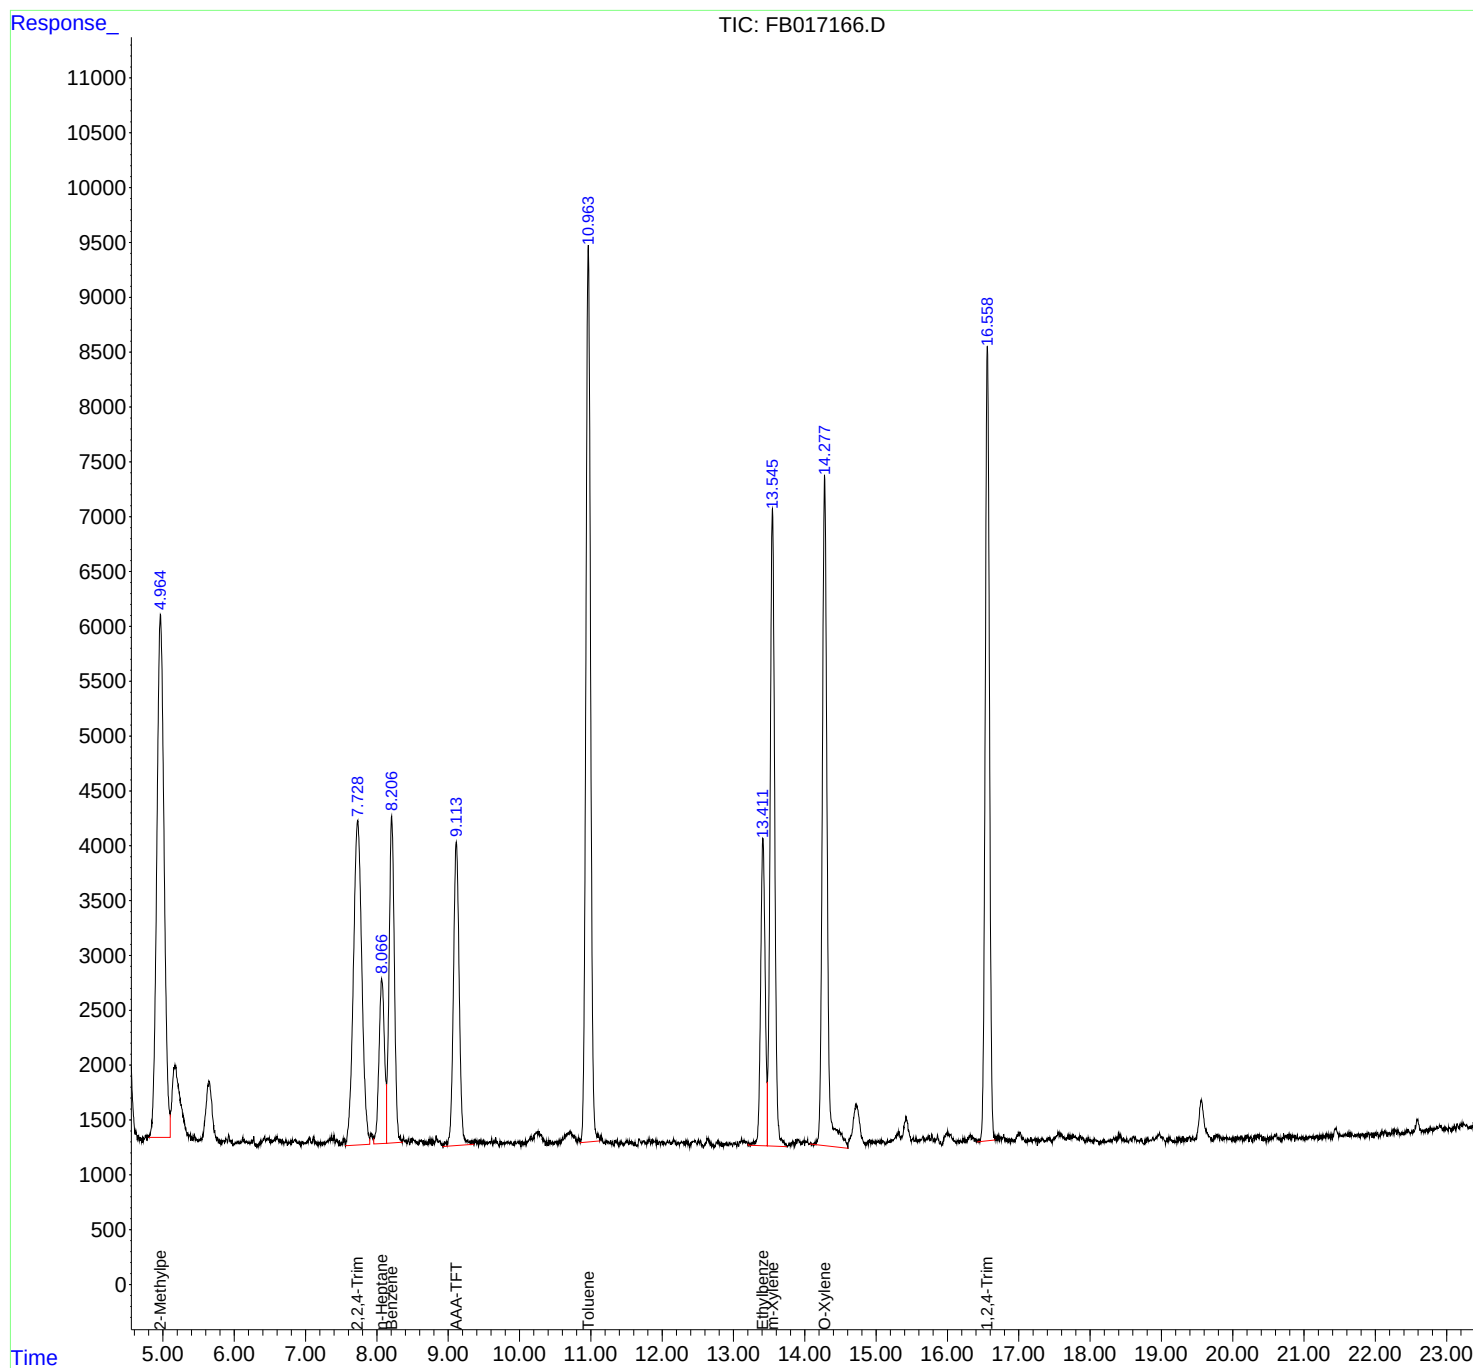

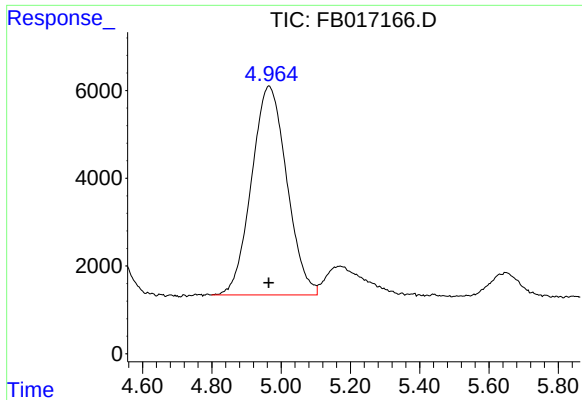


#1 2-Methylpentane

R.T.: 4.966 min
Delta R.T.: 0.002 min
Response: 336141
Conc: 23.29 ng/ml

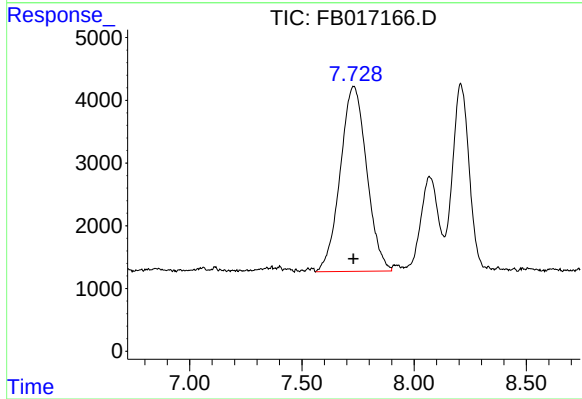


#2 2,2,4-Trimethylpentane

R.T.: 7.731 min
Delta R.T.: 0.000 min
Response: 241286
Conc: 17.25 ng/ml

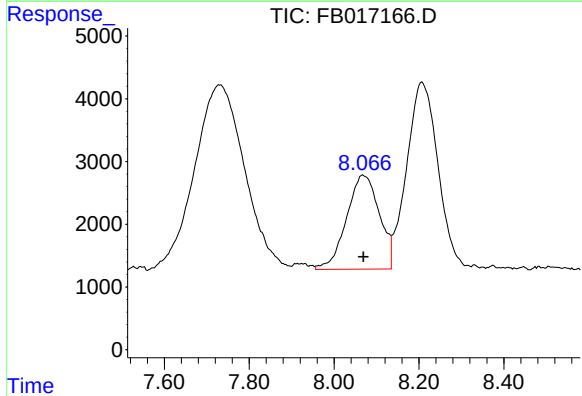


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 80215
Conc: 5.70 ng/ml

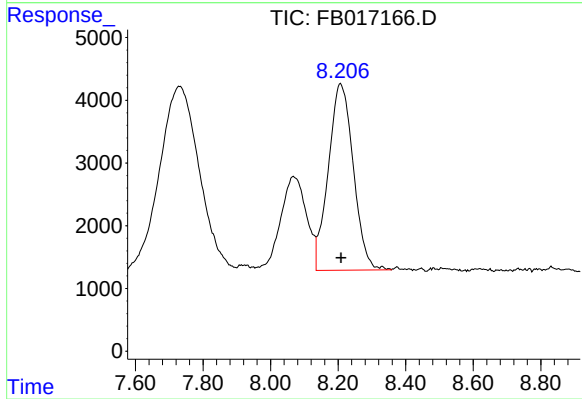


#4 Benzene

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 152759
Conc: 8.70 ng/ml

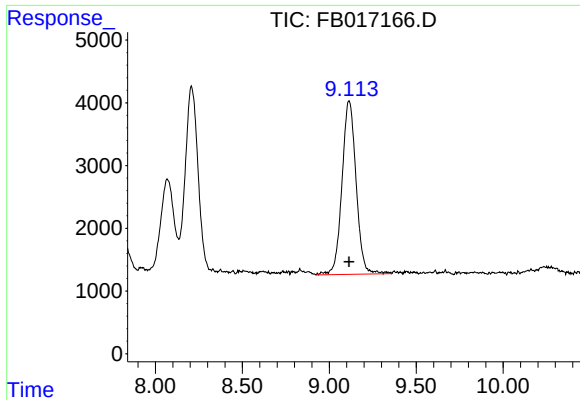


#5 AAA-TFT

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 155881
Conc: 19.70 ng/ml

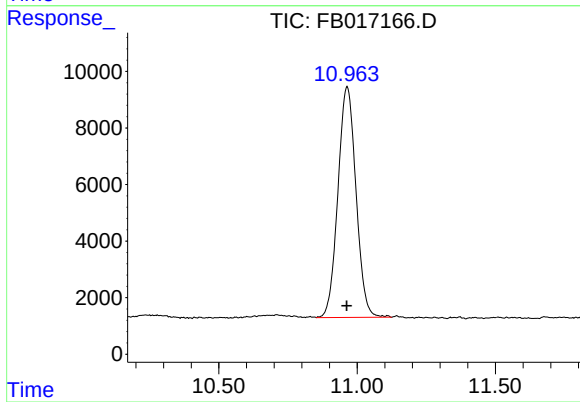


#6 Toluene

R.T.: 10.964 min
Delta R.T.: 0.002 min
Response: 370471
Conc: 26.98 ng/ml

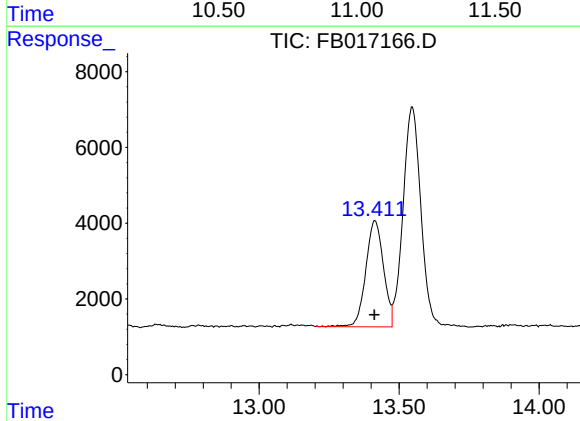


#7 Ethylbenzene

R.T.: 13.414 min
Delta R.T.: 0.002 min
Response: 122391
Conc: 8.98 ng/ml

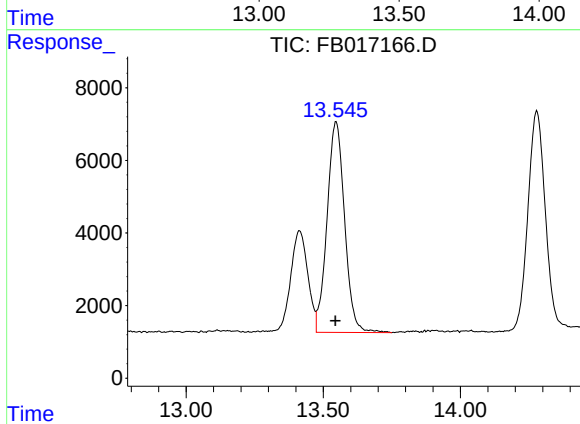


#8 m-Xylene

R.T.: 13.547 min
Delta R.T.: 0.002 min
Response: 258212
Conc: 17.95 ng/ml

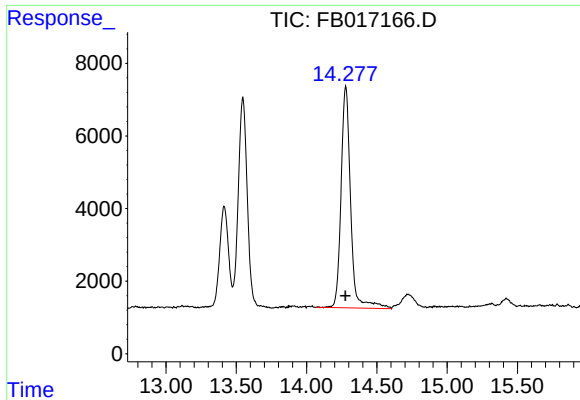

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.003 min
Response: 288251
Conc: 18.90 ng/ml

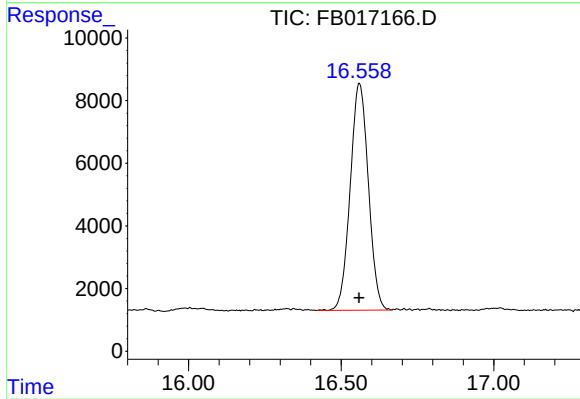

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.002 min
Response: 299493
Conc: 16.23 ng/ml