

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
Data File : FB021927.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2019 9:50
Operator : DD/AJ
Sample : BSF0806S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 14:40:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	273427	20.036 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.863	898233	32.573 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	837919	31.698 ng/ml
3) t	n-Heptane	7.952	260493	10.506 ng/ml
4) t	Benzene	8.087	298928	10.232 ng/ml
6) t	Toluene	10.833	630325	30.634 ng/ml
7) t	Ethylbenzene	13.279	215278	10.348 ng/ml
8) t	m-Xylene	13.412	459424	20.681 ng/ml
9) t	O-Xylene	14.141	476102	20.698 ng/ml
10) t	1,2,4-Trimethylbenzene	16.420	490342	20.798 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
Data File : FB021927.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2019 9:50
Operator : DD/AJ
Sample : BSF0806S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 14:40:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

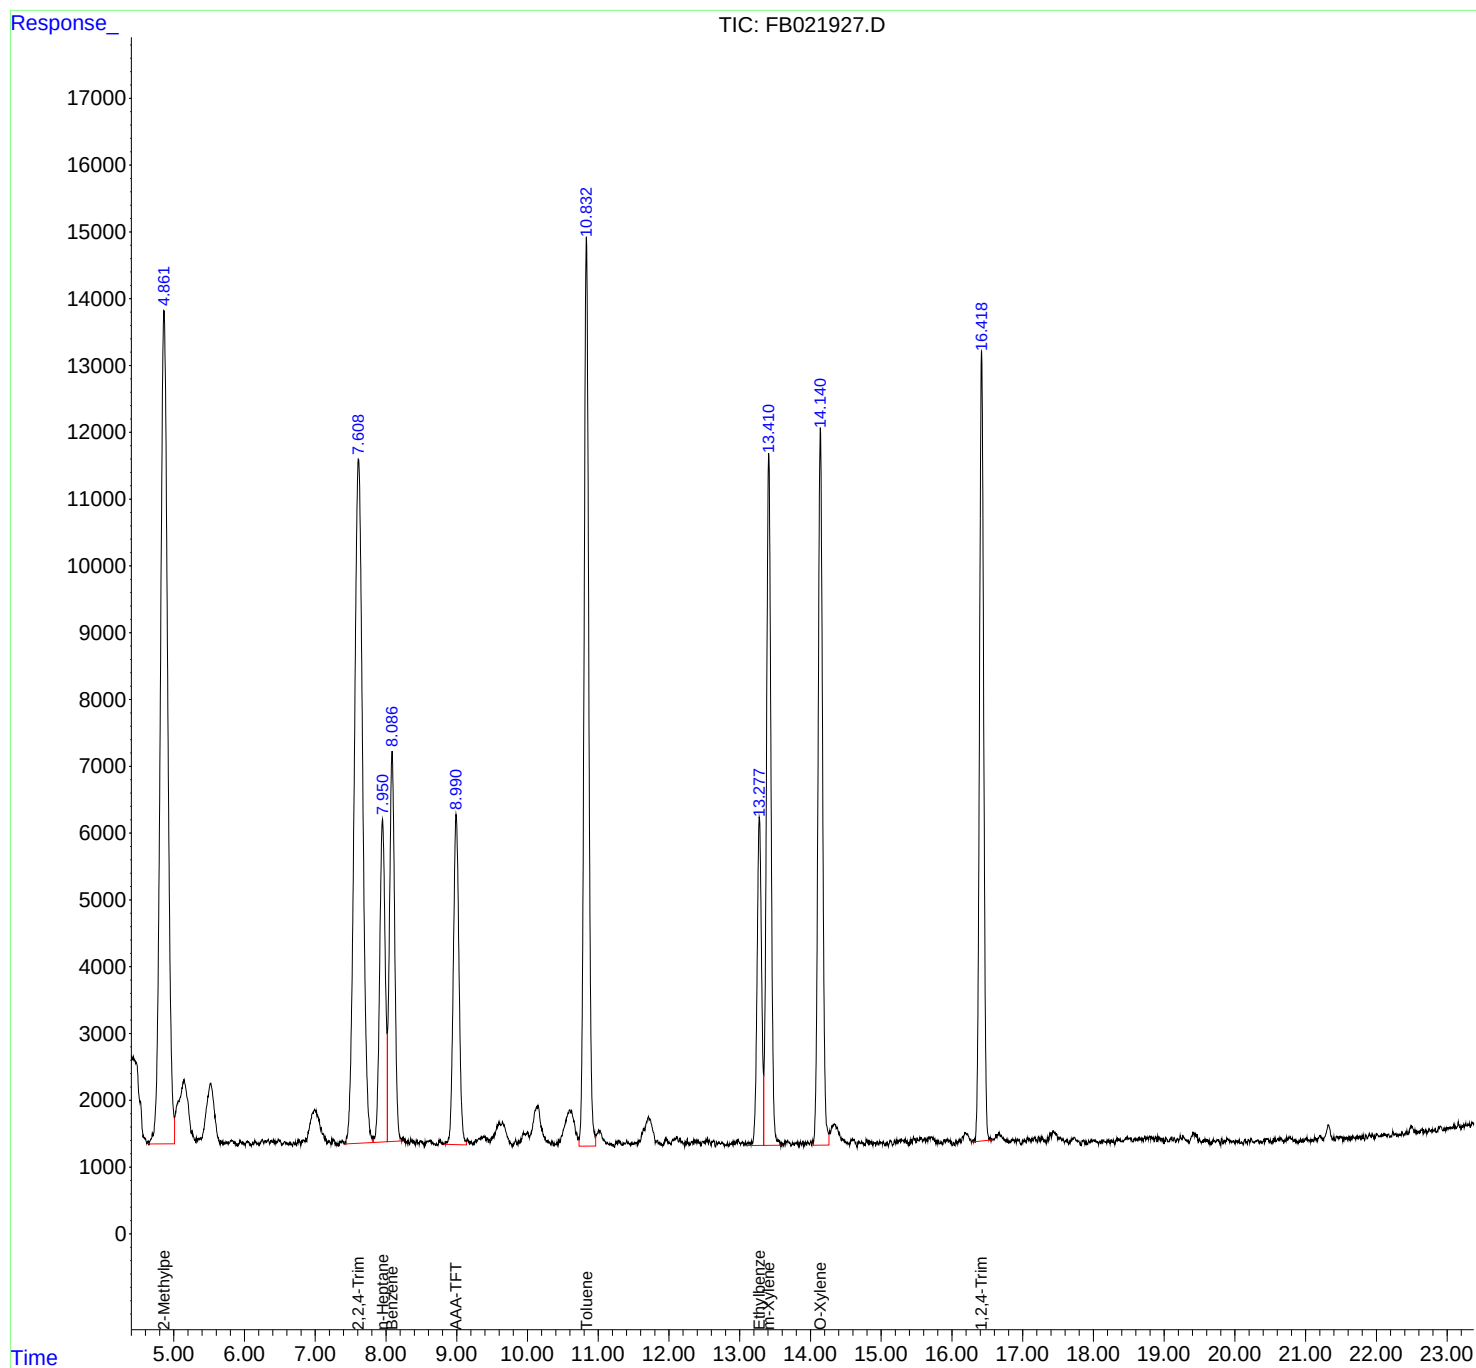

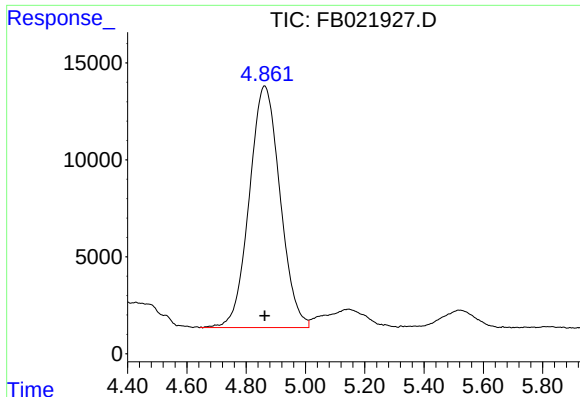


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 898233
Conc: 32.57 ng/ml

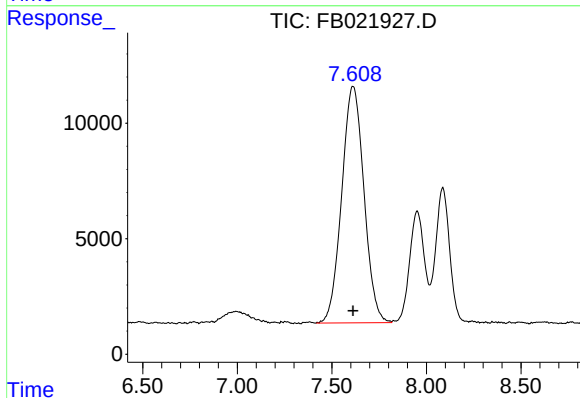


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 837919
Conc: 31.70 ng/ml

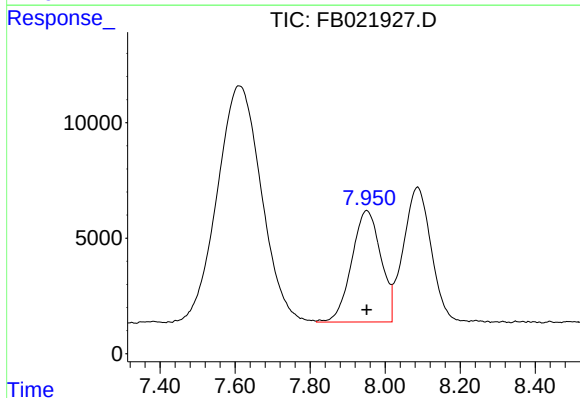


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 260493
Conc: 10.51 ng/ml

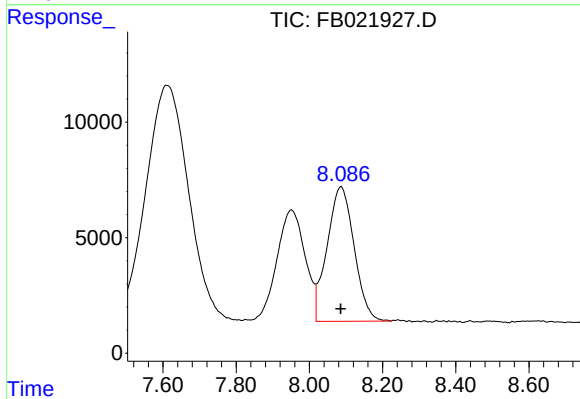


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 298928
Conc: 10.23 ng/ml

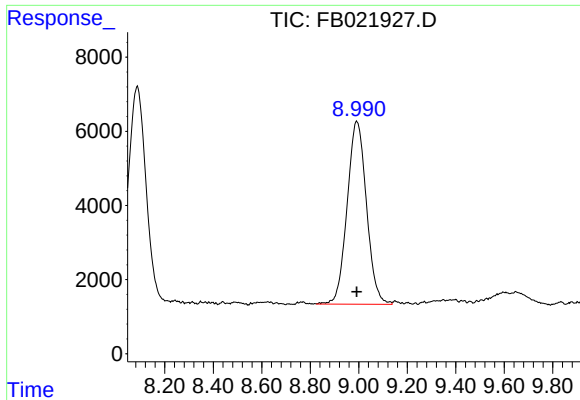


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 273427
Conc: 20.04 ng/ml

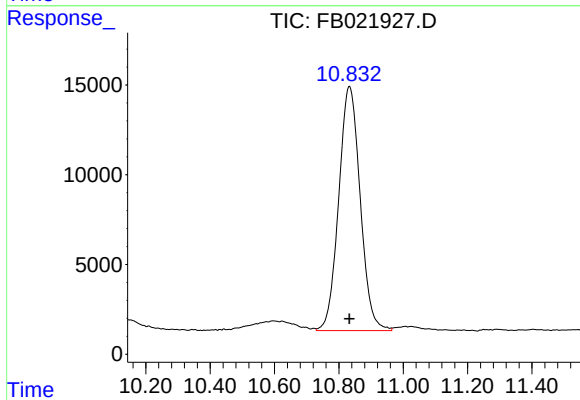


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 630325
Conc: 30.63 ng/ml

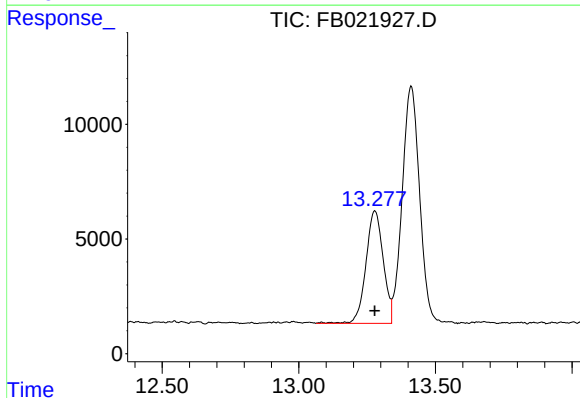


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: 0.001 min
Response: 215278
Conc: 10.35 ng/ml

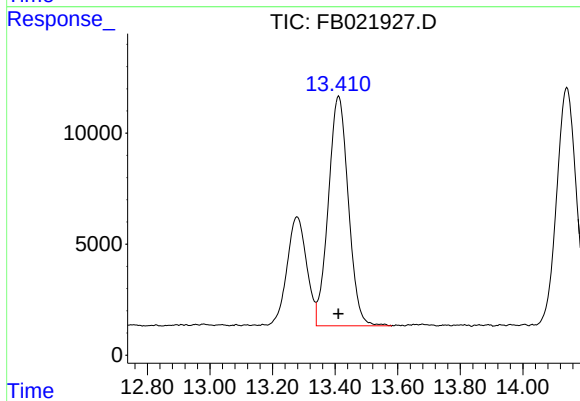

#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.000 min
Response: 459424
Conc: 20.68 ng/ml

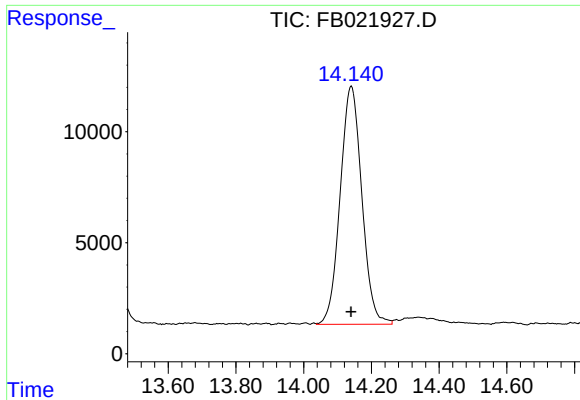


#9 O-Xylene

R.T.: 14.141 min

Delta R.T.: 0.000 min

Response: 476102

Conc: 20.70 ng/ml

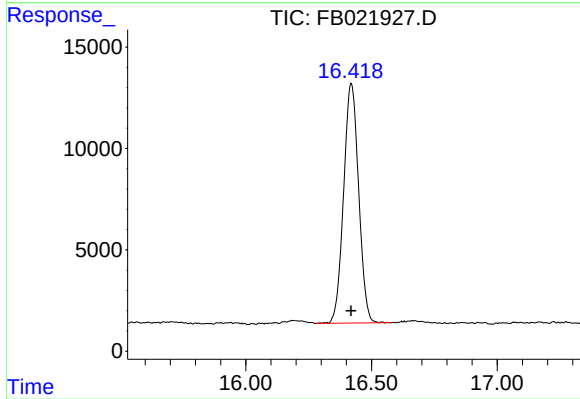

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min

Delta R.T.: 0.000 min

Response: 490342

Conc: 20.80 ng/ml