

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
 Data File : FB021929.D
 Signal(s) : FID2B.CH
 Acq On : 6 Aug 2019 11:58
 Operator : DD/AJ
 Sample : K4162-02MS
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 14:40:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	306585	22.466 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	687180	24.919 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	691144	26.146 ng/ml
3) t n-Heptane	7.952	202819	8.180 ng/ml
4) t Benzene	8.087	284749	9.747 ng/ml
6) t Toluene	10.834	578927	28.136 ng/ml
7) t Ethylbenzene	13.279	183934	8.841 ng/ml
8) t m-Xylene	13.411	391104	17.605 ng/ml
9) t O-Xylene	14.140	413923	17.995 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	404335	17.150 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
Data File : FB021929.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2019 11:58
Operator : DD/AJ
Sample : K4162-02MS
Misc : 5.01/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 14:40:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

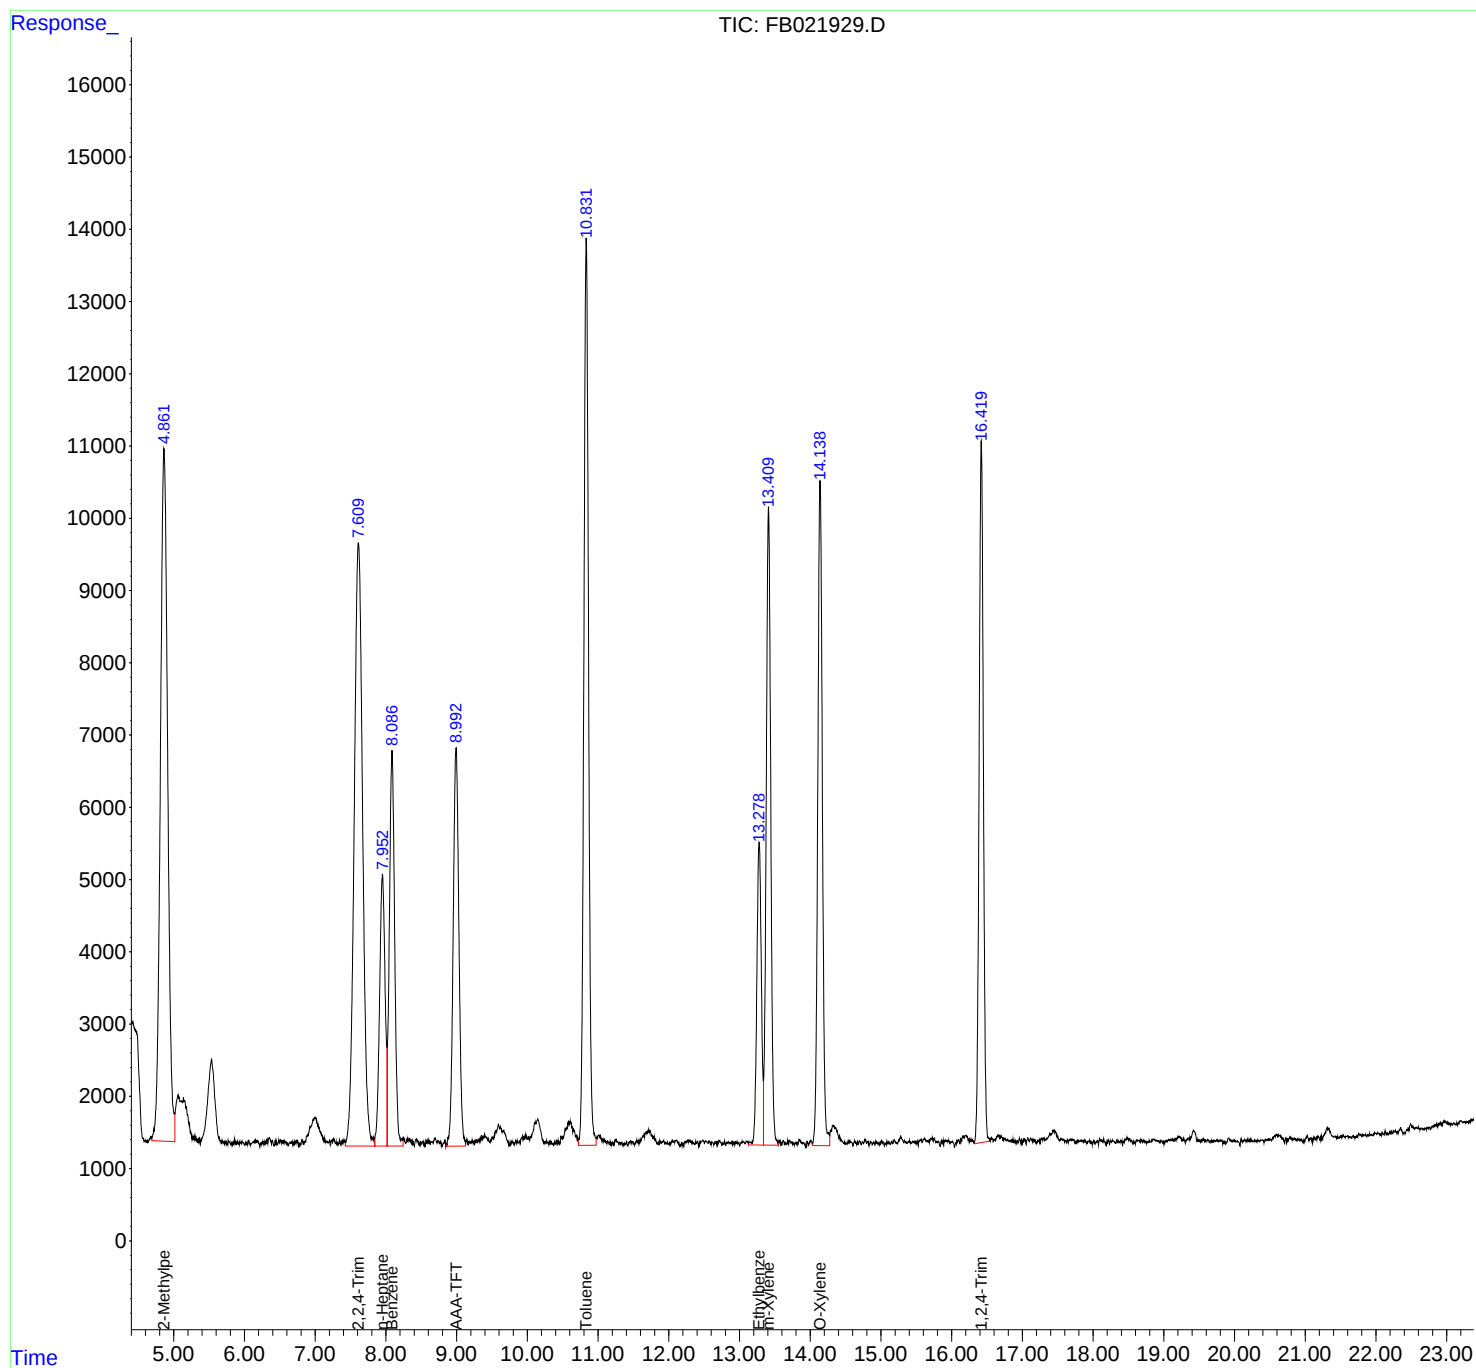

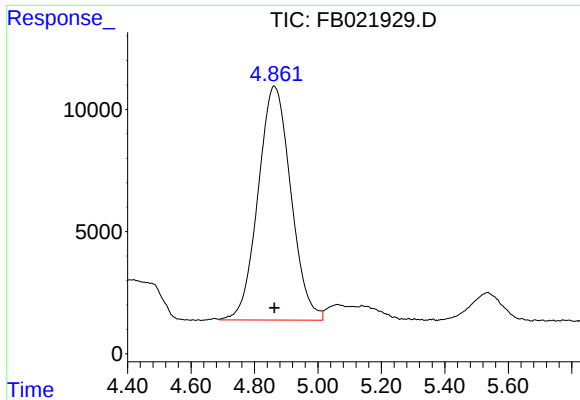


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 687180
Conc: 24.92 ng/ml

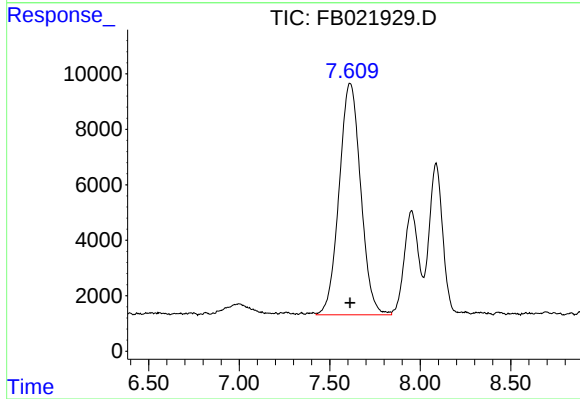


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 691144
Conc: 26.15 ng/ml

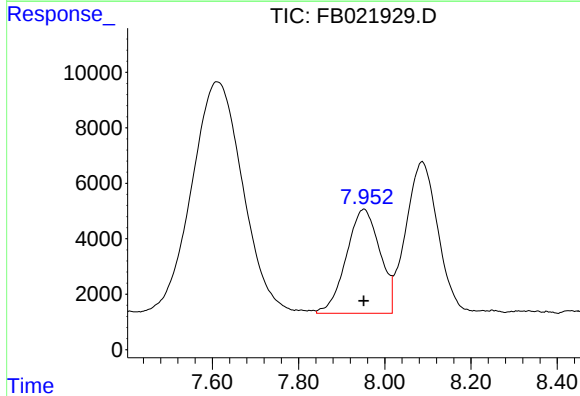


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 202819
Conc: 8.18 ng/ml

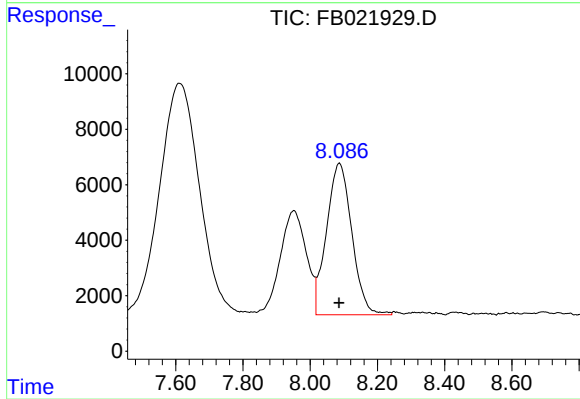


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.001 min
Response: 284749
Conc: 9.75 ng/ml

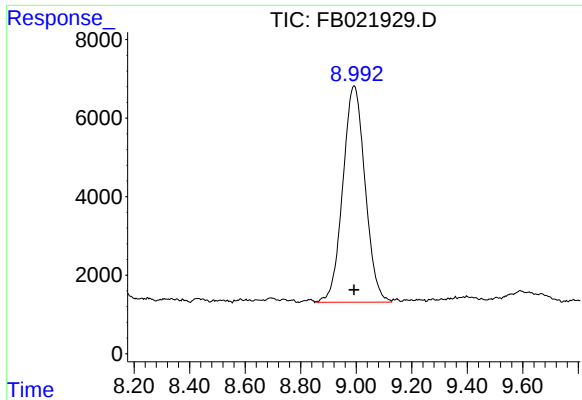


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 306585
Conc: 22.47 ng/ml

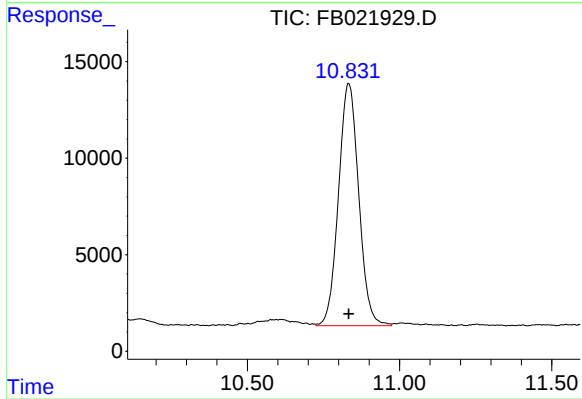


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 578927
Conc: 28.14 ng/ml

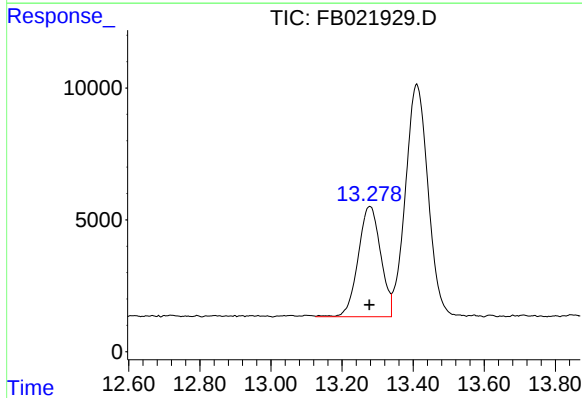


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: 0.000 min
Response: 183934
Conc: 8.84 ng/ml

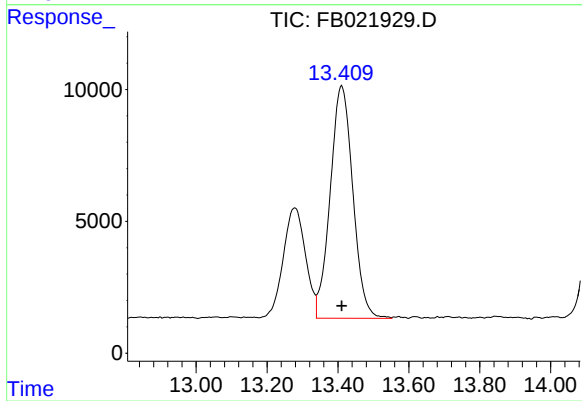


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 391104
Conc: 17.61 ng/ml

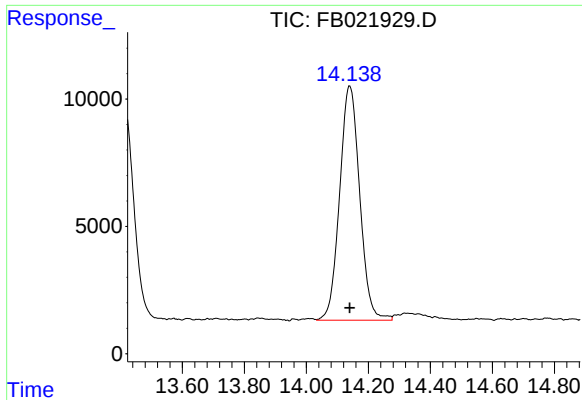

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 413923
Conc: 17.99 ng/ml

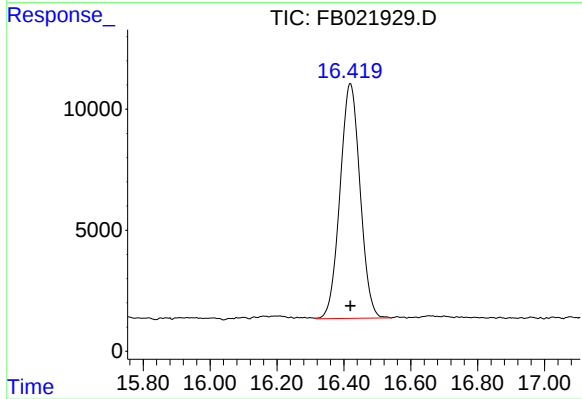

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 404335
Conc: 17.15 ng/ml