

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
 Data File : FB021930.D
 Signal(s) : FID2B.CH
 Acq On : 6 Aug 2019 12:29
 Operator : DD/AJ
 Sample : K4162-02MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 06 14:40:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	293494	21.507 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	635639	23.050 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	630348	23.846 ng/ml
3) t	n-Heptane	7.951	187967	7.581 ng/ml
4) t	Benzene	8.086	273350	9.357 ng/ml
6) t	Toluene	10.833	549881	26.724 ng/ml
7) t	Ethylbenzene	13.278	176929	8.504 ng/ml
8) t	m-Xylene	13.411	368068	16.568 ng/ml
9) t	O-Xylene	14.141	390495	16.976 ng/ml
10) t	1,2,4-Trimethylbenzene	16.420	369163	15.658 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
Data File : FB021930.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2019 12:29
Operator : DD/AJ
Sample : K4162-02MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 14:40:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

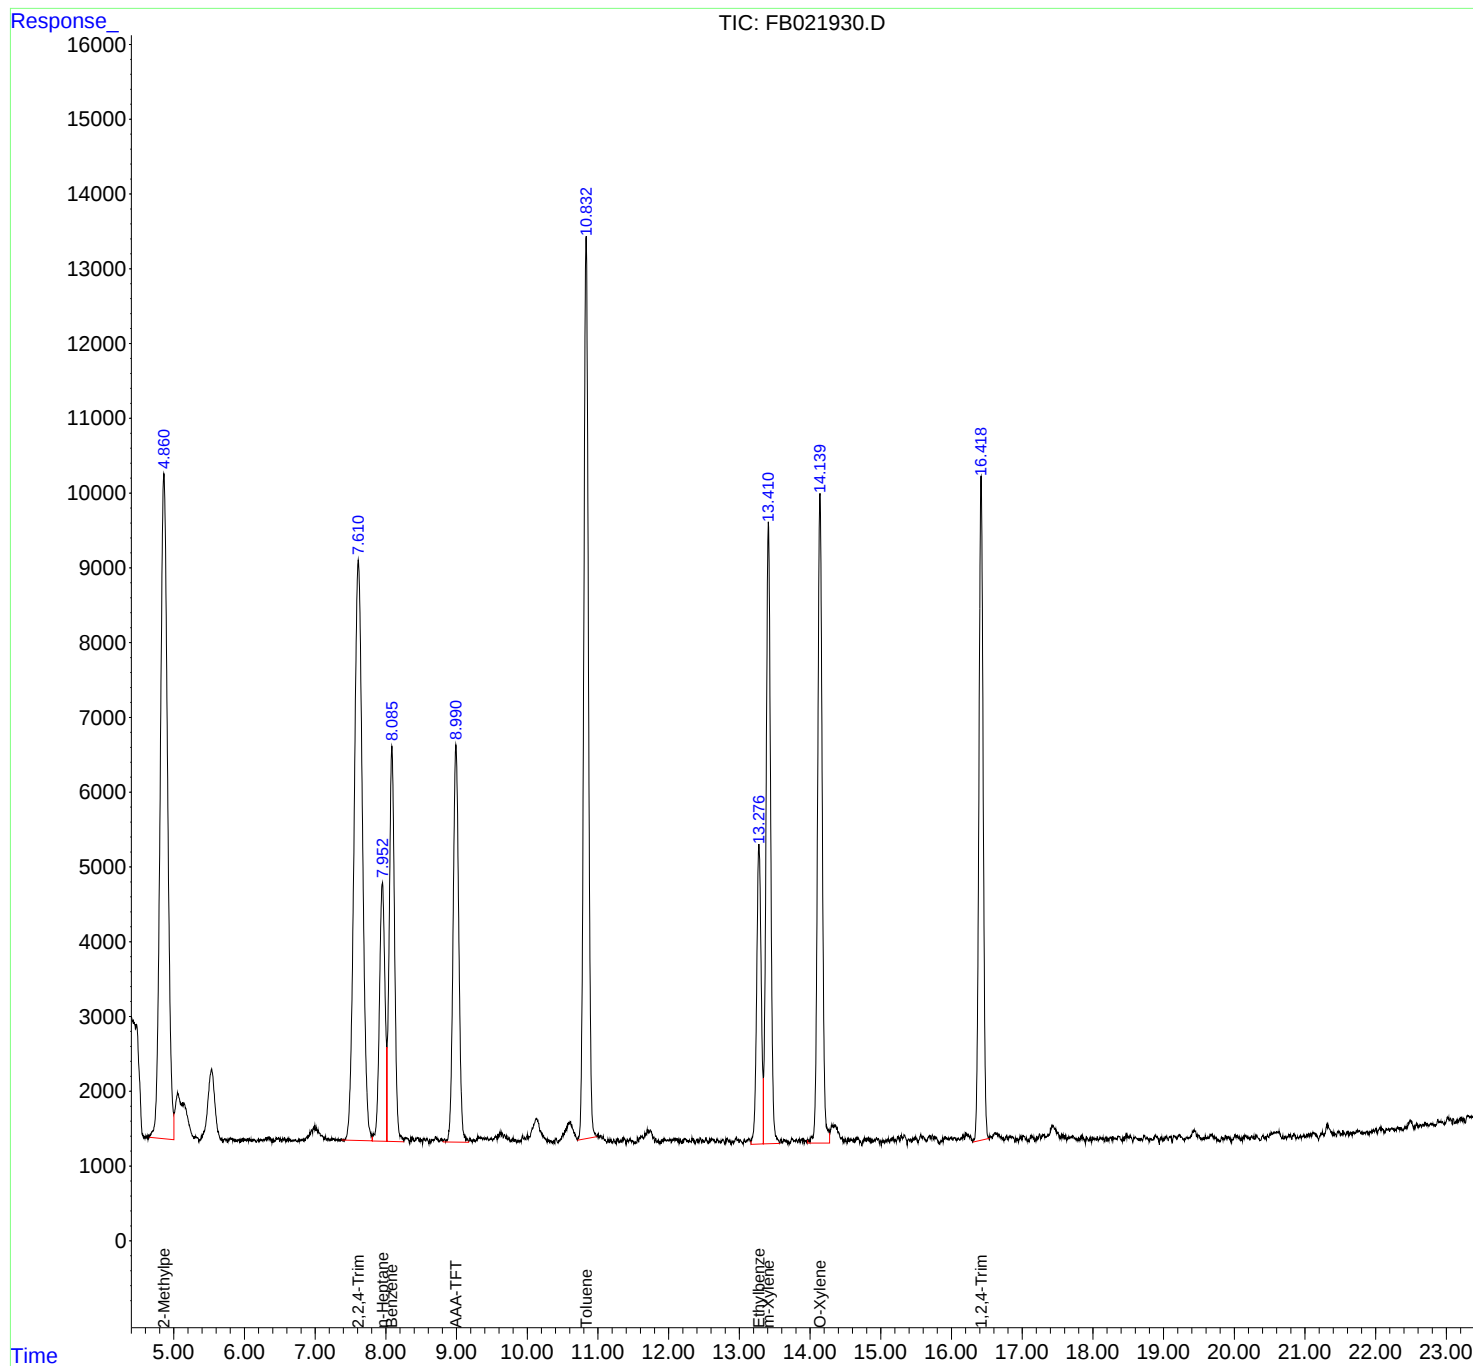

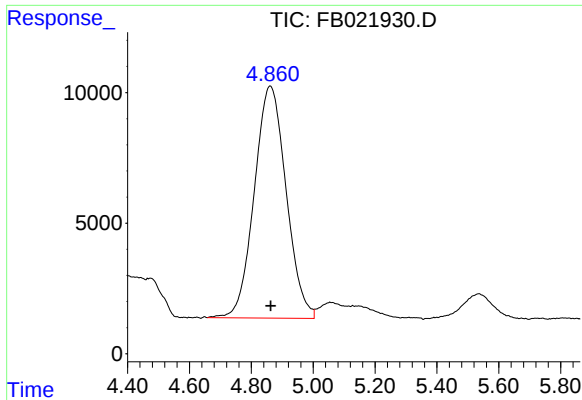


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 635639
Conc: 23.05 ng/ml

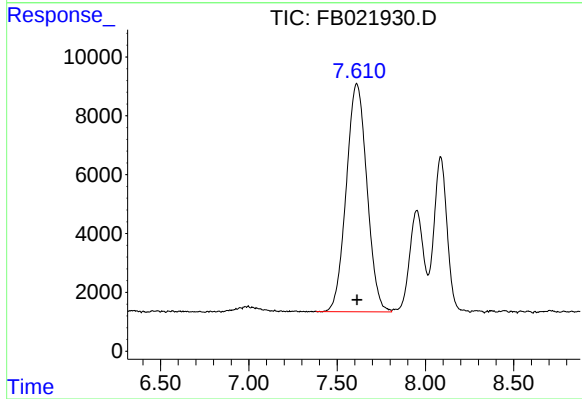


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 630348
Conc: 23.85 ng/ml

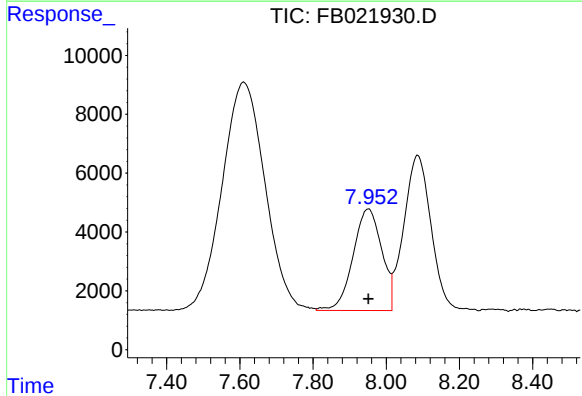


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 187967
Conc: 7.58 ng/ml

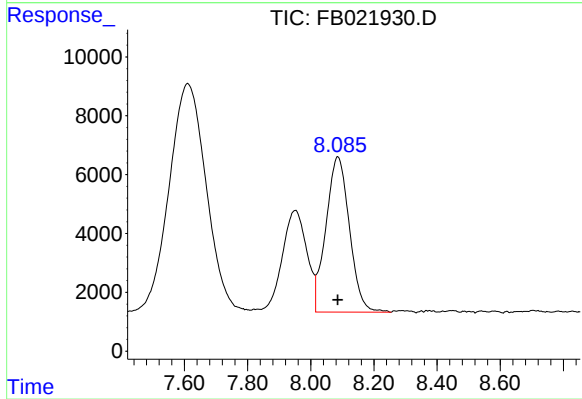


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 273350
Conc: 9.36 ng/ml

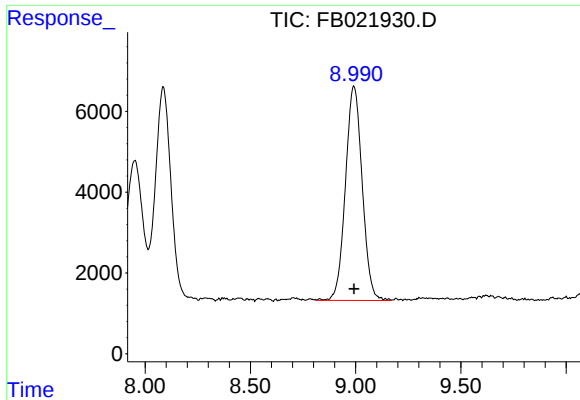


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 293494
Conc: 21.51 ng/ml

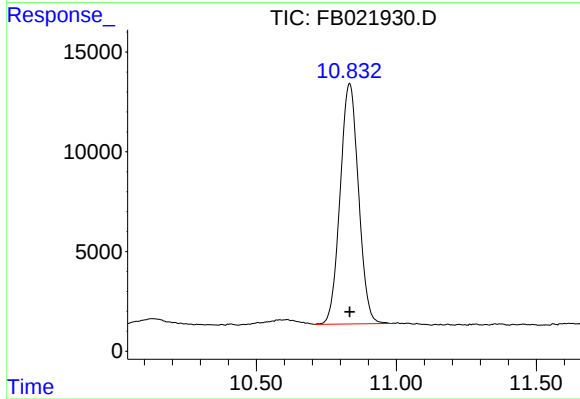


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 549881
Conc: 26.72 ng/ml

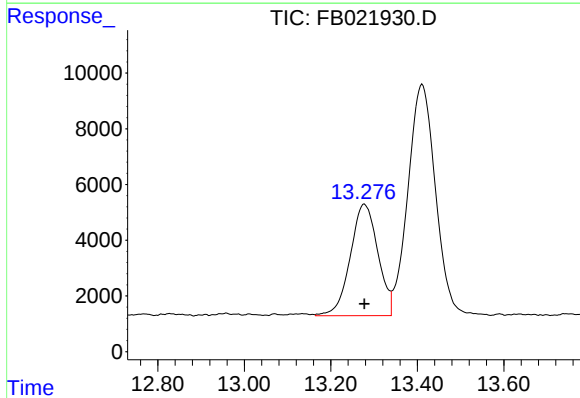


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 176929
Conc: 8.50 ng/ml

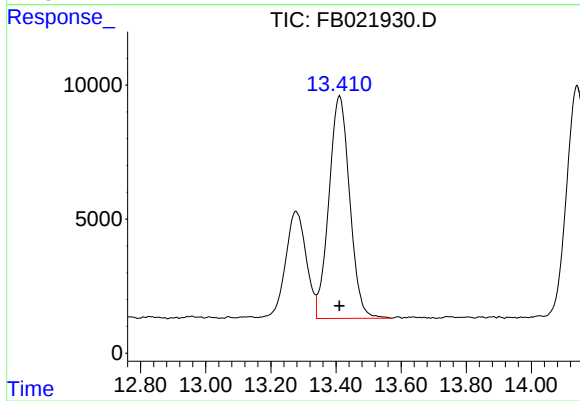


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 368068
Conc: 16.57 ng/ml

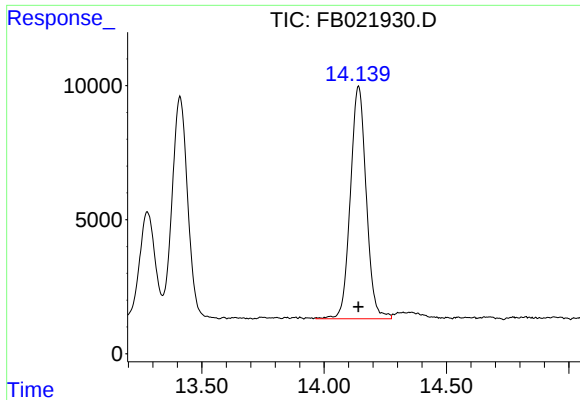

#9 O-Xylene

R.T.: 14.141 min
Delta R.T.: 0.000 min
Response: 390495
Conc: 16.98 ng/ml

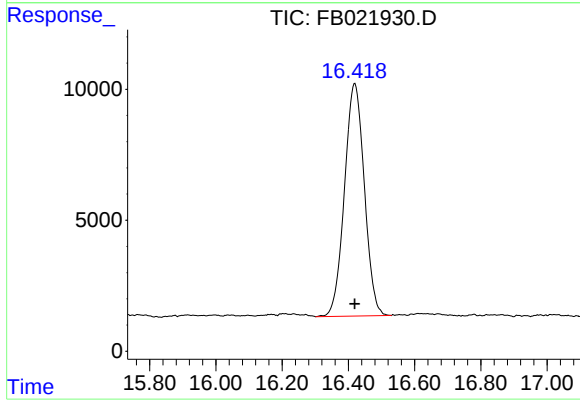

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.000 min
Response: 369163
Conc: 15.66 ng/ml