

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
Data File : FB021935.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2019 15:02
Operator : DD/AJ
Sample : K4156-02
Misc : 5.91/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 17:06:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	305877	22.414 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	7128	0.258 ng/ml
6) t Toluene	10.877	2530	0.123 ng/ml
8) t m-Xylene	13.413	2389	0.108 ng/ml
9) t O-Xylene	14.143	3371	0.147 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080619\
Data File : FB021935.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2019 15:02
Operator : DD/AJ
Sample : K4156-02
Misc : 5.91/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 06 17:06:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

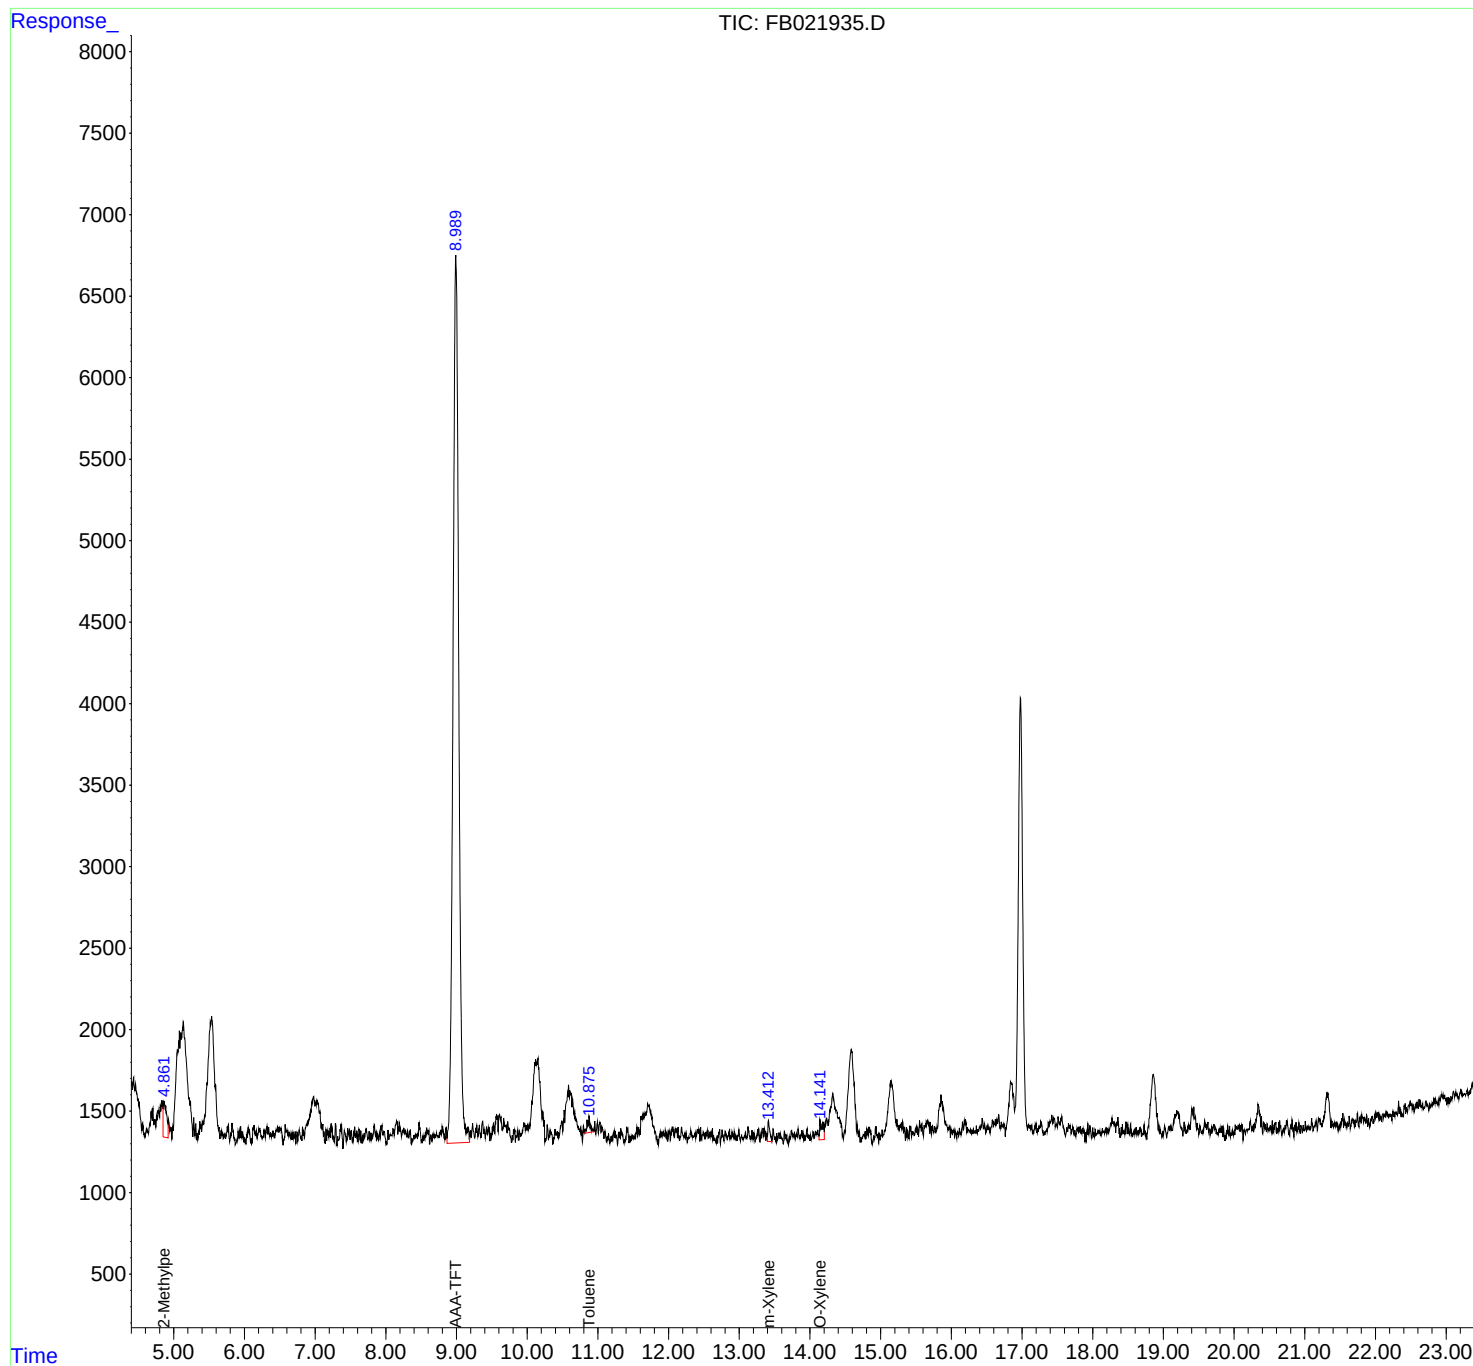

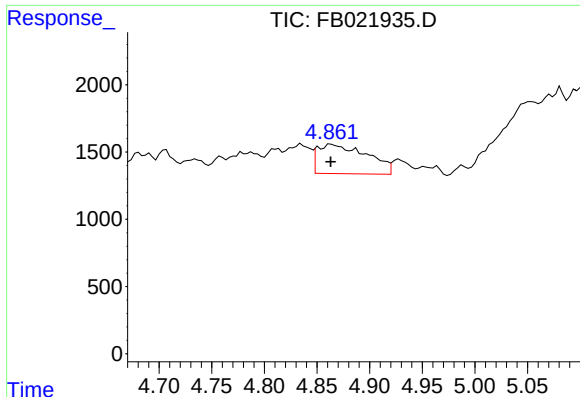


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 7128
Conc: 0.26 ng/ml

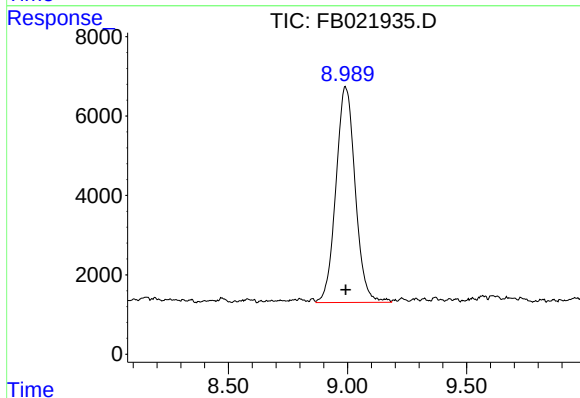


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.002 min
Response: 305877
Conc: 22.41 ng/ml

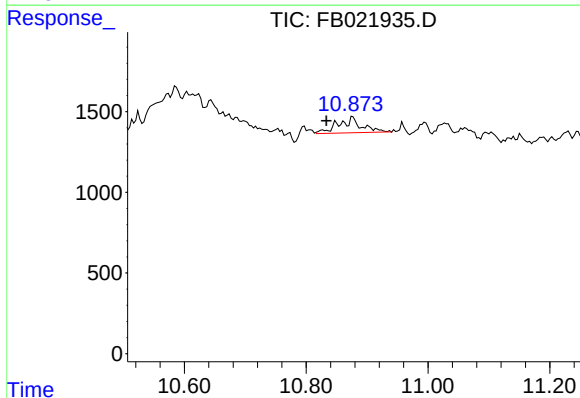


#6 Toluene

R.T.: 10.877 min
Delta R.T.: 0.044 min
Response: 2530
Conc: 0.12 ng/ml

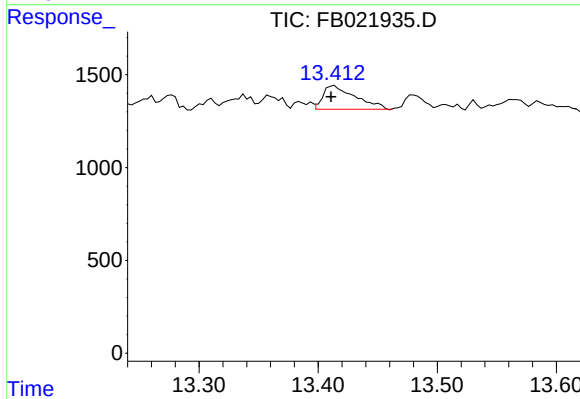

#8 m-Xylene

R.T.: 13.413 min
Delta R.T.: 0.003 min
Response: 2389
Conc: 0.11 ng/ml

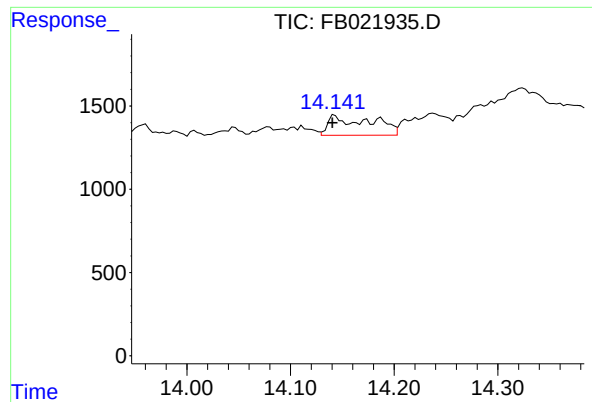

#9 O-Xylene

R.T.: 14.143 min
Delta R.T.: 0.003 min
Response: 3371
Conc: 0.15 ng/ml