

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080620\
 Data File : FB024724.D
 Signal(s) : FID2B.CH
 Acq On : 6 Aug 2020 13:28
 Operator : DD/AJ
 Sample : L3553-03MSD
 Misc : 5.07g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 07 02:26:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	522569	22.686 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	828065	27.982 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	821626	26.244 ng/ml
3) t	n-Heptane	7.757	254685	8.191 ng/ml
4) t	Benzene	7.891	389708	10.224 ng/ml
6) t	Toluene	10.629	1060903	29.015 ng/ml
7) t	Ethylbenzene	13.069	318733	9.332 ng/ml
8) t	m-Xylene	13.202	621166	18.407 ng/ml
9) t	O-Xylene	13.929	612368	18.632 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	488059	18.093 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080620\
Data File : FB024724.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2020 13:28
Operator : DD/AJ
Sample : L3553-03MSD
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 07 02:26:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

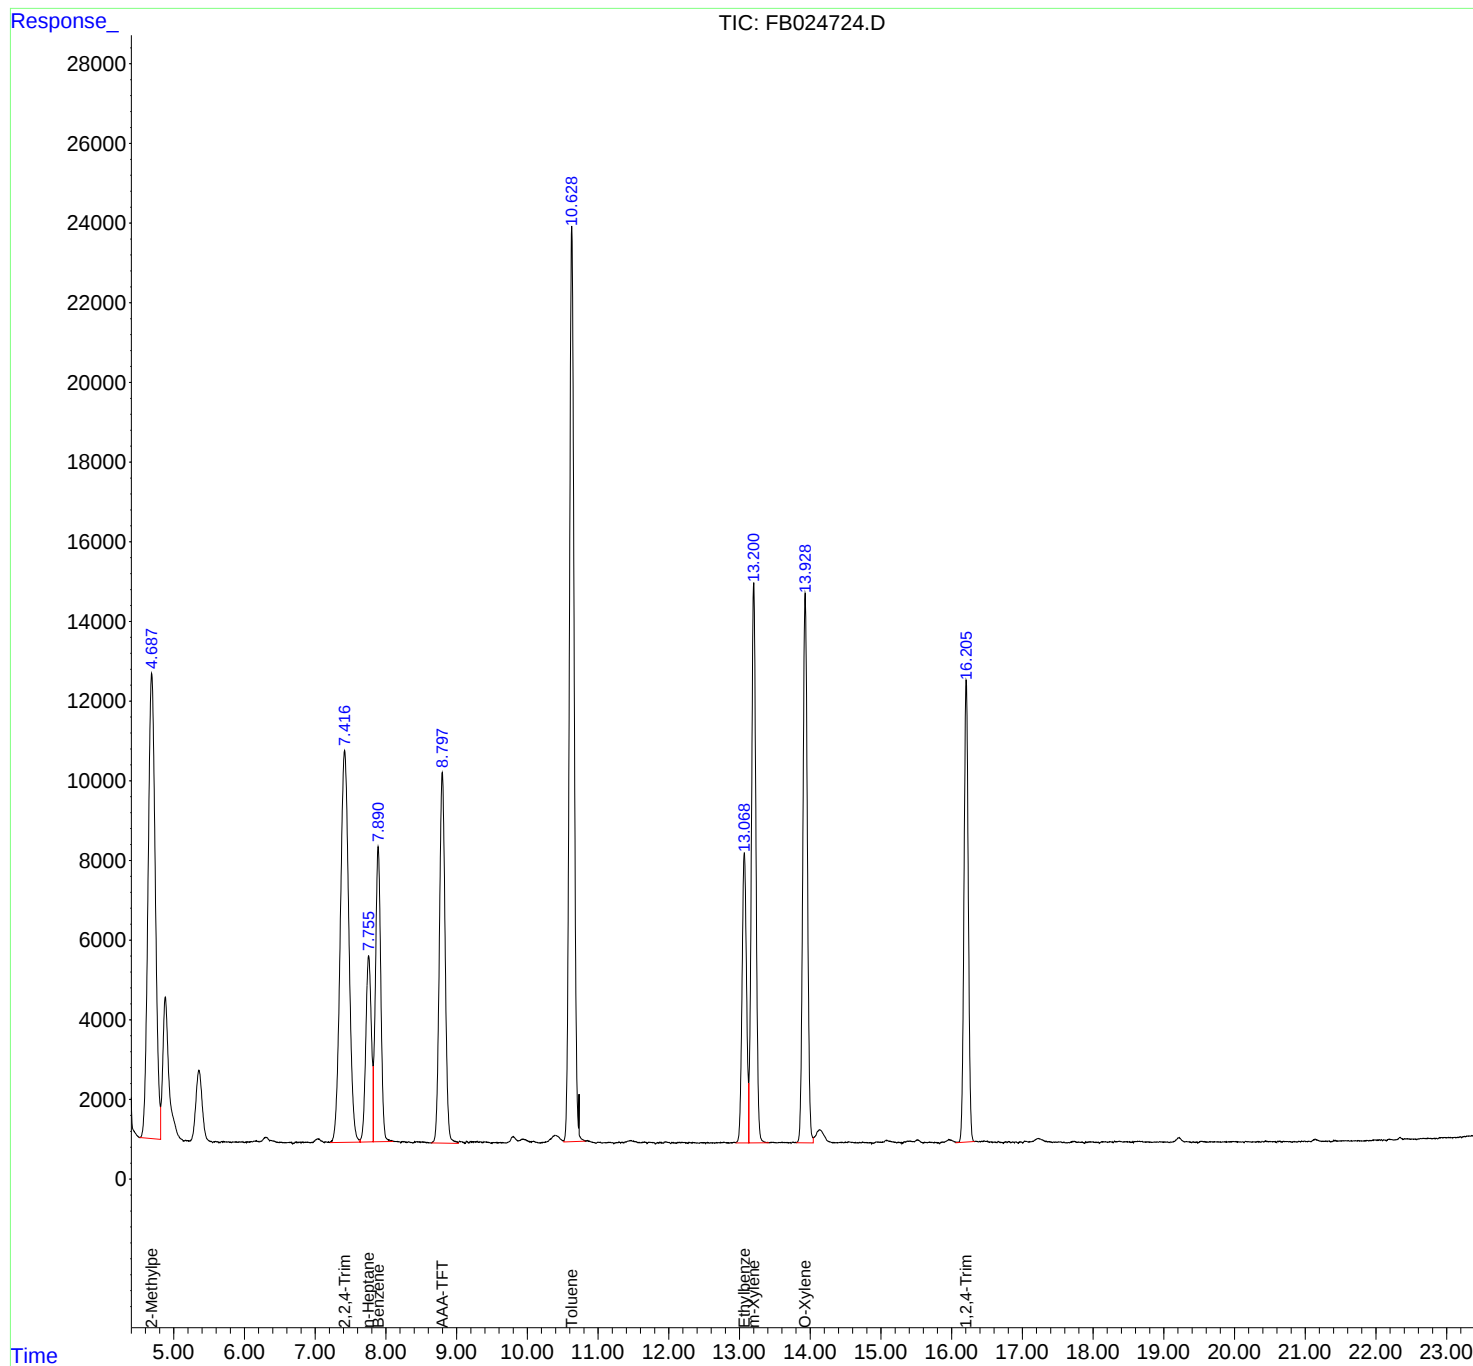


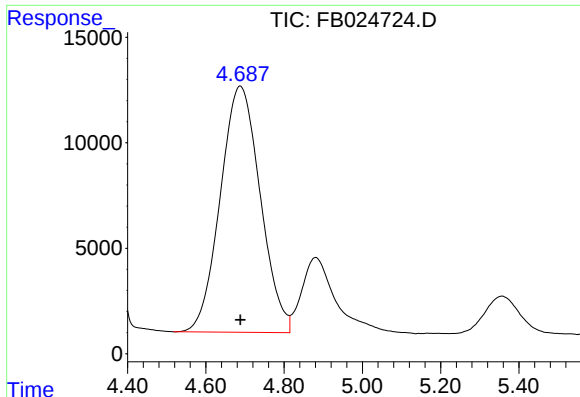

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 828065
Conc: 27.98 ng/ml

Instrument :
FID_B
ClientSampleId :

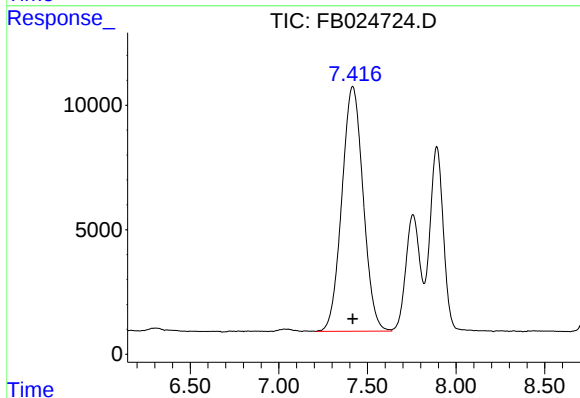


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 821626
Conc: 26.24 ng/ml

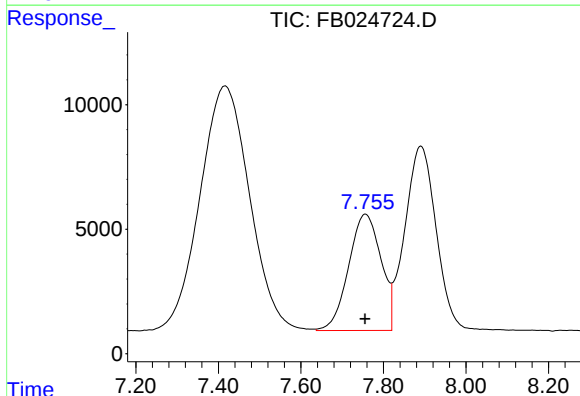


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 254685
Conc: 8.19 ng/ml

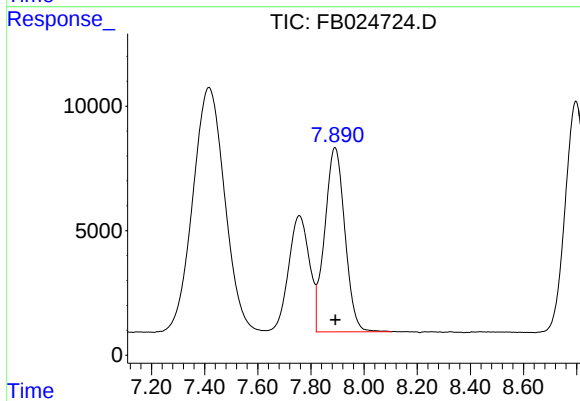

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 389708
Conc: 10.22 ng/ml

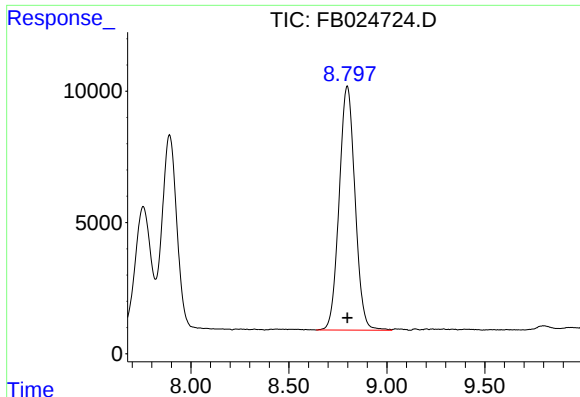

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 522569
Conc: 22.69 ng/ml

Instrument :
FID_B
ClientSampleId :

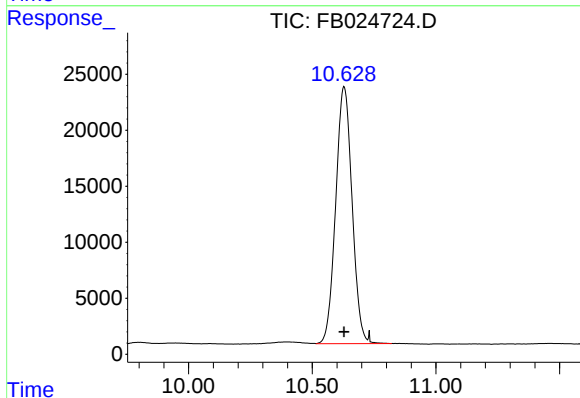


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1060903
Conc: 29.01 ng/ml

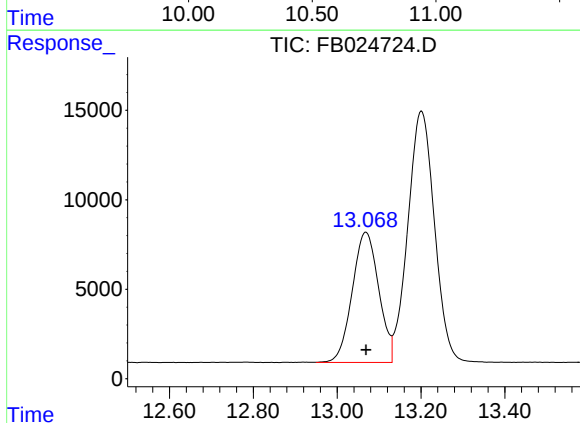


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 318733
Conc: 9.33 ng/ml

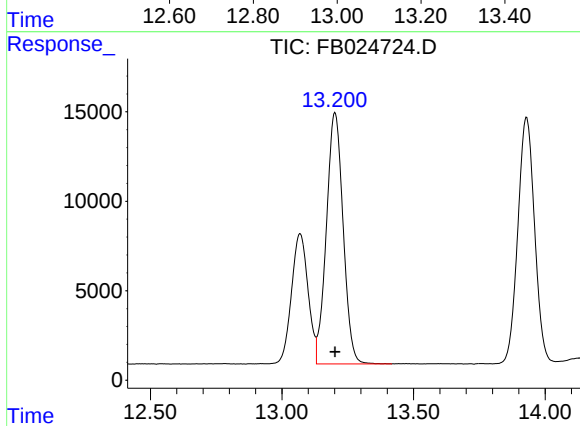

#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 621166
Conc: 18.41 ng/ml

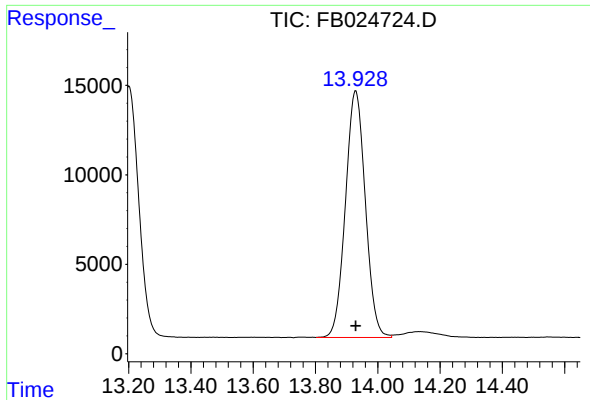

#9 O-Xylene


R.T.: 13.929 min

Delta R.T.: 0.000 min

Response: 612368

Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :

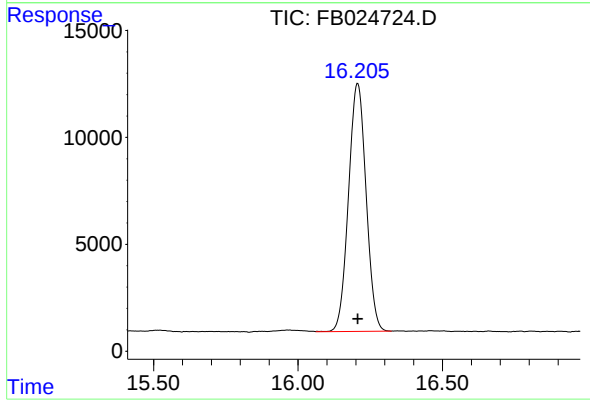

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min

Delta R.T.: 0.000 min

Response: 488059

Conc: 18.09 ng/ml