

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080620\
 Data File : FB024727.D
 Signal(s) : FID2B.CH
 Acq On : 6 Aug 2020 16:29
 Operator : DD/AJ
 Sample : L3508-02
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 07 02:26:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	547981	23.789 ng/ml
Target Compounds			
6) t Toluene	10.628	6243	0.171 ng/ml
8) t m-Xylene	13.198	4102	0.122 ng/ml
9) t O-Xylene	13.937	2097	0.064 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	9330	0.346 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080620\
Data File : FB024727.D
Signal(s) : FID2B.CH
Acq On : 6 Aug 2020 16:29
Operator : DD/AJ
Sample : L3508-02
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 07 02:26:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

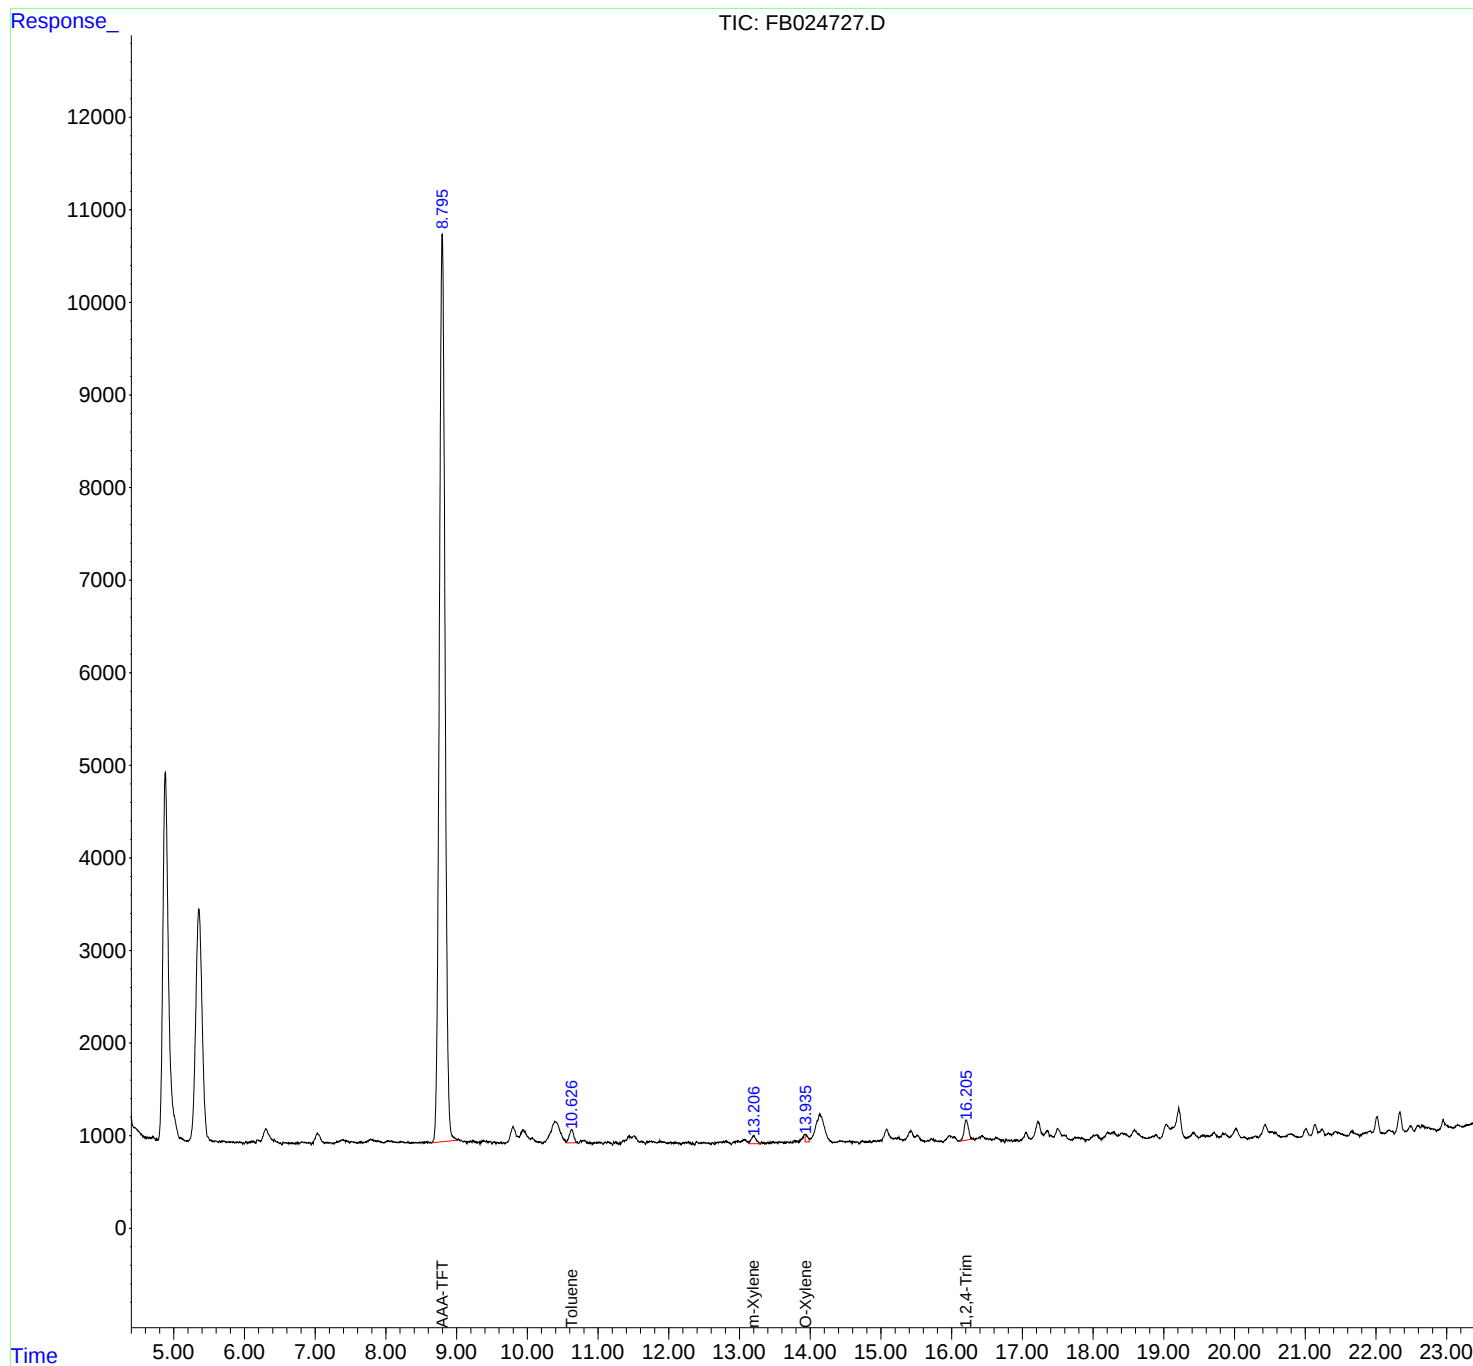


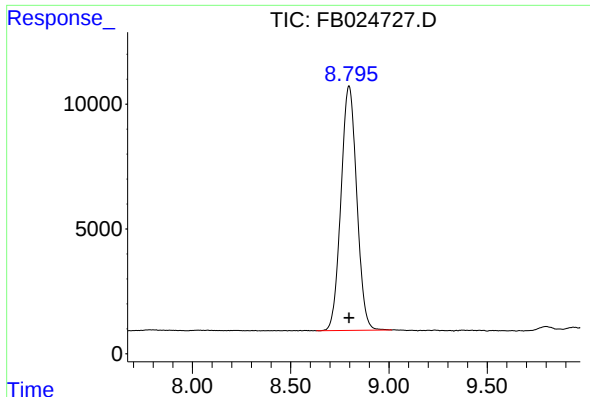

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 547981
Conc: 23.79 ng/ml

Instrument :
FID_B
ClientSampleId :

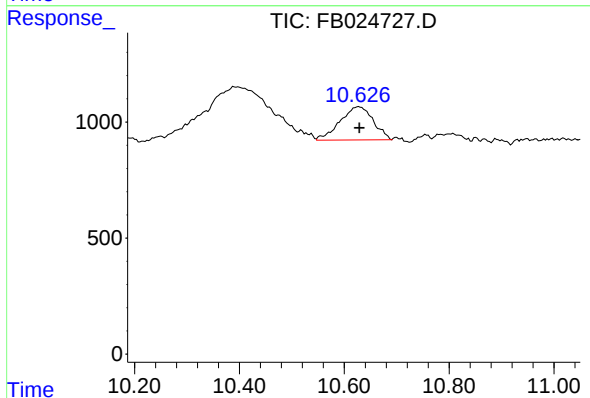


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 6243
Conc: 0.17 ng/ml

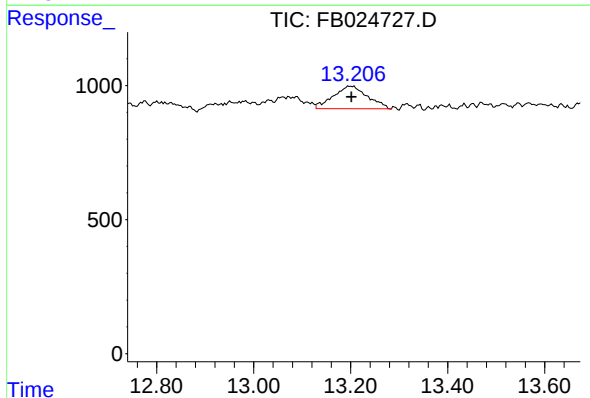


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.003 min
Response: 4102
Conc: 0.12 ng/ml

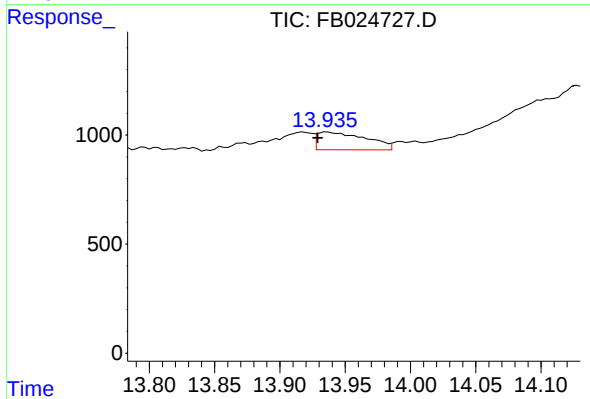

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.008 min
Response: 2097
Conc: 0.06 ng/ml

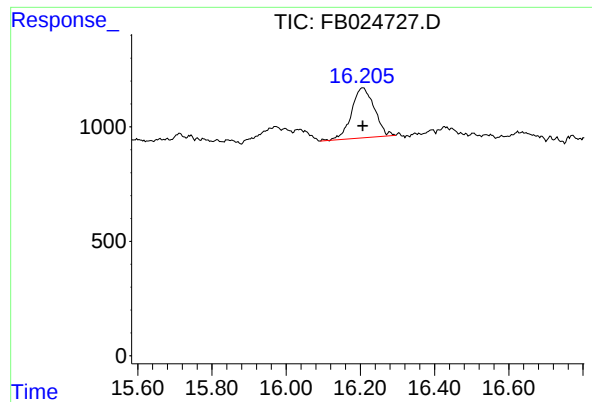

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 9330
Conc: 0.35 ng/ml

Instrument :
FID_B
ClientSampleId :