

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080718\
 Data File : FB017191.D
 Signal(s) : FID2B.CH
 Acq On : 7 Aug 2018 9:18
 Operator : MJ/SJ
 Sample : BSF0807S1
 Misc : 5.03g/5.00ml DI water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 07 15:30:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
 Quant Title :
 QLast Update : Fri Jul 27 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.114	165169	20.870 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	436986	30.273 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	433097	30.960 ng/ml
3) t n-Heptane	8.069	136371	9.698 ng/ml
4) t Benzene	8.208	173560	9.880 ng/ml
6) t Toluene	10.963	423383	30.830 ng/ml
7) t Ethylbenzene	13.413	140987	10.339 ng/ml
8) t m-Xylene	13.545	296602	20.615 ng/ml
9) t O-Xylene	14.277	311364	20.416 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	371159	20.109 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080718\
Data File : FB017191.D
Signal(s) : FID2B.CH
Acq On : 7 Aug 2018 9:18
Operator : MJ/SJ
Sample : BSF0807S1
Misc : 5.03g/5.00ml DI water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 07 15:30:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072718.M
Quant Title :
QLast Update : Fri Jul 27 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

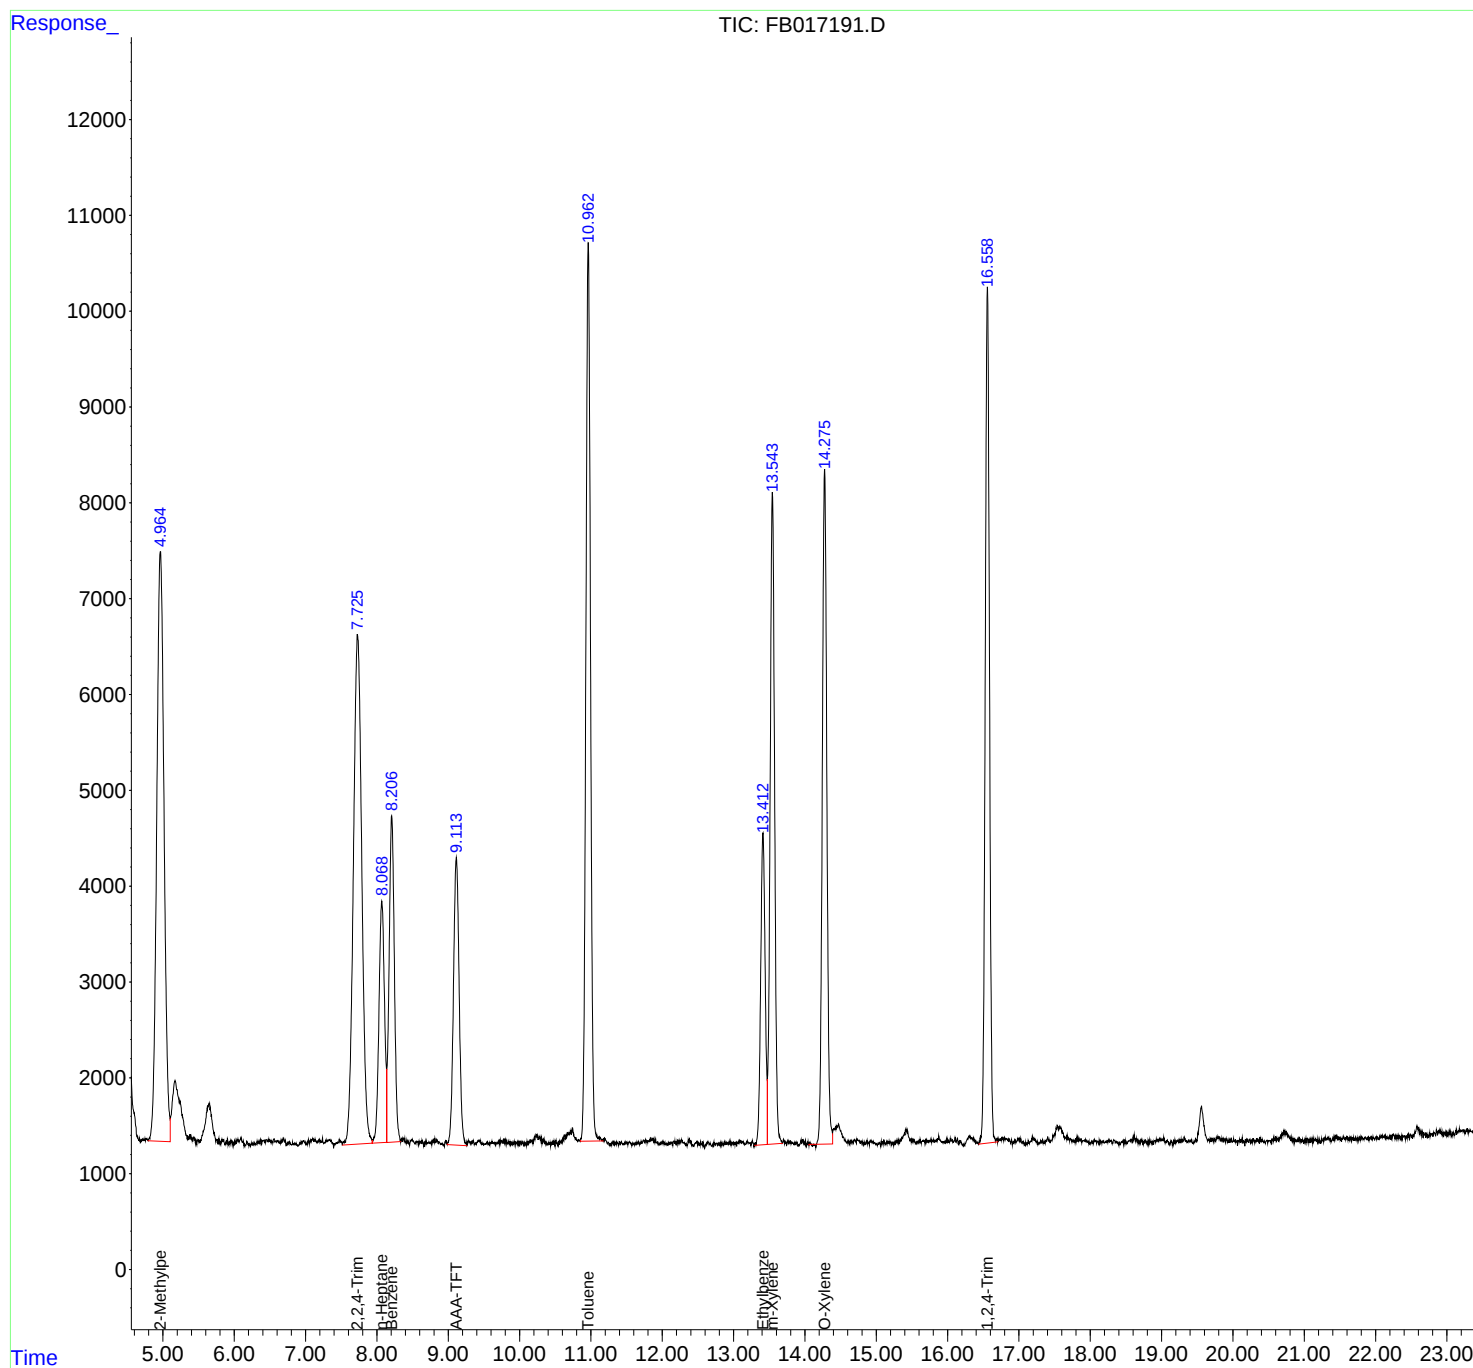

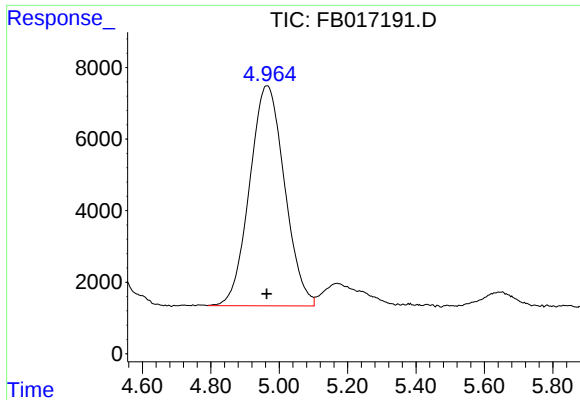


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 436986
Conc: 30.27 ng/ml

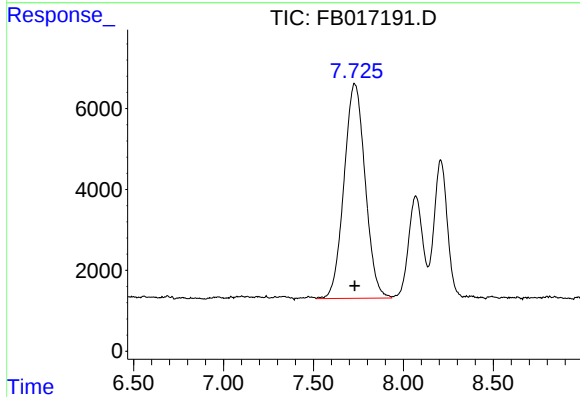


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: -0.001 min
Response: 433097
Conc: 30.96 ng/ml

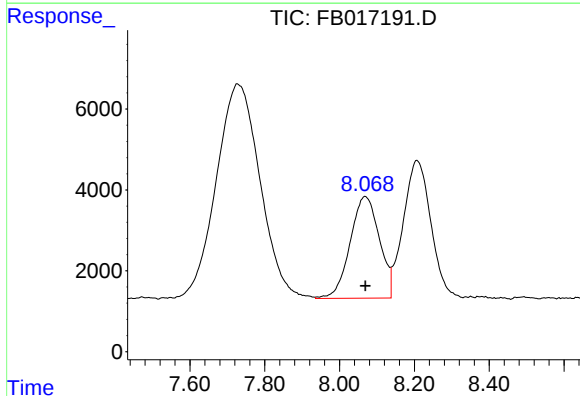


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 136371
Conc: 9.70 ng/ml

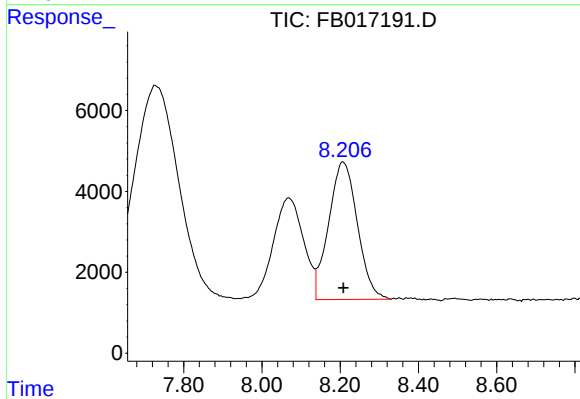


#4 Benzene

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 173560
Conc: 9.88 ng/ml

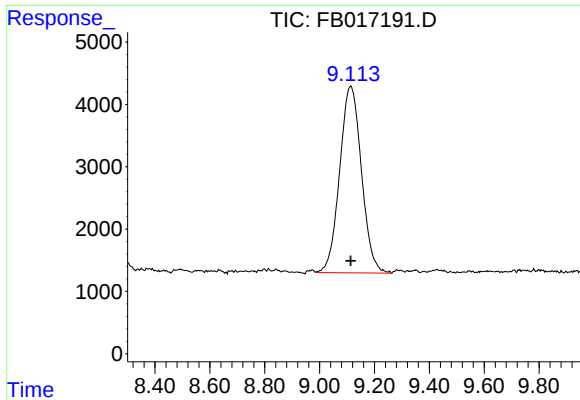


#5 AAA-TFT

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 165169
Conc: 20.87 ng/ml

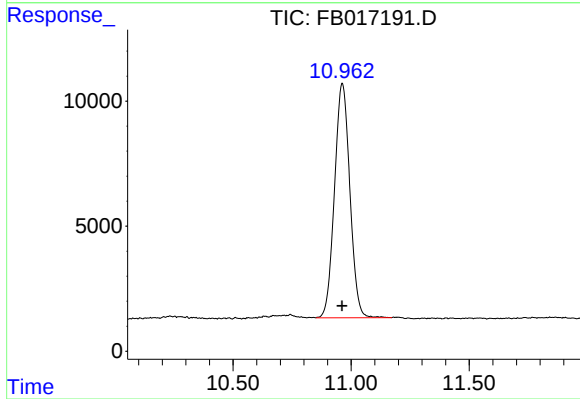


#6 Toluene

R.T.: 10.963 min
Delta R.T.: 0.000 min
Response: 423383
Conc: 30.83 ng/ml

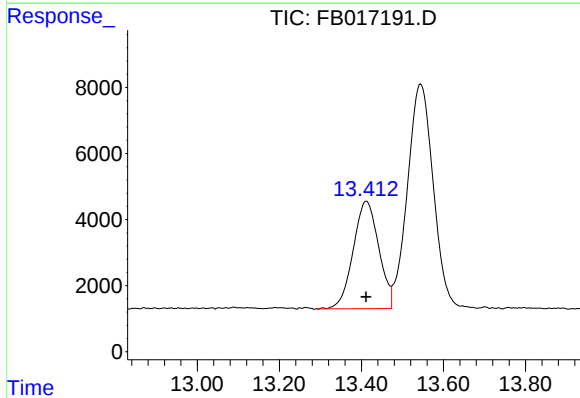


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: 0.000 min
Response: 140987
Conc: 10.34 ng/ml

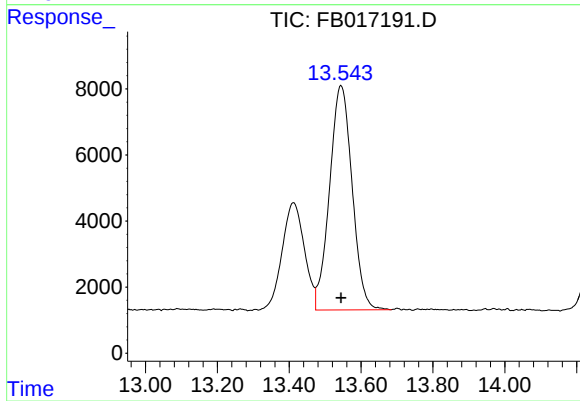


#8 m-Xylene

R.T.: 13.545 min
Delta R.T.: 0.000 min
Response: 296602
Conc: 20.62 ng/ml

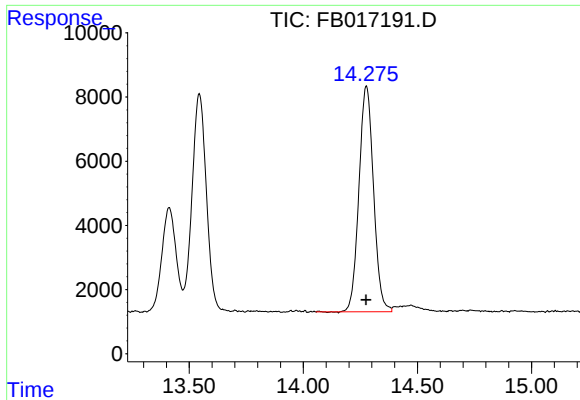

#9 O-Xylene

R.T.: 14.277 min
Delta R.T.: 0.000 min
Response: 311364
Conc: 20.42 ng/ml

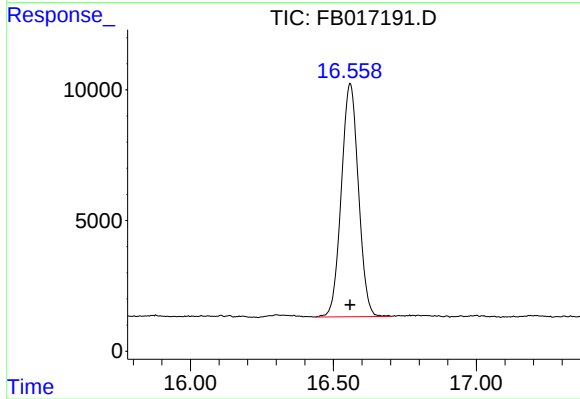

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.000 min
Response: 371159
Conc: 20.11 ng/ml