

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080719\
 Data File : FB021941.D
 Signal(s) : FID2B.CH
 Acq On : 7 Aug 2019 9:48
 Operator : DD/AJ
 Sample : BSF0807S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 08 01:02:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	261073	19.131 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	820516	29.755 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	804122	30.420 ng/ml
3) t n-Heptane	7.950	253269	10.215 ng/ml
4) t Benzene	8.084	296683	10.155 ng/ml
6) t Toluene	10.831	613354	29.809 ng/ml
7) t Ethylbenzene	13.276	213448	10.260 ng/ml
8) t m-Xylene	13.409	457806	20.608 ng/ml
9) t O-Xylene	14.139	477792	20.771 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	483833	20.522 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080719\
Data File : FB021941.D
Signal(s) : FID2B.CH
Acq On : 7 Aug 2019 9:48
Operator : DD/AJ
Sample : BSF0807S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 08 01:02:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

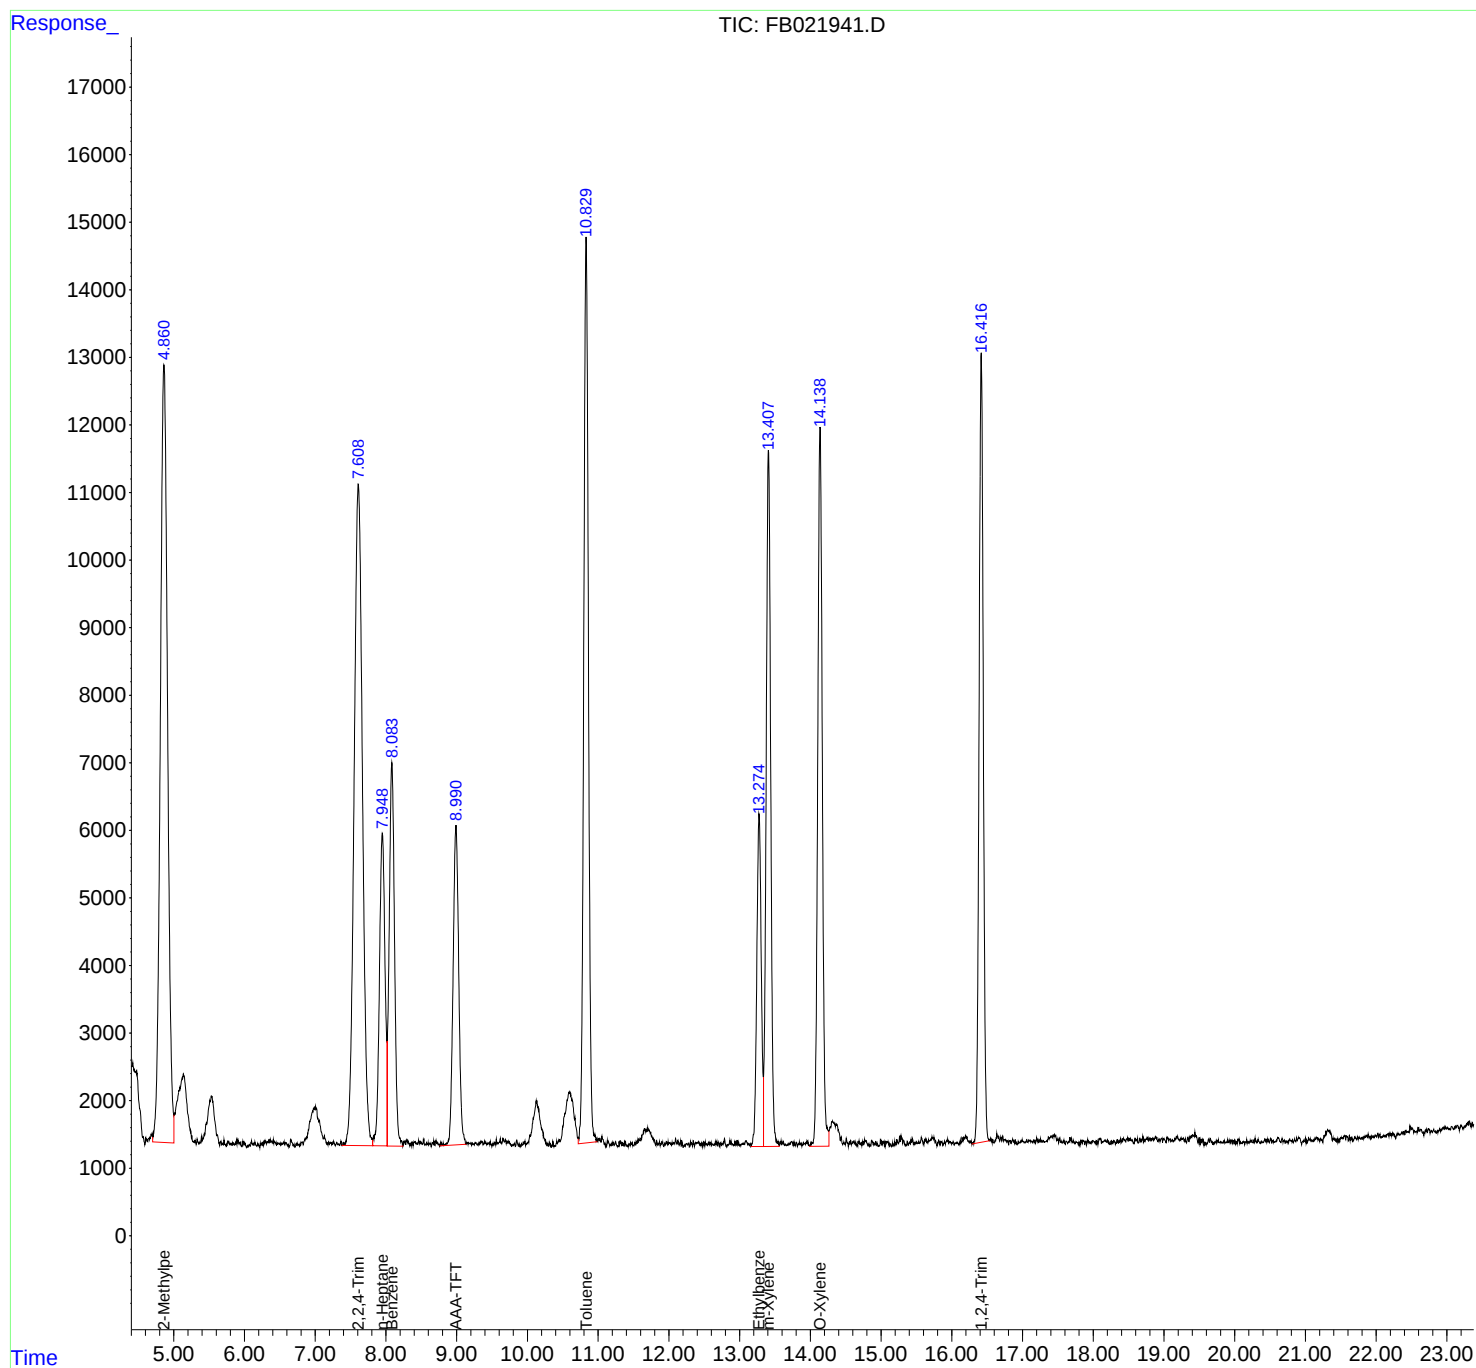

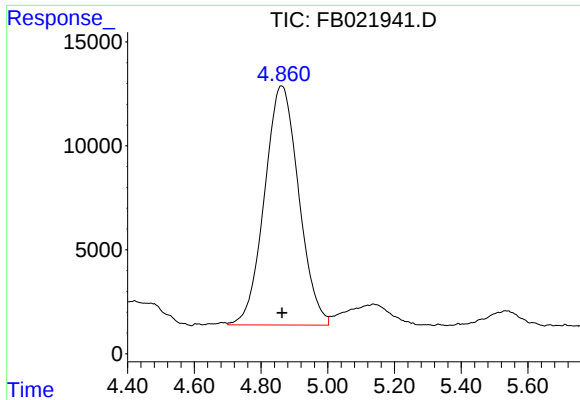


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 820516
Conc: 29.75 ng/ml

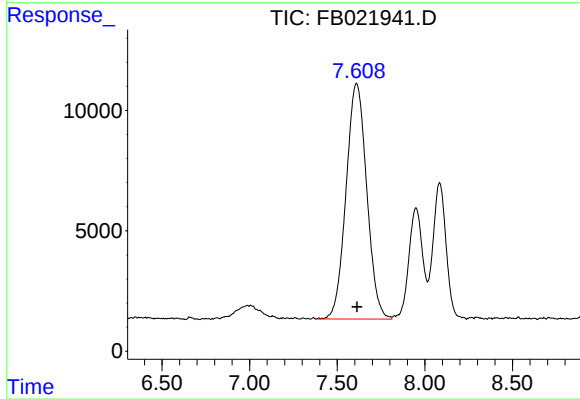


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.002 min
Response: 804122
Conc: 30.42 ng/ml

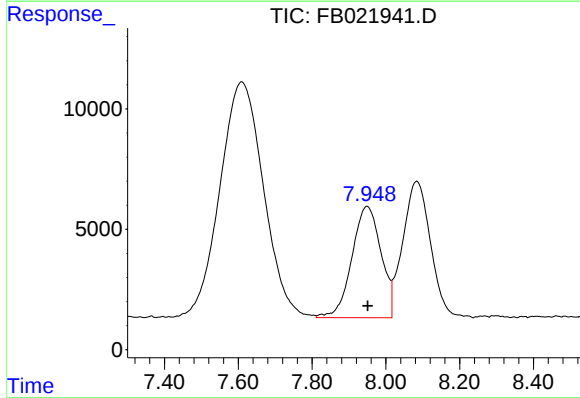


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.002 min
Response: 253269
Conc: 10.21 ng/ml

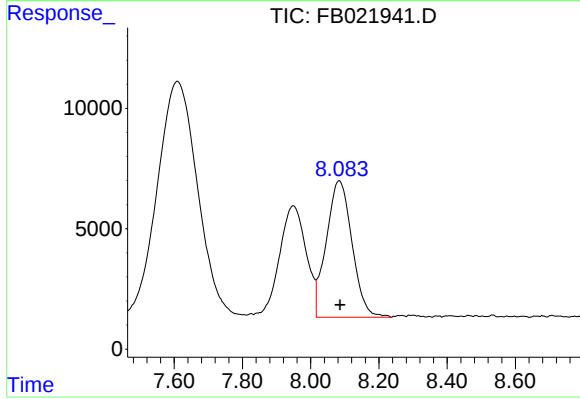


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 296683
Conc: 10.16 ng/ml

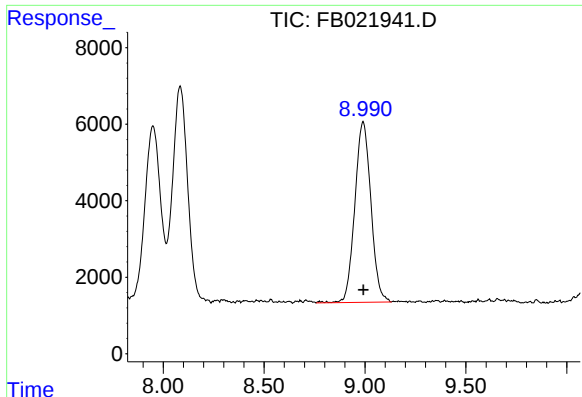


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 261073
Conc: 19.13 ng/ml

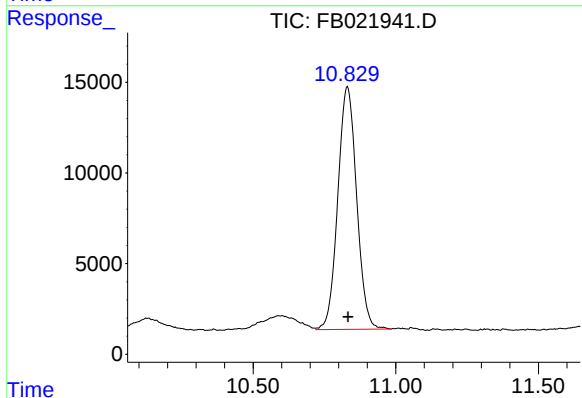


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 613354
Conc: 29.81 ng/ml

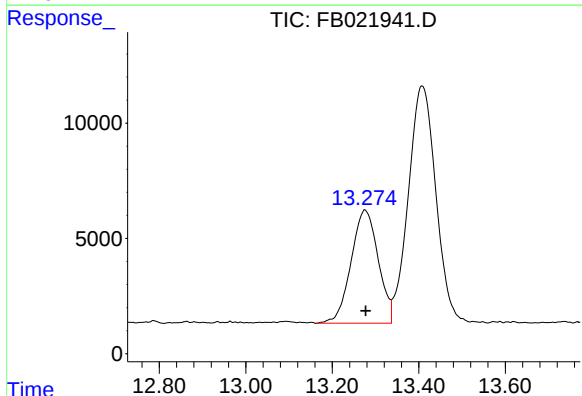


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.001 min
Response: 213448
Conc: 10.26 ng/ml

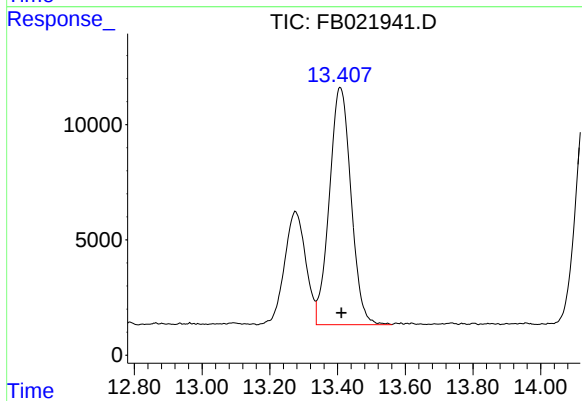

#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 457806
Conc: 20.61 ng/ml

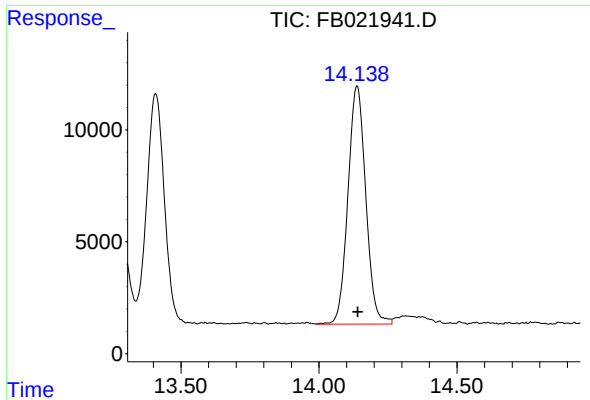


#9 O-Xylene

R.T.: 14.139 min

Delta R.T.: -0.002 min

Response: 477792

Conc: 20.77 ng/ml

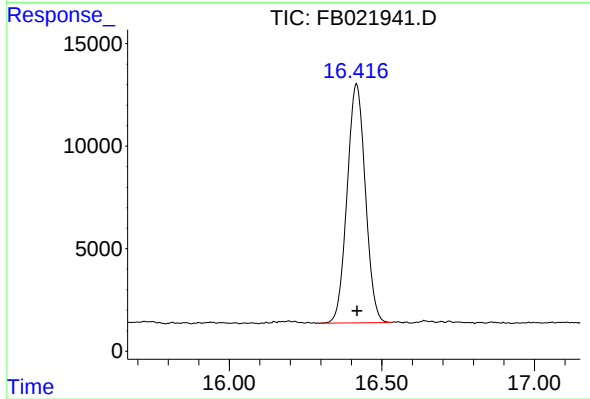

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min

Delta R.T.: -0.002 min

Response: 483833

Conc: 20.52 ng/ml