

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080719\
 Data File : FB021943.D
 Signal(s) : FID2B.CH
 Acq On : 7 Aug 2019 12:49
 Operator : DD/AJ
 Sample : K4178-02MS
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 08 01:02:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.989	253940	18.608 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.860	712152	25.825 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	622014	23.531 ng/ml
3) t	n-Heptane	7.948	190731	7.693 ng/ml
4) t	Benzene	8.083	282512	9.670 ng/ml
6) t	Toluene	10.830	584687	28.416 ng/ml
7) t	Ethylbenzene	13.276	203278	9.771 ng/ml
8) t	m-Xylene	13.408	426524	19.200 ng/ml
9) t	O-Xylene	14.137	451128	19.612 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	434364	18.423 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080719\
Data File : FB021943.D
Signal(s) : FID2B.CH
Acq On : 7 Aug 2019 12:49
Operator : DD/AJ
Sample : K4178-02MS
Misc : 5.04/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 08 01:02:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

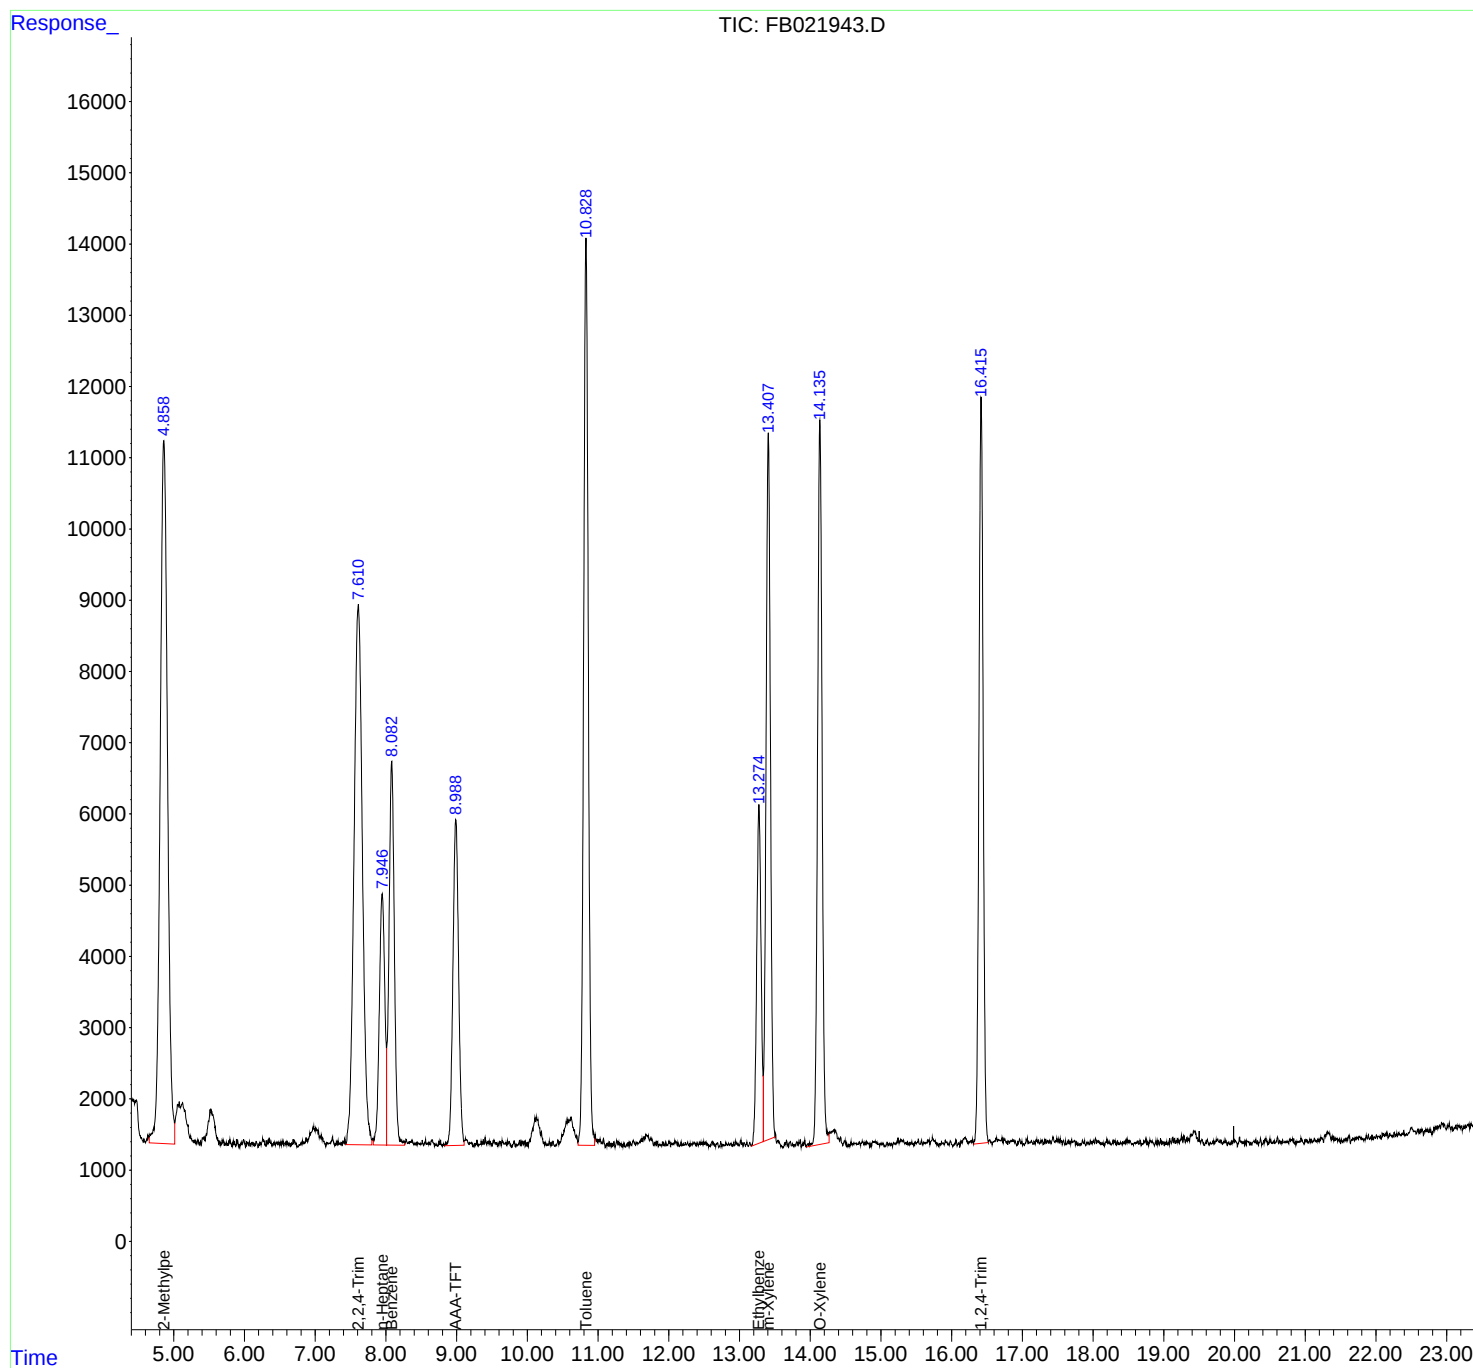

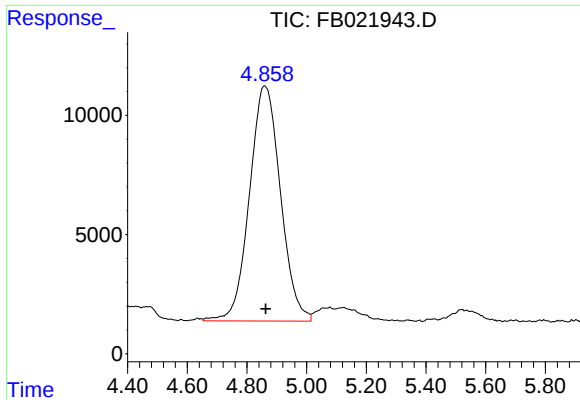


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.003 min
Response: 712152
Conc: 25.82 ng/ml

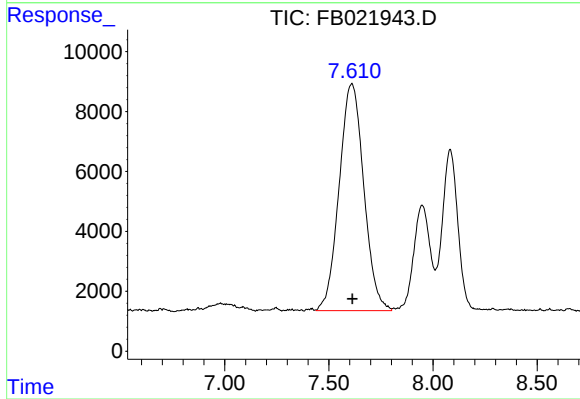


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 622014
Conc: 23.53 ng/ml

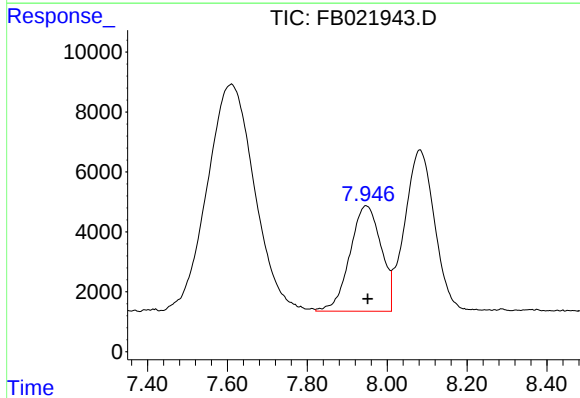


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 190731
Conc: 7.69 ng/ml

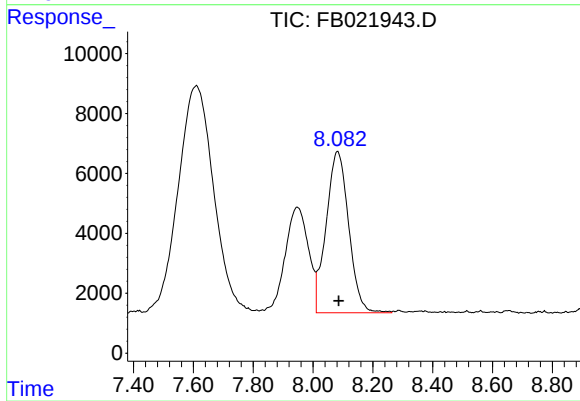


#4 Benzene

R.T.: 8.083 min
Delta R.T.: -0.003 min
Response: 282512
Conc: 9.67 ng/ml

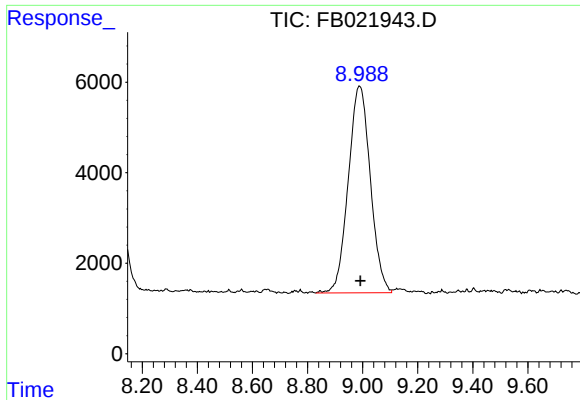


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 253940
Conc: 18.61 ng/ml

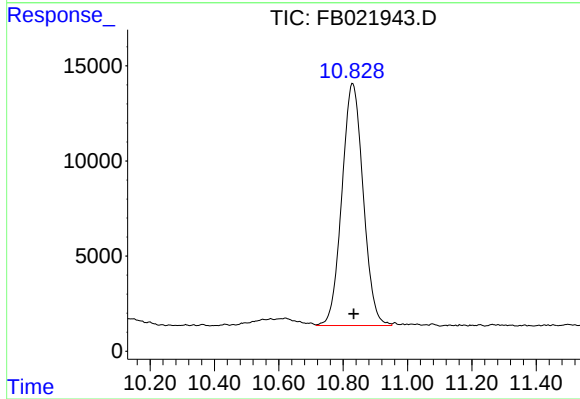


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.004 min
Response: 584687
Conc: 28.42 ng/ml

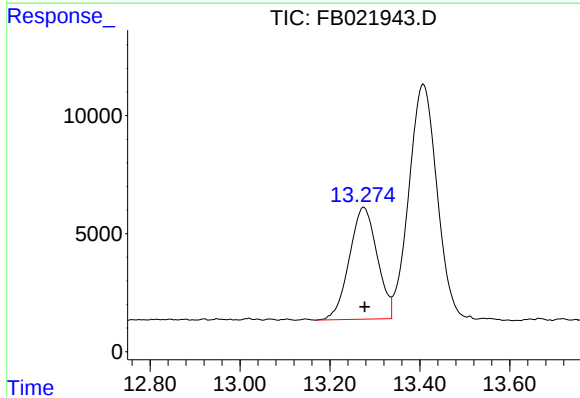


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 203278
Conc: 9.77 ng/ml

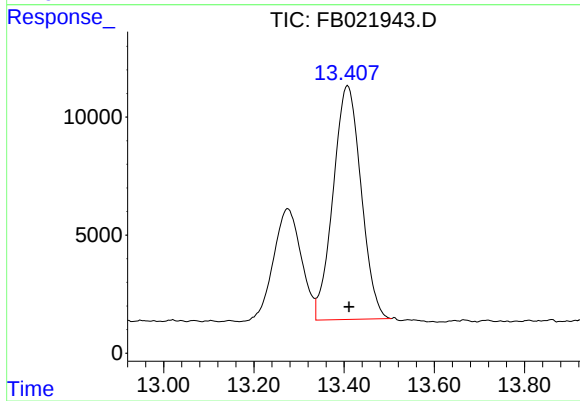


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 426524
Conc: 19.20 ng/ml

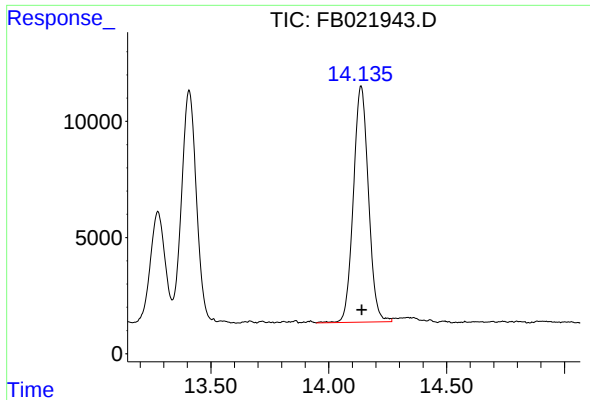

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: -0.003 min
Response: 451128
Conc: 19.61 ng/ml

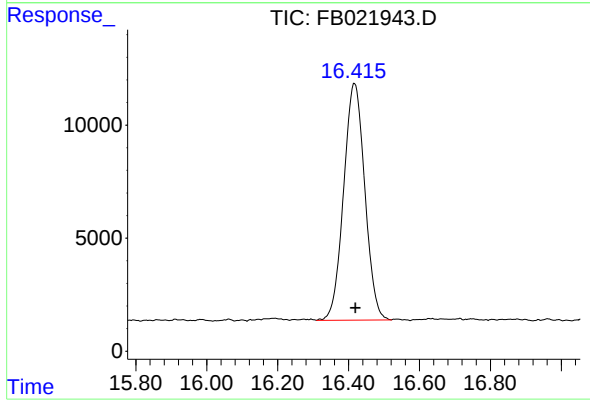

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.002 min
Response: 434364
Conc: 18.42 ng/ml