

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080719\
 Data File : FB021944.D
 Signal(s) : FID2B.CH
 Acq On : 7 Aug 2019 13:19
 Operator : DD/AJ
 Sample : K4178-02MSD
 Misc : 5.06/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 08 01:03:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	248726	18.226 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	656154	23.794 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	568814	21.518 ng/ml
3) t n-Heptane	7.949	171384	6.912 ng/ml
4) t Benzene	8.085	265469	9.087 ng/ml
6) t Toluene	10.832	560414	27.236 ng/ml
7) t Ethylbenzene	13.277	185636	8.923 ng/ml
8) t m-Xylene	13.409	395601	17.808 ng/ml
9) t O-Xylene	14.139	411308	17.881 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	394052	16.714 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080719\
Data File : FB021944.D
Signal(s) : FID2B.CH
Acq On : 7 Aug 2019 13:19
Operator : DD/AJ
Sample : K4178-02MSD
Misc : 5.06/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 08 01:03:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

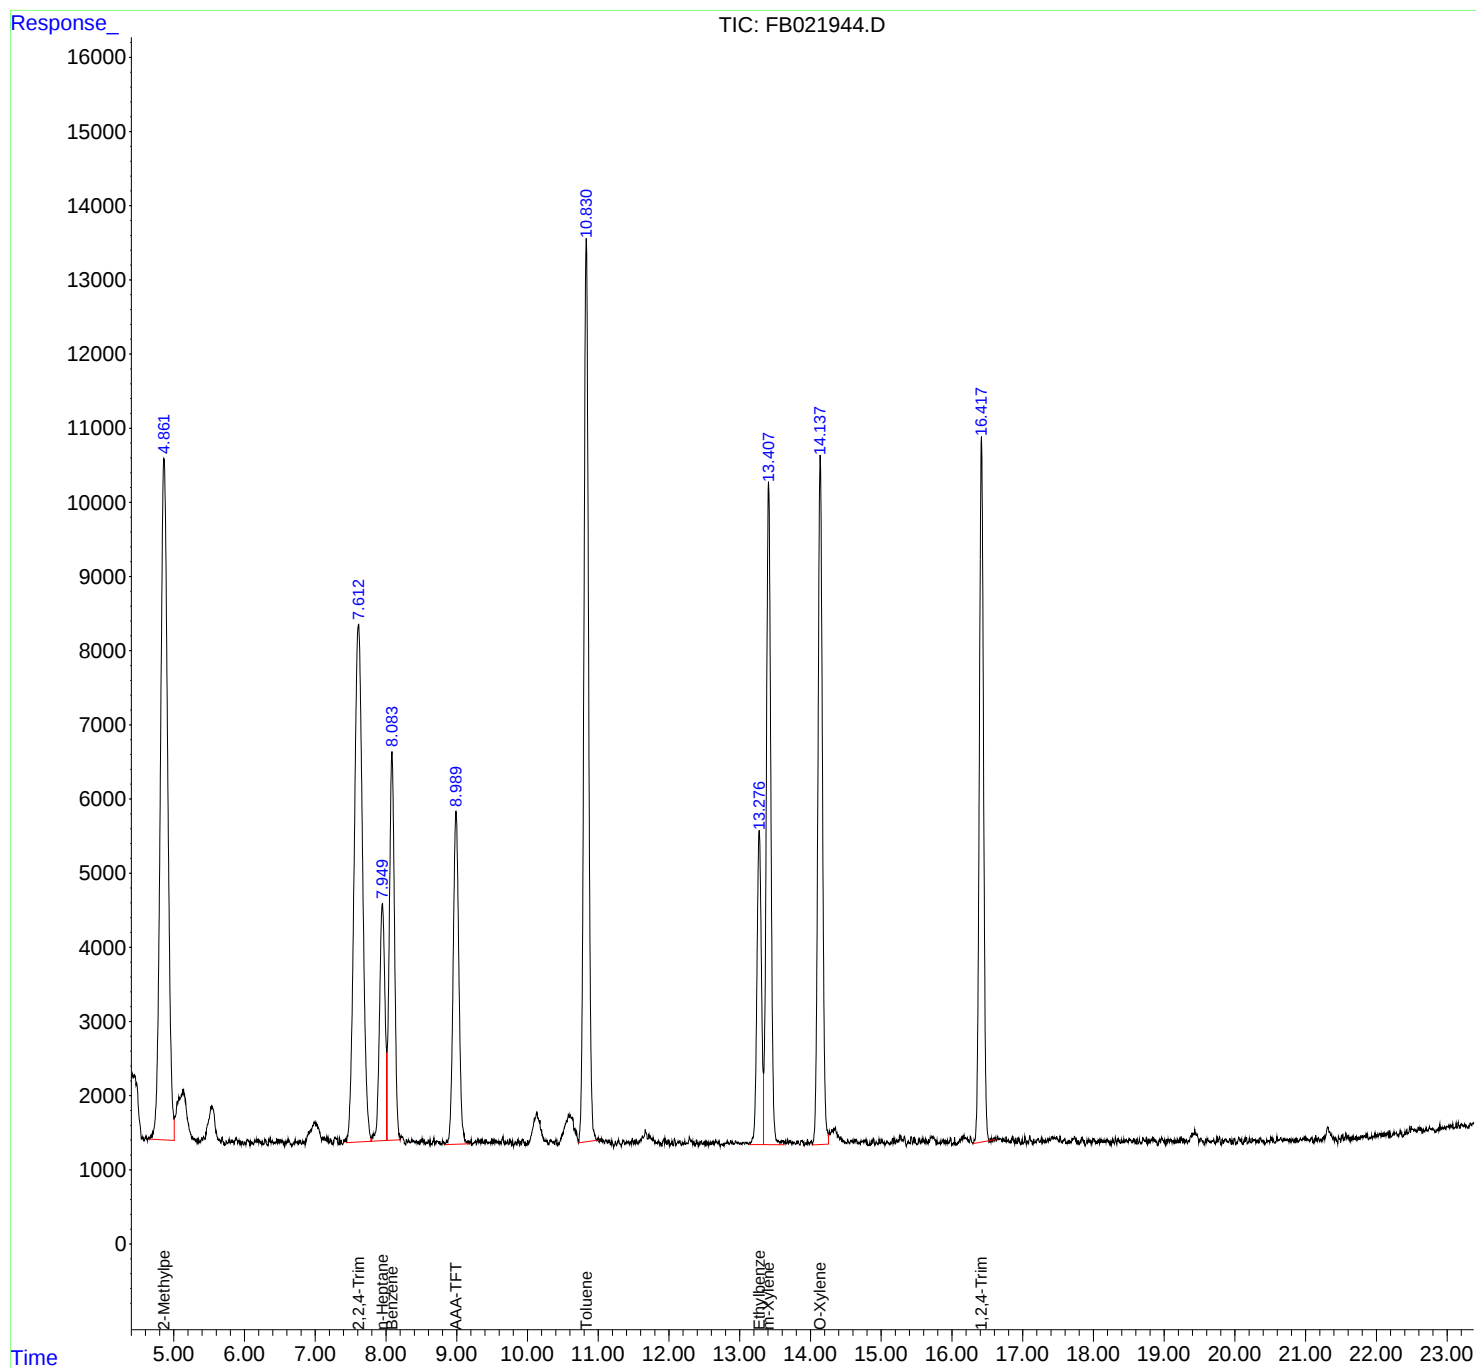

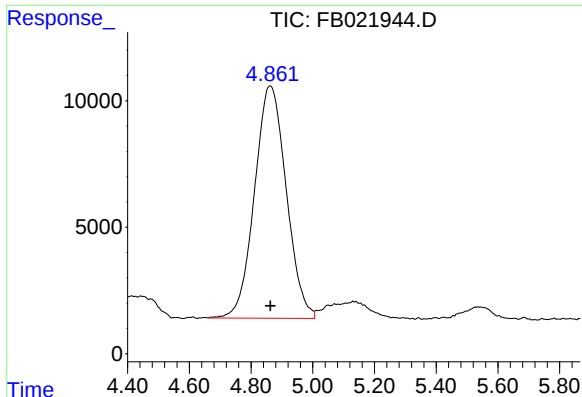


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 656154
Conc: 23.79 ng/ml

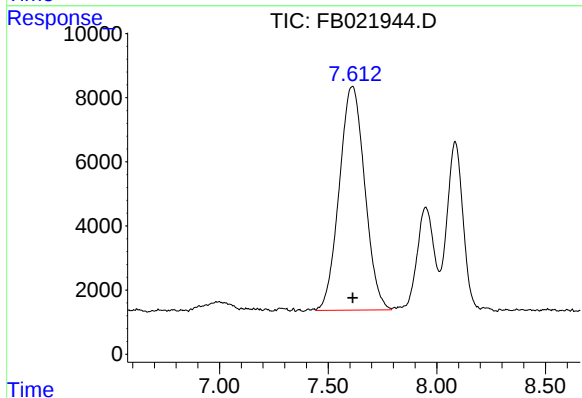


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 568814
Conc: 21.52 ng/ml

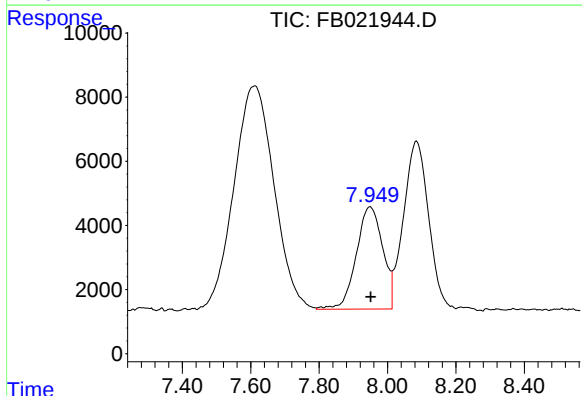


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 171384
Conc: 6.91 ng/ml

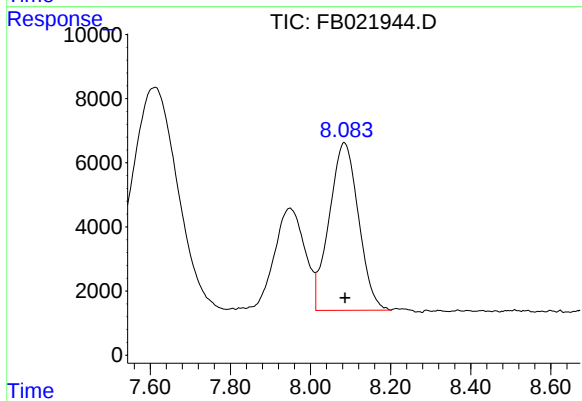


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 265469
Conc: 9.09 ng/ml

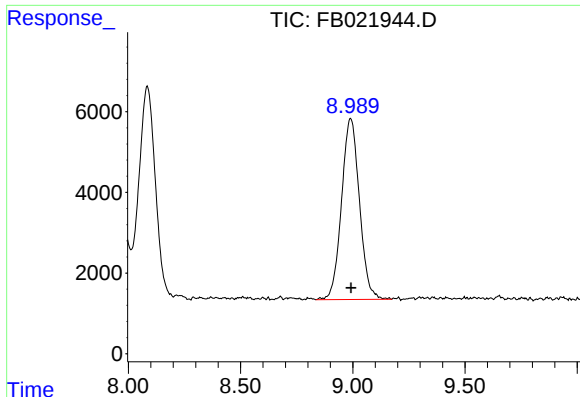


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 248726
Conc: 18.23 ng/ml

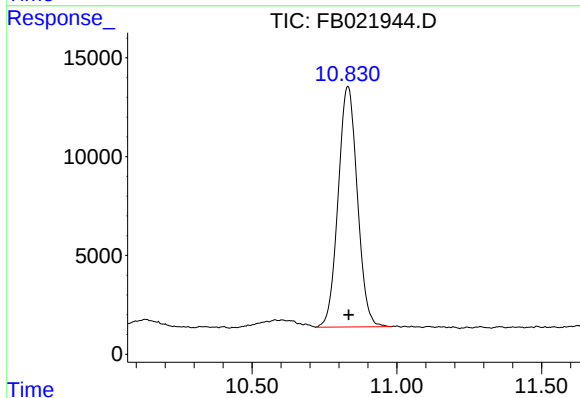


#6 Toluene

R.T.: 10.832 min
Delta R.T.: -0.002 min
Response: 560414
Conc: 27.24 ng/ml

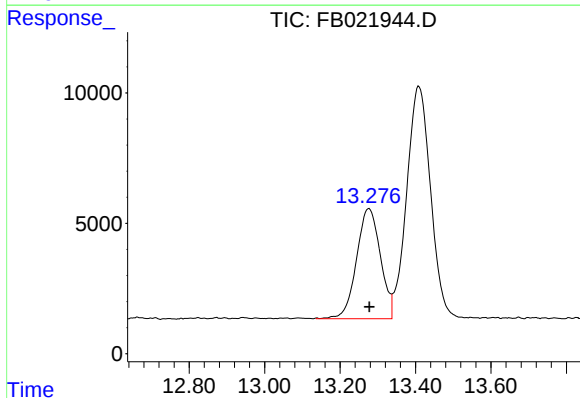


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: -0.001 min
Response: 185636
Conc: 8.92 ng/ml

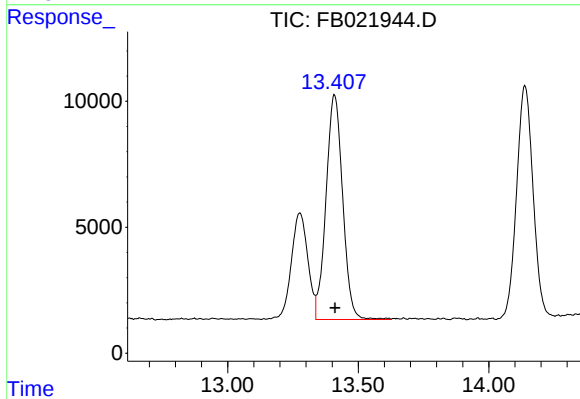


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.001 min
Response: 395601
Conc: 17.81 ng/ml

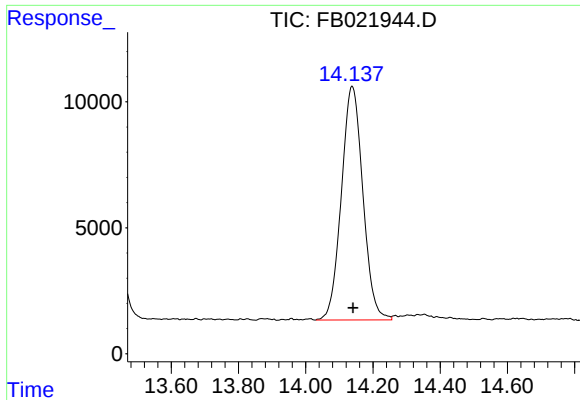

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.002 min
Response: 411308
Conc: 17.88 ng/ml

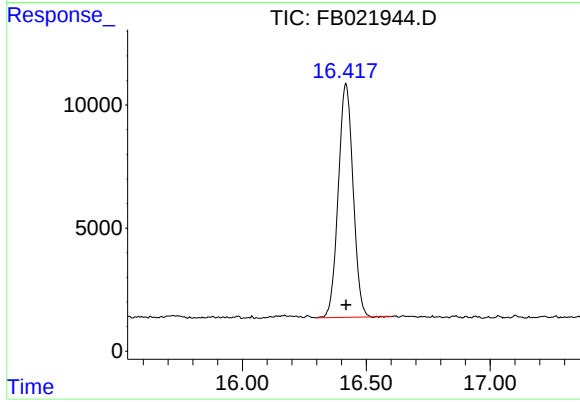

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.001 min
Response: 394052
Conc: 16.71 ng/ml