

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
 Data File : FB021949.D
 Signal(s) : FID2B.CH
 Acq On : 8 Aug 2019 10:17
 Operator : DD/AJ
 Sample : BSF0808S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 09 02:41:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	275078	20.157 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.864	796138	28.871 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	803599	30.400 ng/ml
3) t	n-Heptane	7.950	251072	10.126 ng/ml
4) t	Benzene	8.086	291477	9.977 ng/ml
6) t	Toluene	10.832	628369	30.538 ng/ml
7) t	Ethylbenzene	13.278	212124	10.196 ng/ml
8) t	m-Xylene	13.410	454581	20.463 ng/ml
9) t	O-Xylene	14.140	470566	20.457 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	484539	20.552 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
Data File : FB021949.D
Signal(s) : FID2B.CH
Acq On : 8 Aug 2019 10:17
Operator : DD/AJ
Sample : BSF0808S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 09 02:41:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

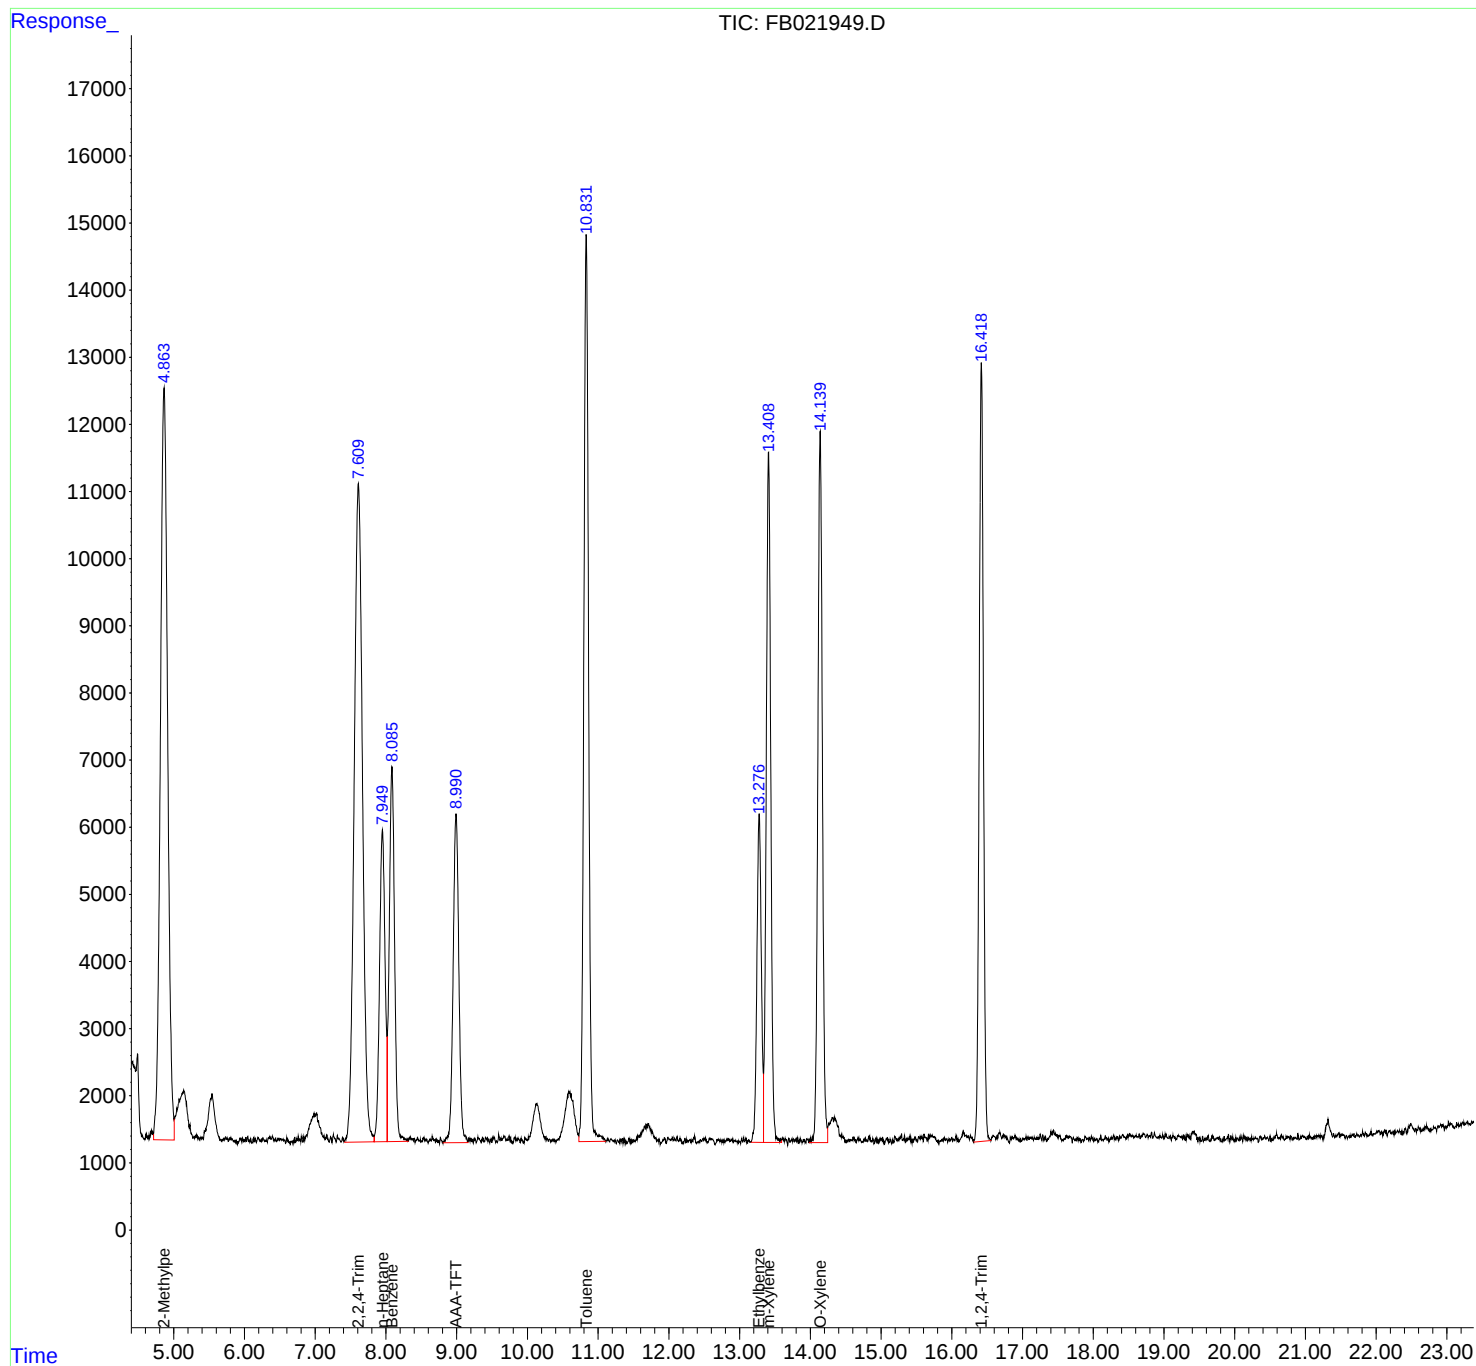

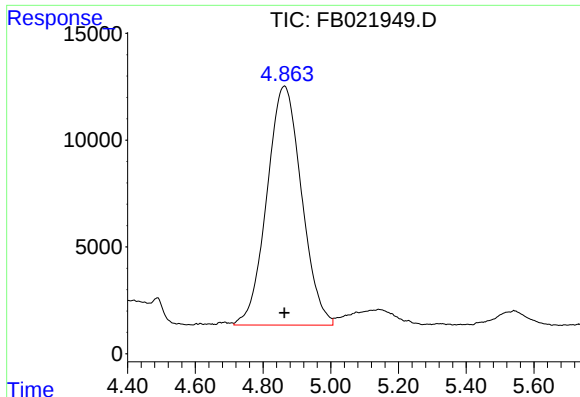


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.001 min
Response: 796138
Conc: 28.87 ng/ml

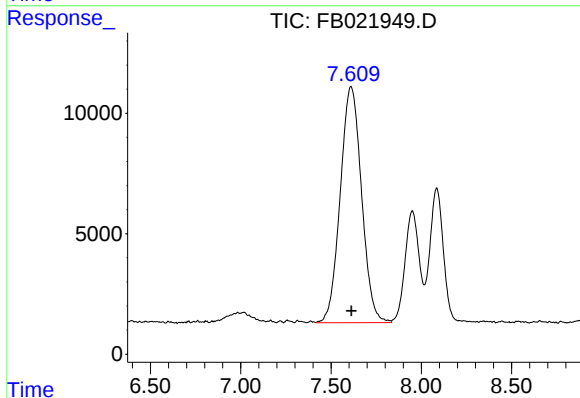


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.002 min
Response: 803599
Conc: 30.40 ng/ml

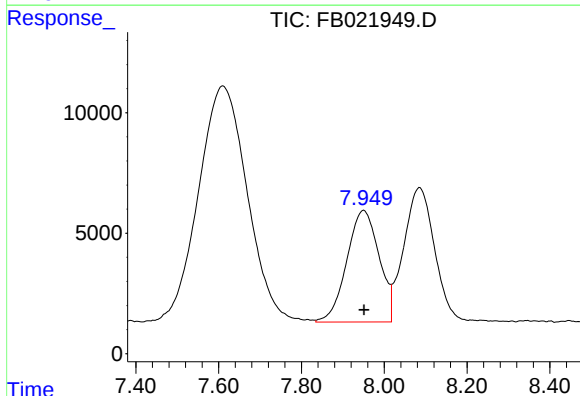


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 251072
Conc: 10.13 ng/ml

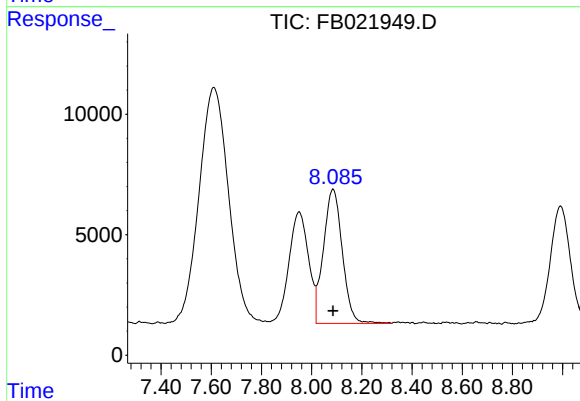


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 291477
Conc: 9.98 ng/ml

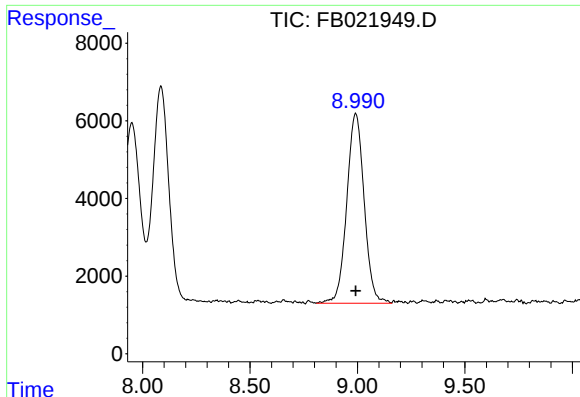


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 275078
Conc: 20.16 ng/ml

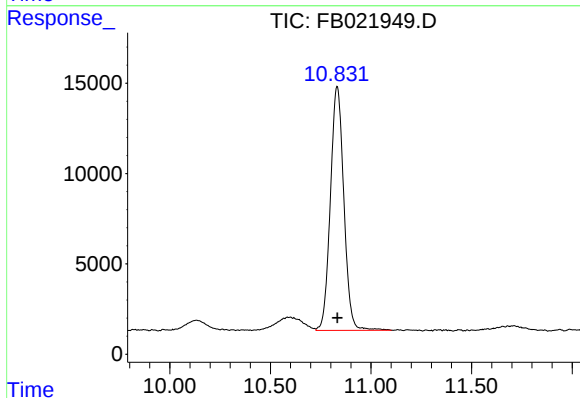


#6 Toluene

R.T.: 10.832 min
Delta R.T.: 0.000 min
Response: 628369
Conc: 30.54 ng/ml

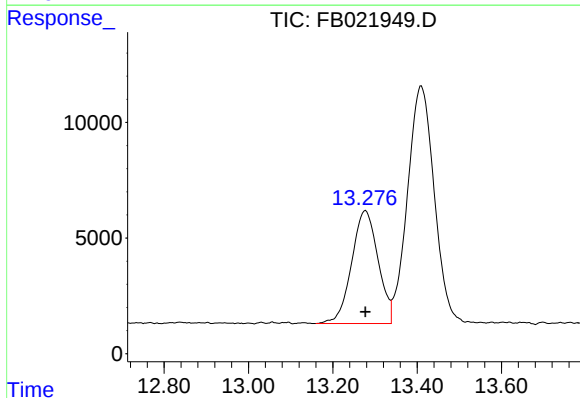


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 212124
Conc: 10.20 ng/ml

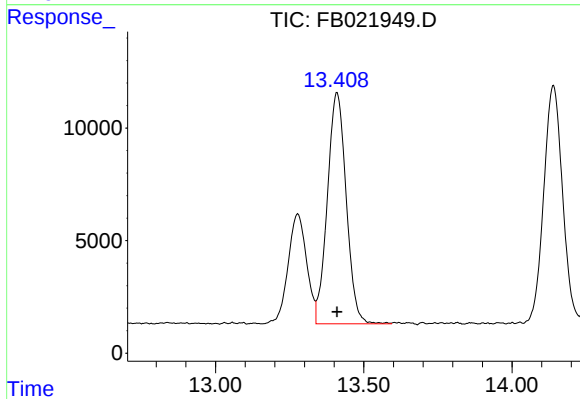


#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: 0.000 min
Response: 454581
Conc: 20.46 ng/ml

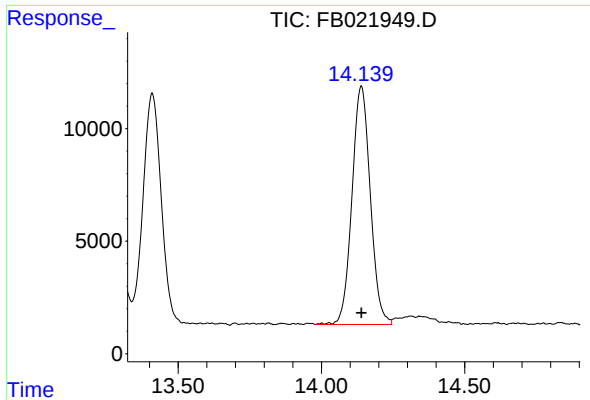

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 470566
Conc: 20.46 ng/ml

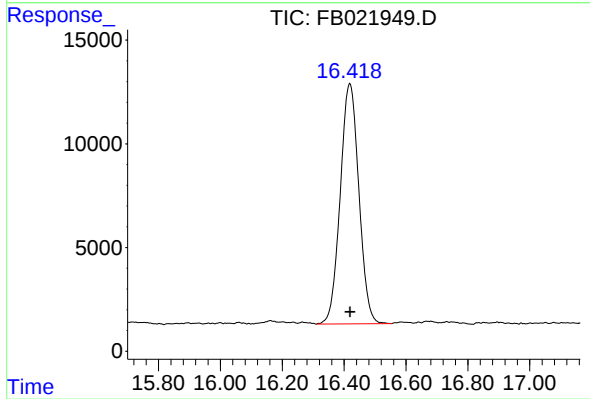

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.000 min
Response: 484539
Conc: 20.55 ng/ml