

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
 Data File : FB021953.D
 Signal(s) : FID2B.CH
 Acq On : 8 Aug 2019 12:19
 Operator : DD/AJ
 Sample : K4092-01MS
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 09 02:41:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.991	277048	20.302 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.865	654471	23.733 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	529338	20.025 ng/ml
3) t	n-Heptane	7.950	158376	6.388 ng/ml
4) t	Benzene	8.086	285262	9.764 ng/ml
6) t	Toluene	10.833	575917	27.989 ng/ml
7) t	Ethylbenzene	13.278	185435	8.913 ng/ml
8) t	m-Xylene	13.411	383596	17.267 ng/ml
9) t	O-Xylene	14.140	405113	17.612 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	358116	15.189 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
Data File : FB021953.D
Signal(s) : FID2B.CH
Acq On : 8 Aug 2019 12:19
Operator : DD/AJ
Sample : K4092-01MS
Misc : 5.01/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 09 02:41:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

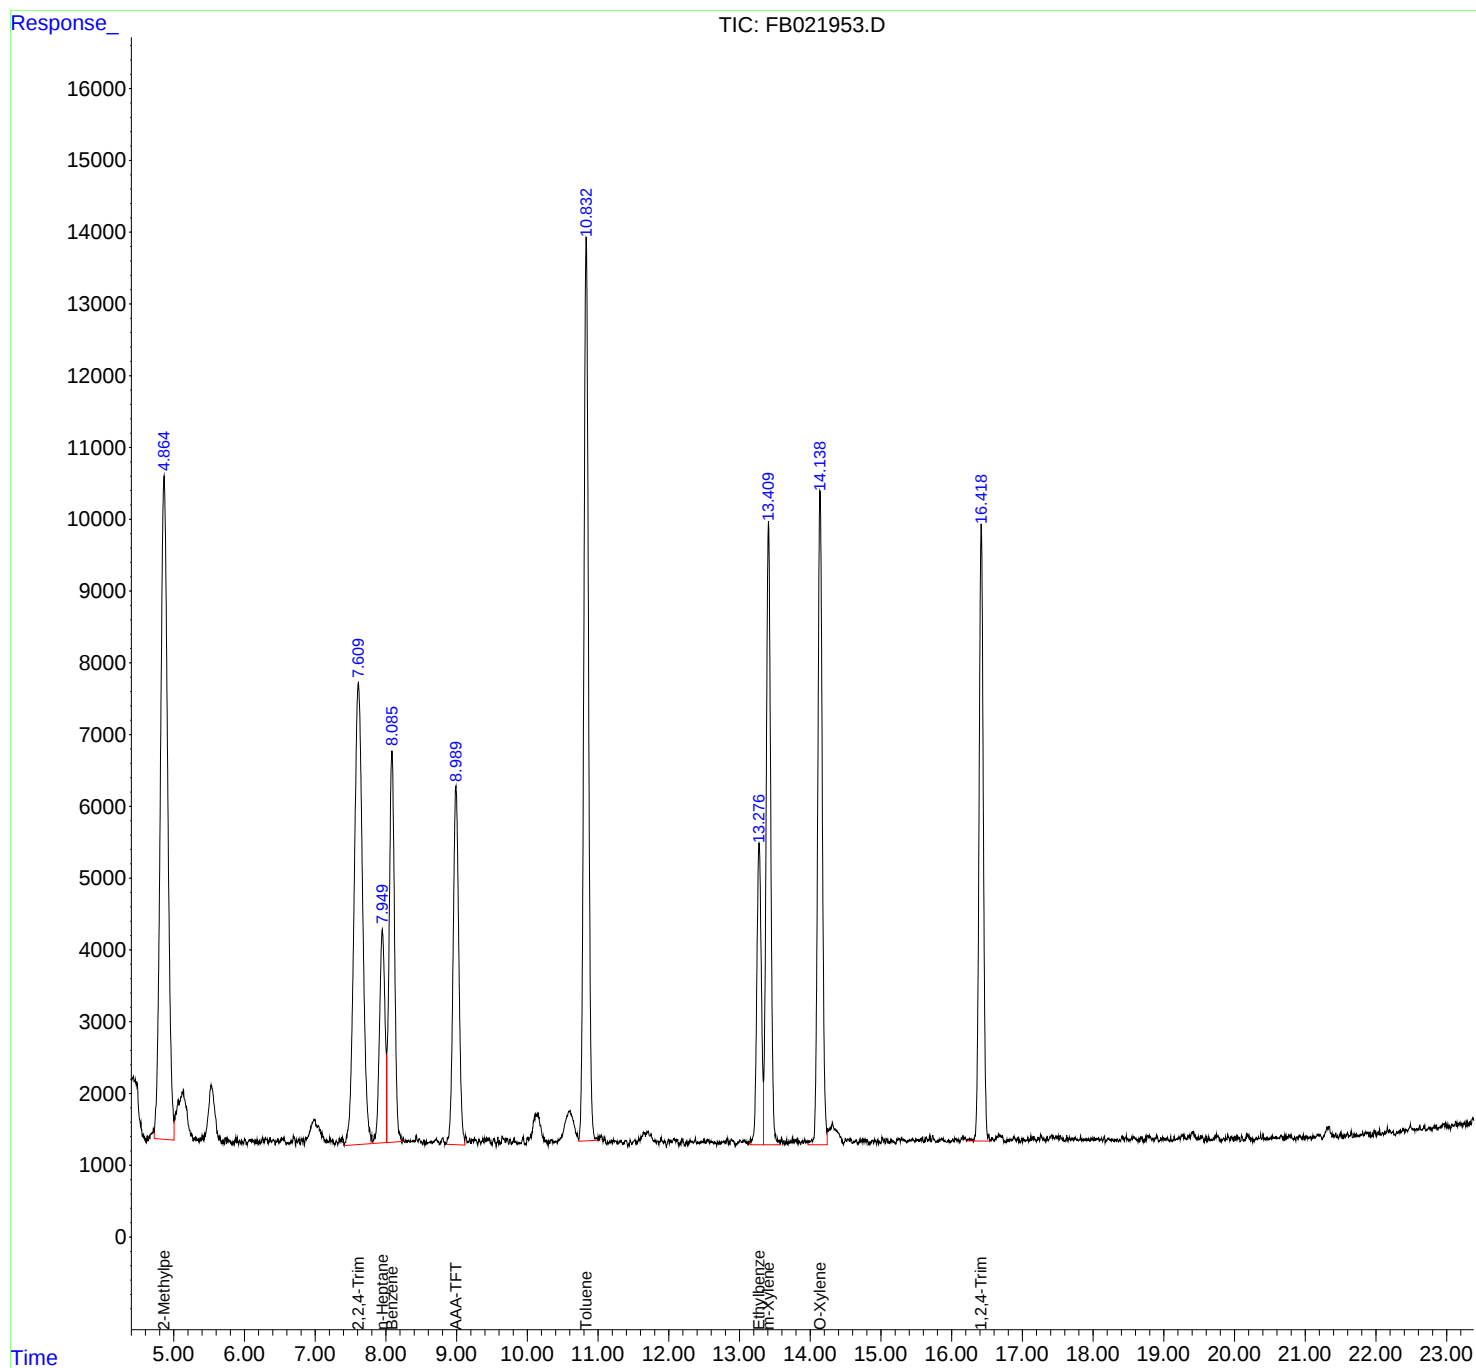

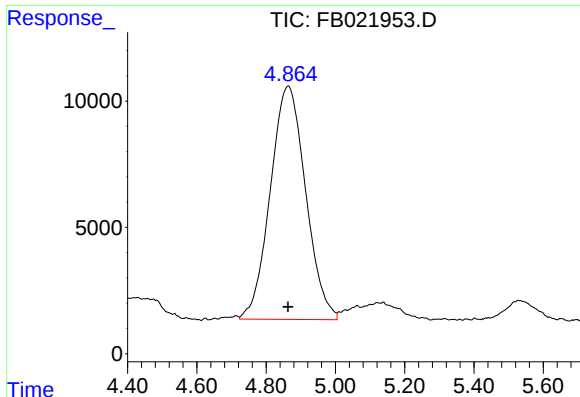


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.002 min
Response: 654471
Conc: 23.73 ng/ml

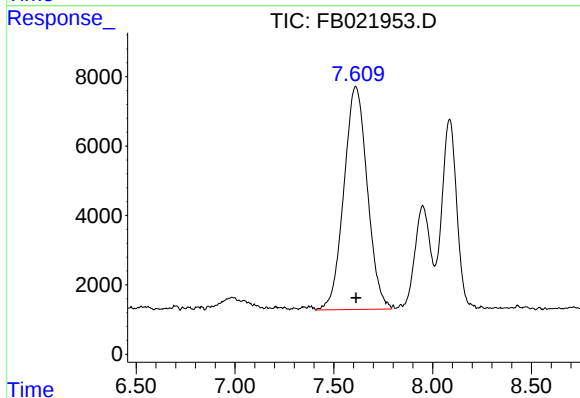


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.002 min
Response: 529338
Conc: 20.02 ng/ml

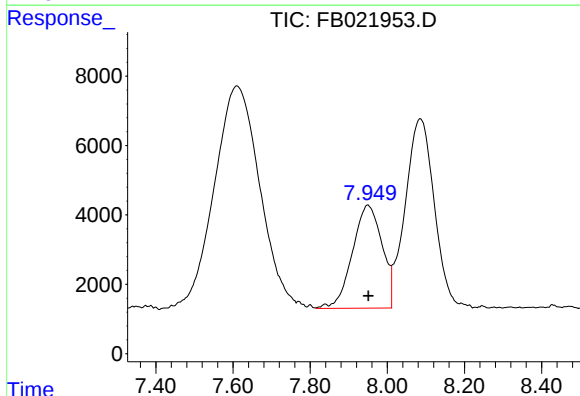


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 158376
Conc: 6.39 ng/ml

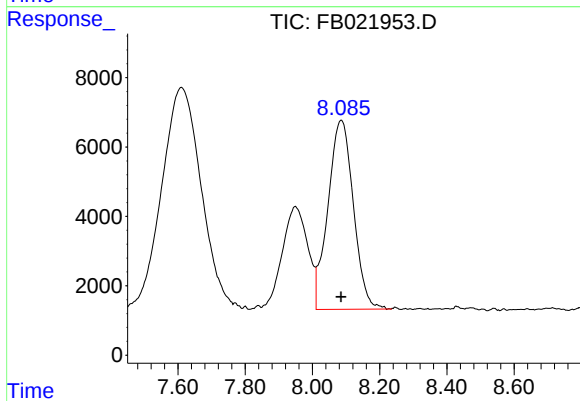


#4 Benzene

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 285262
Conc: 9.76 ng/ml

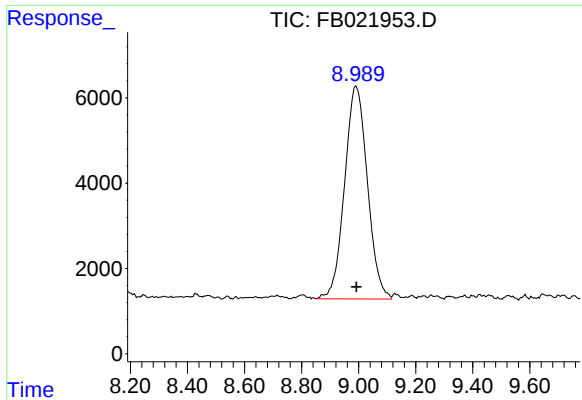


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 277048
Conc: 20.30 ng/ml

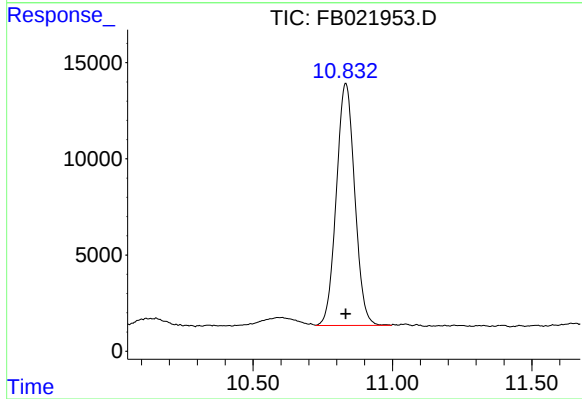


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 575917
Conc: 27.99 ng/ml

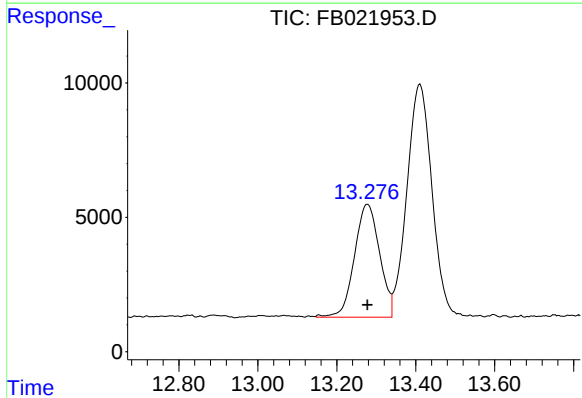


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 185435
Conc: 8.91 ng/ml

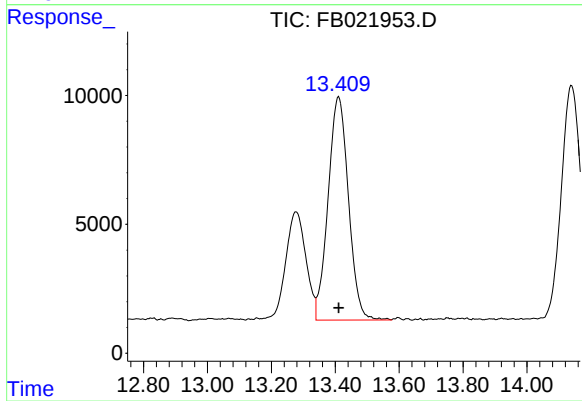


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 383596
Conc: 17.27 ng/ml

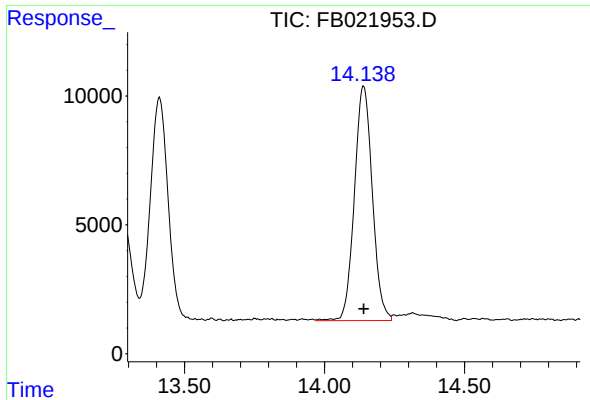

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 405113
Conc: 17.61 ng/ml

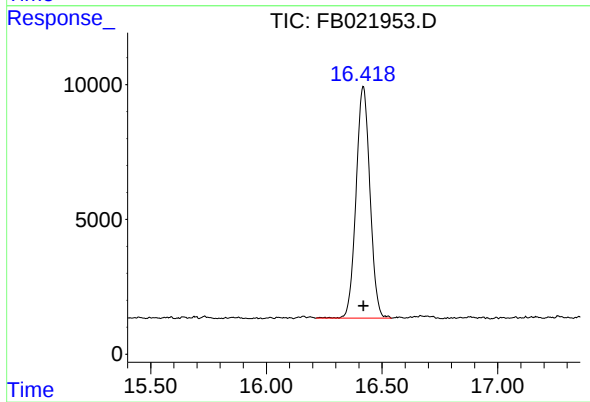

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.000 min
Response: 358116
Conc: 15.19 ng/ml