

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
Data File : FB021955.D
Signal(s) : FID2B.CH
Acq On : 8 Aug 2019 13:21
Operator : DD/AJ
Sample : K4092-03
Misc : 5.03/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 09 02:42:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	273507	20.042 ng/ml
Target Compounds			
7) t Ethylbenzene	13.235	4260	0.205 ng/ml
8) t m-Xylene	13.398	2891	0.130 ng/ml
9) t O-Xylene	14.141	2348	0.102 ng/ml
10) t 1,2,4-Trimethylbenzene	16.421	45114	1.913 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
Data File : FB021955.D
Signal(s) : FID2B.CH
Acq On : 8 Aug 2019 13:21
Operator : DD/AJ
Sample : K4092-03
Misc : 5.03/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 09 02:42:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

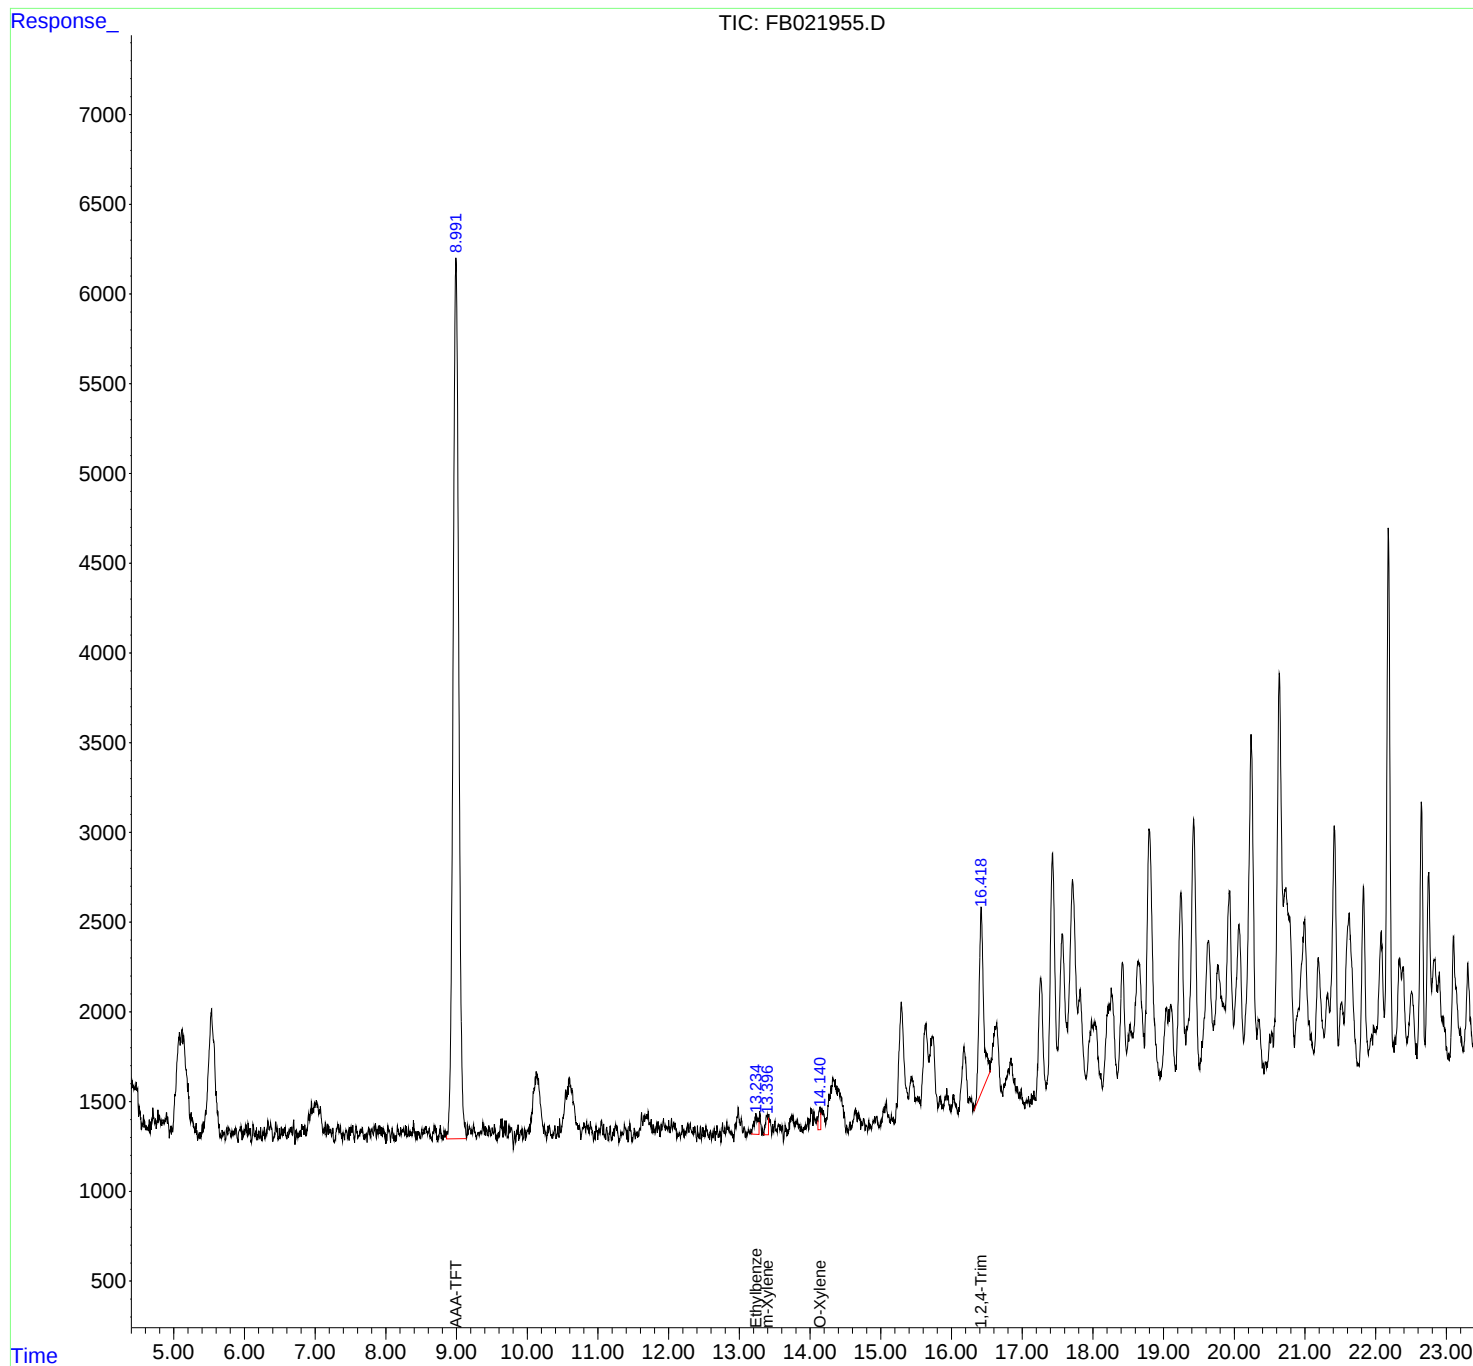

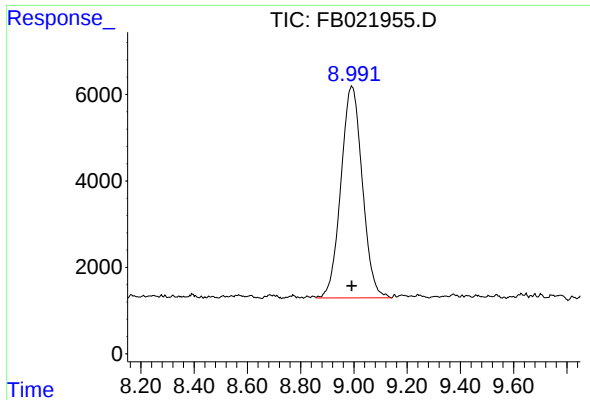


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 273507
Conc: 20.04 ng/ml

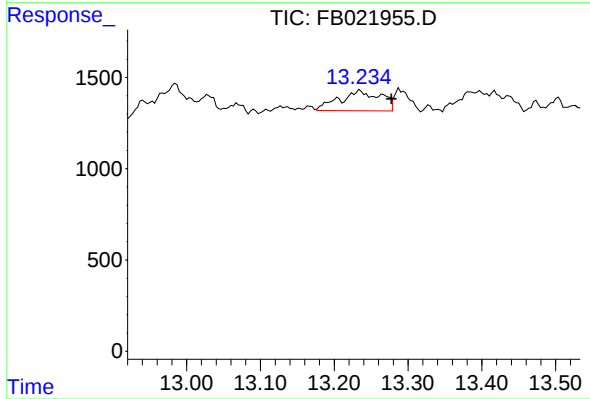


#7 Ethylbenzene

R.T.: 13.235 min
Delta R.T.: -0.043 min
Response: 4260
Conc: 0.20 ng/ml

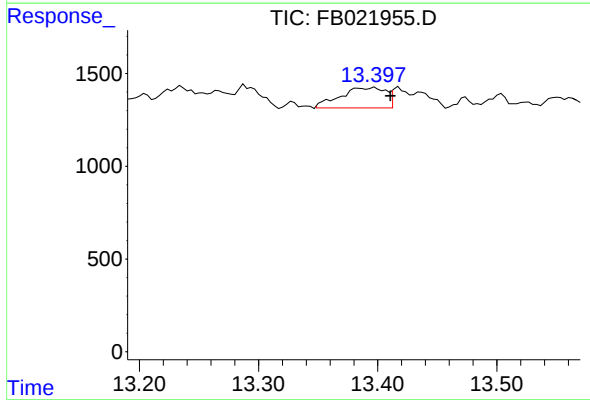


#8 m-Xylene

R.T.: 13.398 min
Delta R.T.: -0.013 min
Response: 2891
Conc: 0.13 ng/ml

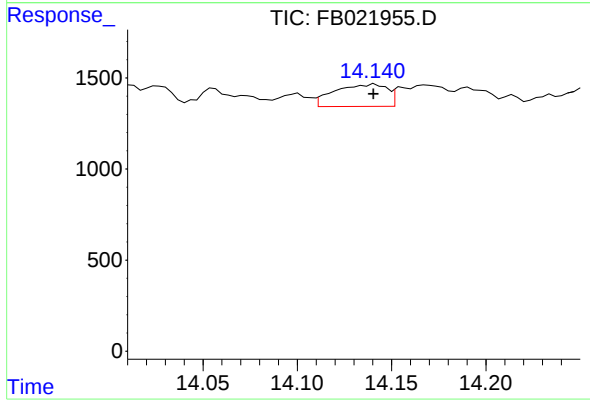

#9 O-Xylene

R.T.: 14.141 min
Delta R.T.: 0.000 min
Response: 2348
Conc: 0.10 ng/ml

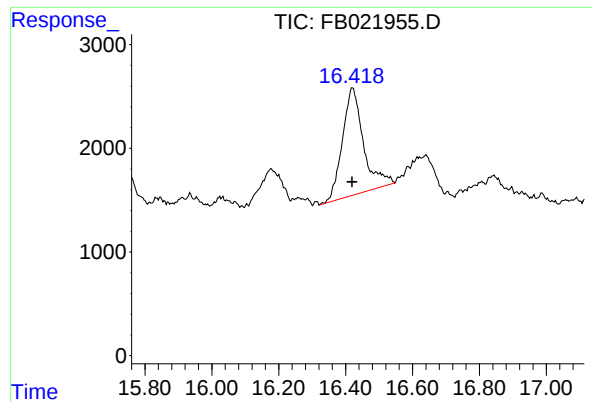

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: 0.002 min
Response: 45114
Conc: 1.91 ng/ml