

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
 Data File : FB021954.D
 Signal(s) : FID2B.CH
 Acq On : 8 Aug 2019 12:51
 Operator : DD/AJ
 Sample : K4092-01MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 09 02:42:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	270986	19.857 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	623928	22.626 ng/ml
2) t 2,2,4-Trimethylpentane	7.614	490724	18.564 ng/ml
3) t n-Heptane	7.951	152487	6.150 ng/ml
4) t Benzene	8.084	278970	9.549 ng/ml
6) t Toluene	10.831	561994	27.313 ng/ml
7) t Ethylbenzene	13.277	183409	8.816 ng/ml
8) t m-Xylene	13.409	374186	16.844 ng/ml
9) t O-Xylene	14.140	395511	17.194 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	344450	14.610 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080819\
Data File : FB021954.D
Signal(s) : FID2B.CH
Acq On : 8 Aug 2019 12:51
Operator : DD/AJ
Sample : K4092-01MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 09 02:42:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

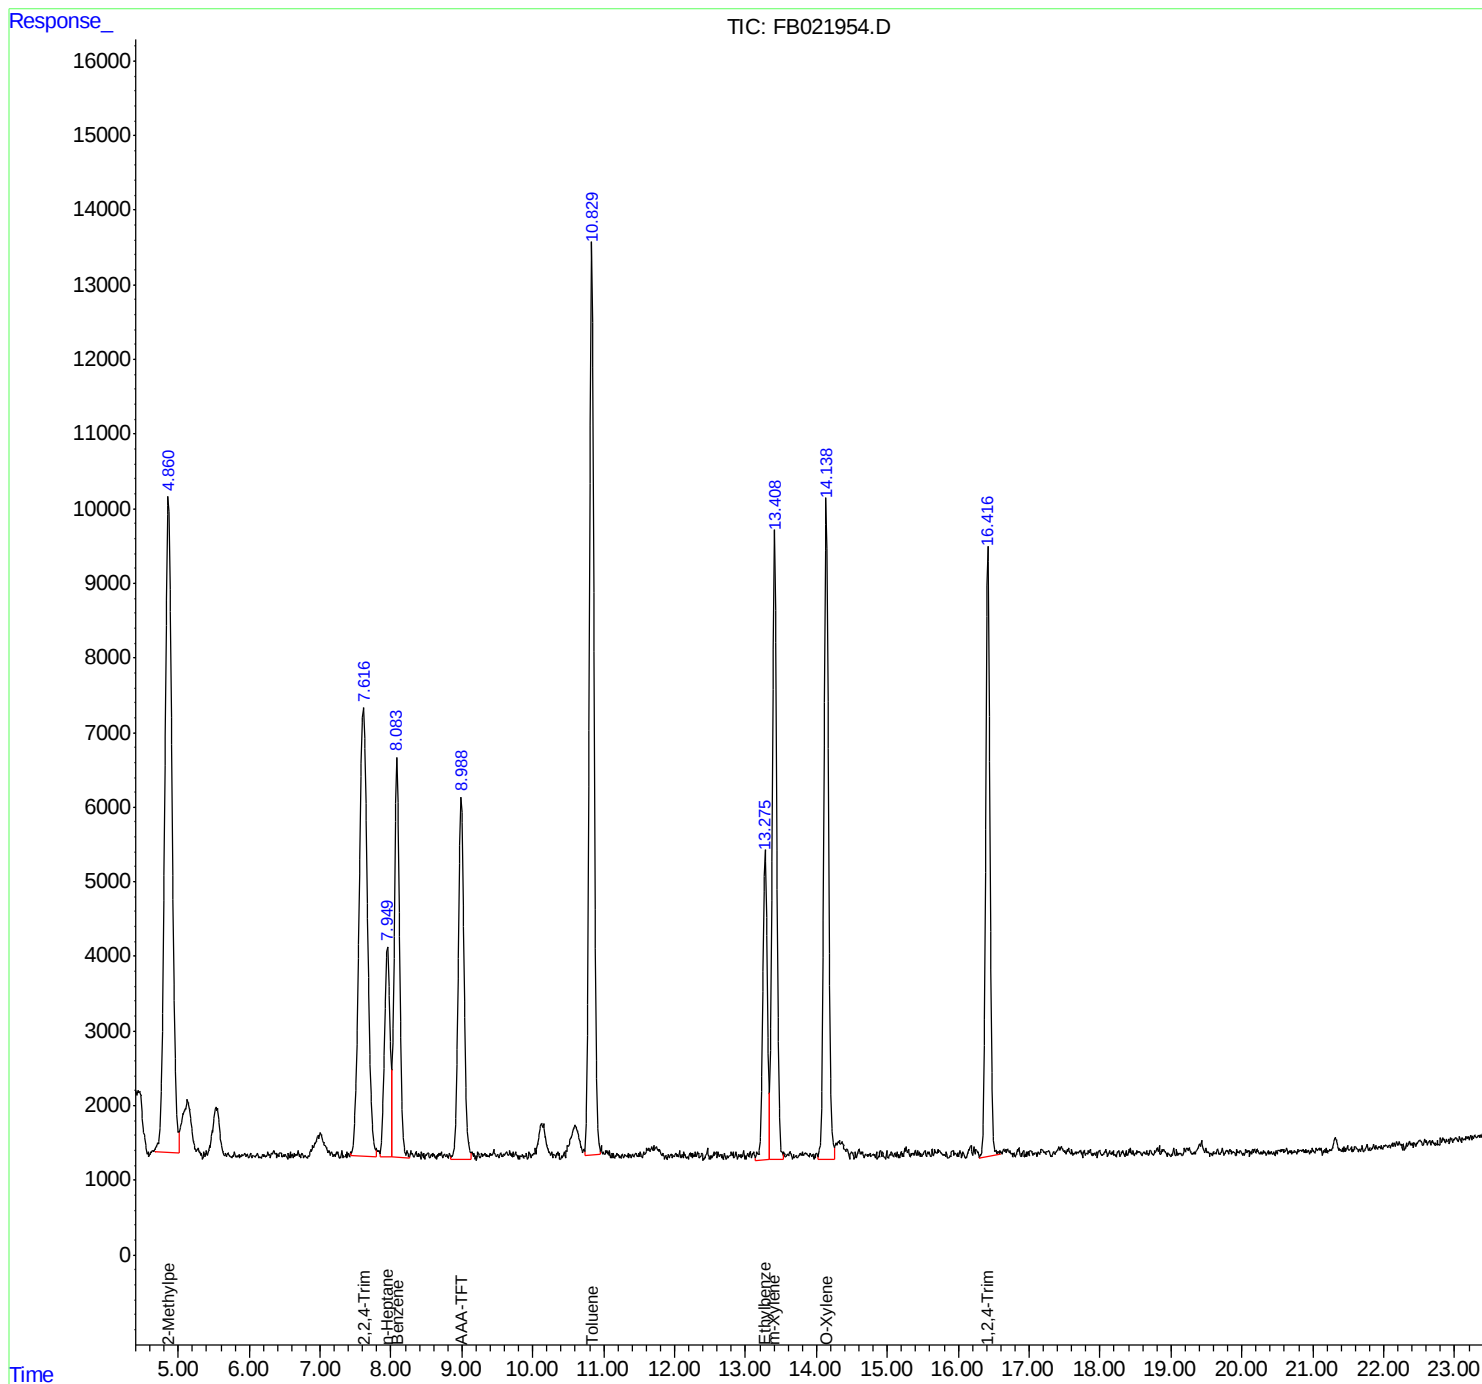

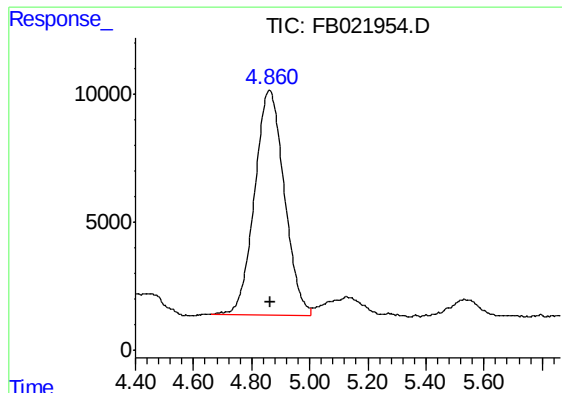


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 623928
Conc: 22.63 ng/ml

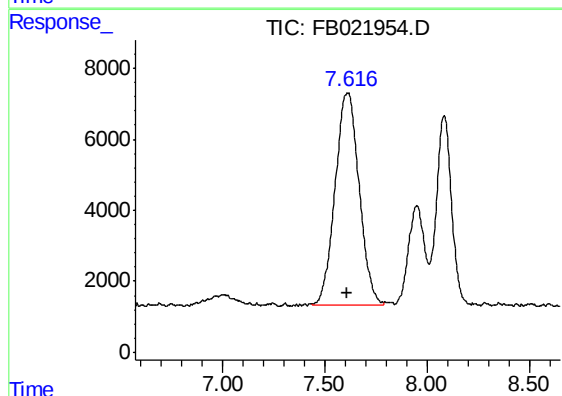


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min
Delta R.T.: 0.002 min
Response: 490724
Conc: 18.56 ng/ml

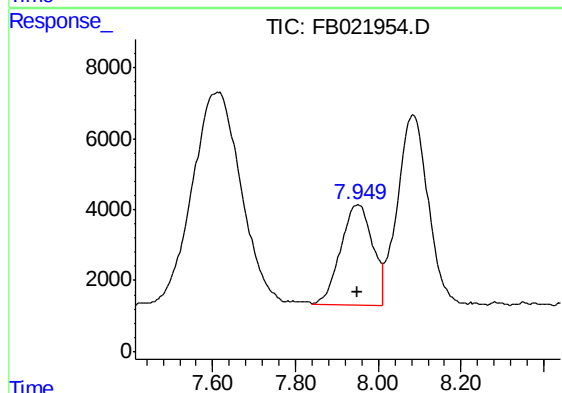


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 152487
Conc: 6.15 ng/ml

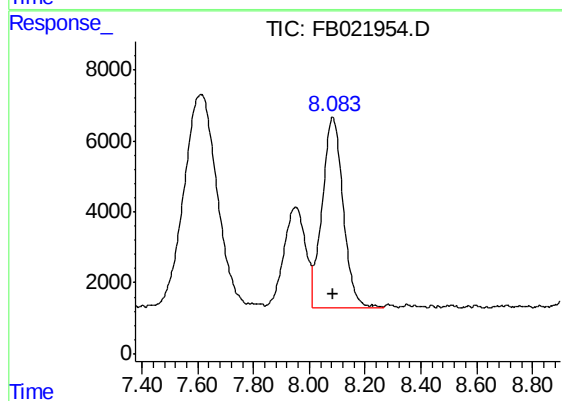


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 278970
Conc: 9.55 ng/ml

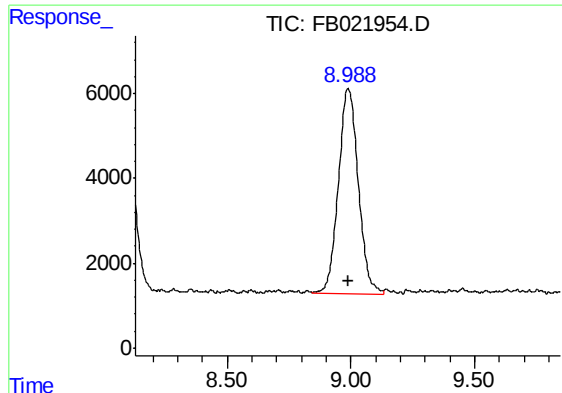


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 270986
Conc: 19.86 ng/ml

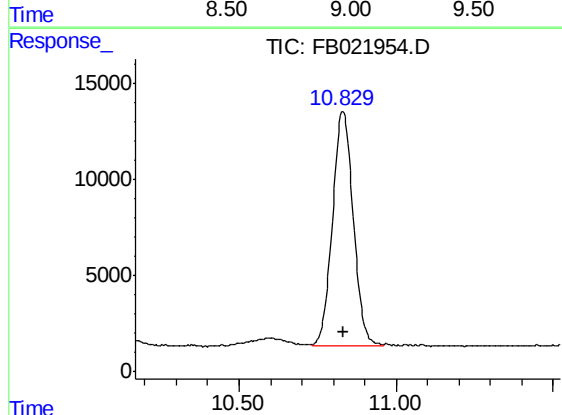


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 561994
Conc: 27.31 ng/ml

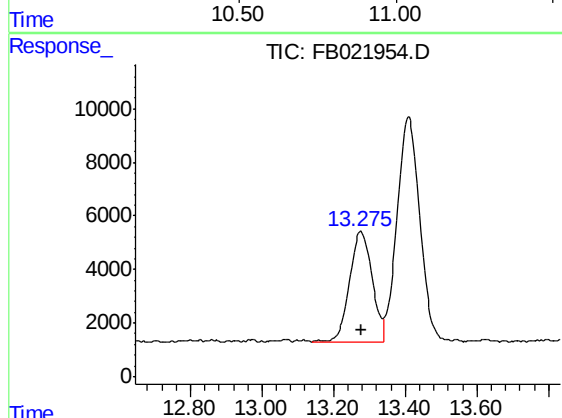


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.000 min
Response: 183409
Conc: 8.82 ng/ml

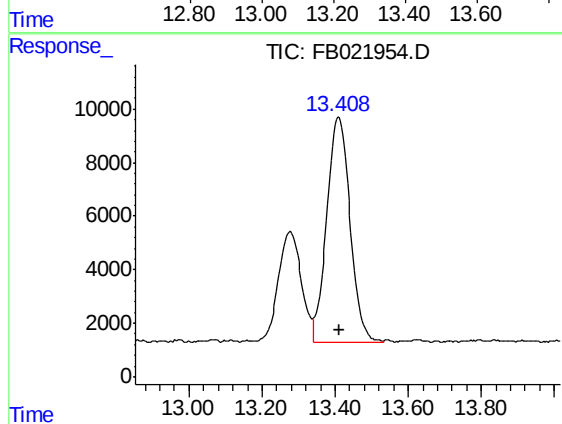


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.001 min
Response: 374186
Conc: 16.84 ng/ml

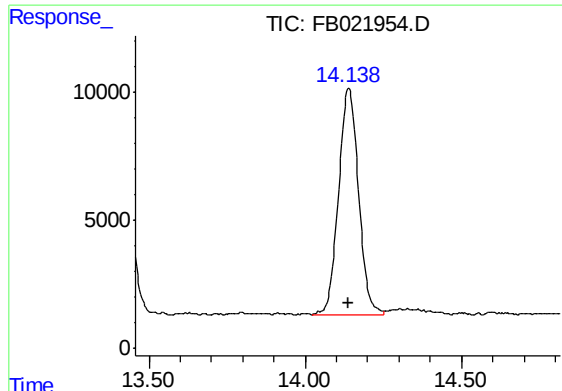

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 395511
Conc: 17.19 ng/ml

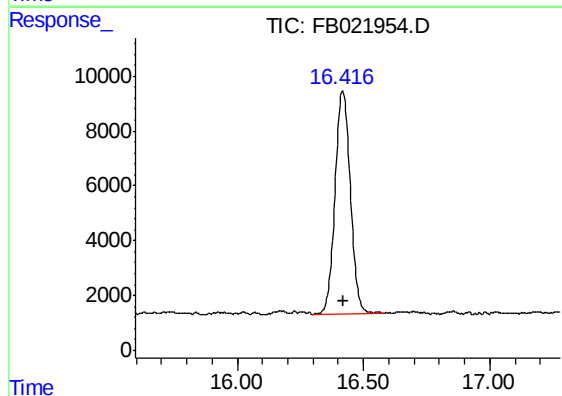

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: 0.000 min
Response: 344450
Conc: 14.61 ng/ml