

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080919\
 Data File : FB021968.D
 Signal(s) : FID2B.CH
 Acq On : 9 Aug 2019 10:53
 Operator : DD/AJ
 Sample : BSF0809S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 10 01:45:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.989	250439	18.352 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	751280	27.244 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	756193	28.606 ng/ml
3) t	n-Heptane	7.948	237082	9.562 ng/ml
4) t	Benzene	8.084	277376	9.494 ng/ml
6) t	Toluene	10.831	596921	29.010 ng/ml
7) t	Ethylbenzene	13.277	206964	9.948 ng/ml
8) t	m-Xylene	13.410	436460	19.647 ng/ml
9) t	O-Xylene	14.139	454469	19.757 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	474541	20.127 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080919\
Data File : FB021968.D
Signal(s) : FID2B.CH
Acq On : 9 Aug 2019 10:53
Operator : DD/AJ
Sample : BSF0809S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 10 01:45:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

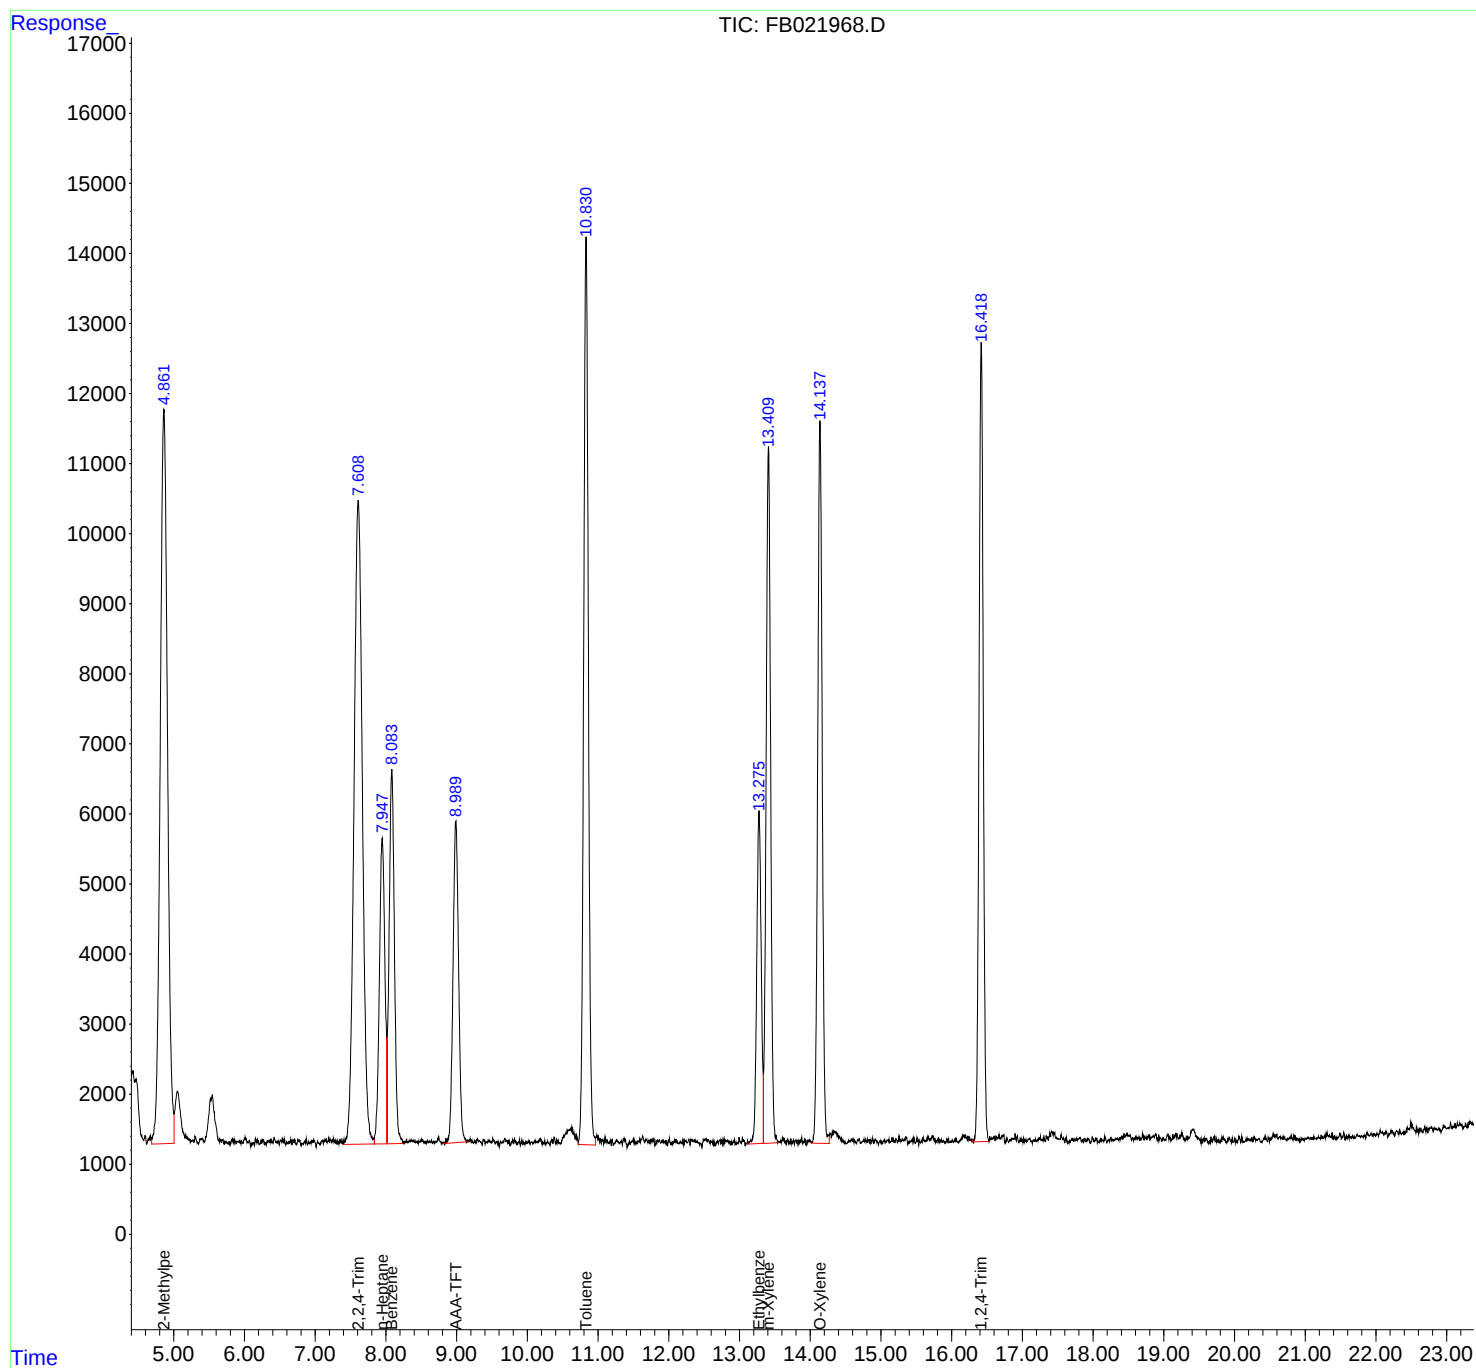

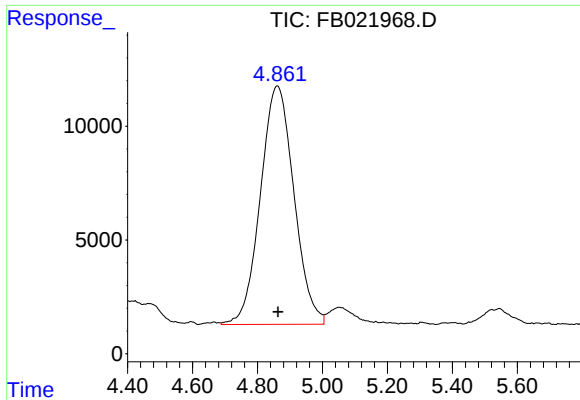


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 751280
Conc: 27.24 ng/ml

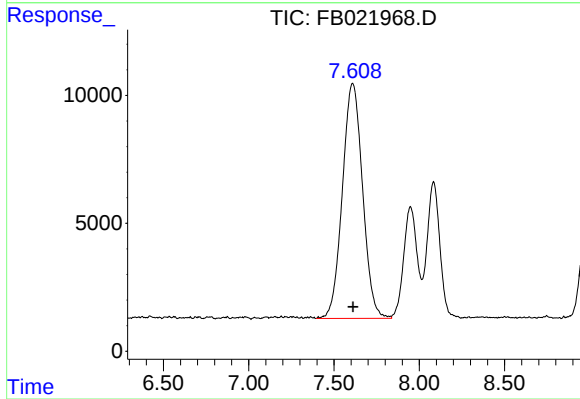


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 756193
Conc: 28.61 ng/ml

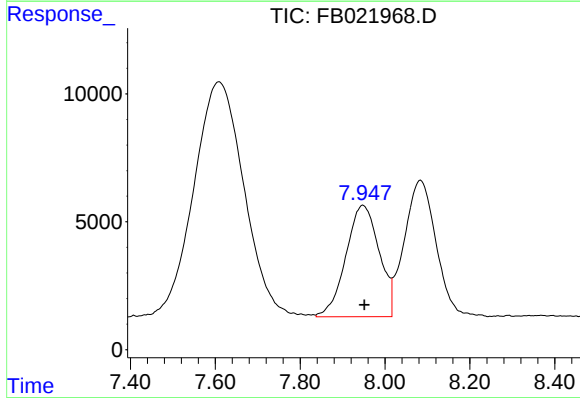


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 237082
Conc: 9.56 ng/ml

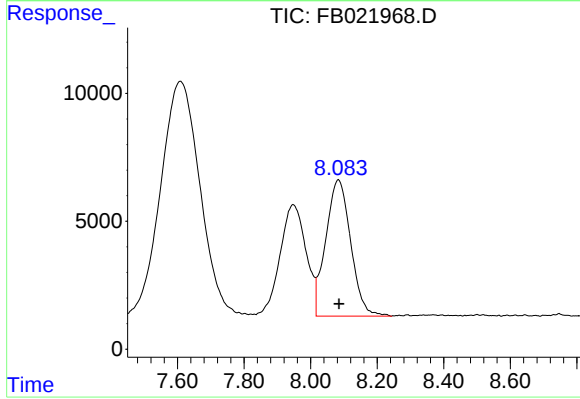


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 277376
Conc: 9.49 ng/ml

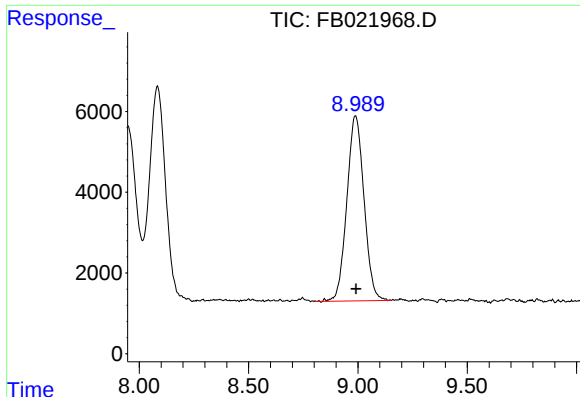


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: -0.003 min
Response: 250439
Conc: 18.35 ng/ml

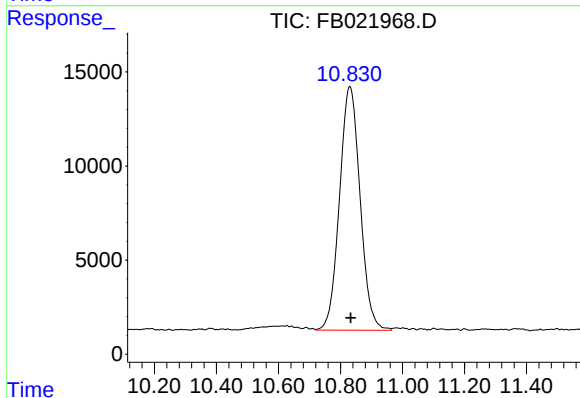


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 596921
Conc: 29.01 ng/ml

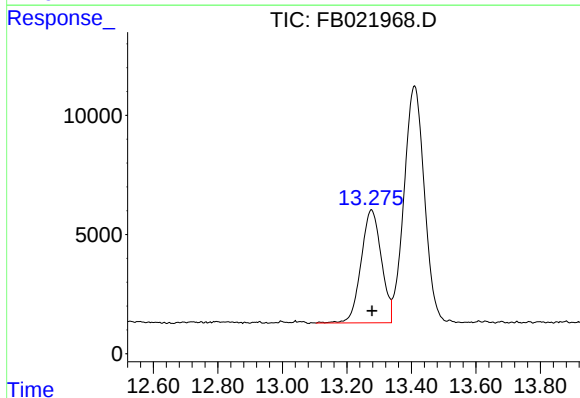


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: -0.001 min
Response: 206964
Conc: 9.95 ng/ml

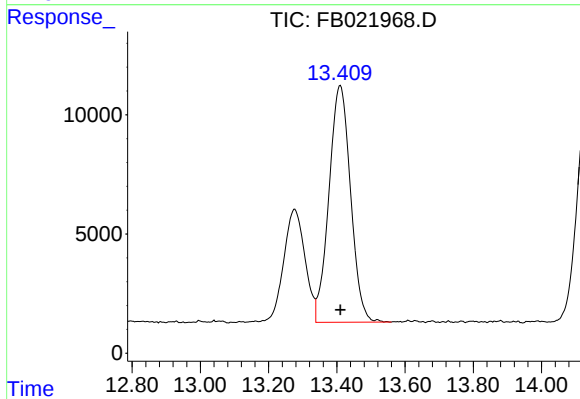

#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: 0.000 min
Response: 436460
Conc: 19.65 ng/ml

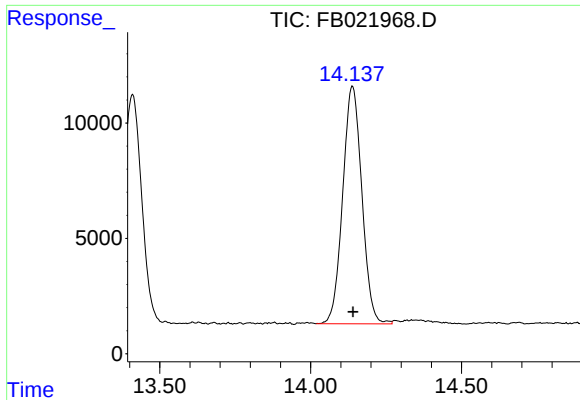


#9 O-Xylene

R.T.: 14.139 min

Delta R.T.: -0.002 min

Response: 454469

Conc: 19.76 ng/ml

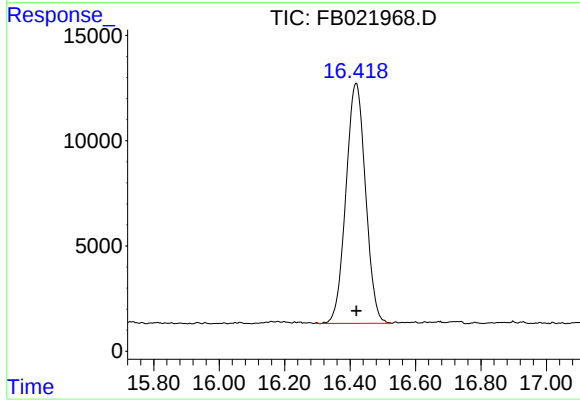

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min

Delta R.T.: 0.000 min

Response: 474541

Conc: 20.13 ng/ml