

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080919\
 Data File : FB021970.D
 Signal(s) : FID2B.CH
 Acq On : 9 Aug 2019 12:41
 Operator : DD/AJ
 Sample : K4238-07MS
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 10 01:45:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	264732	19.399 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	651233	23.616 ng/ml
2) t	2,2,4-Trimethylpentane	7.610	614728	23.255 ng/ml
3) t	n-Heptane	7.949	190807	7.696 ng/ml
4) t	Benzene	8.084	261371	8.947 ng/ml
6) t	Toluene	10.831	539092	26.200 ng/ml
7) t	Ethylbenzene	13.277	187777	9.026 ng/ml
8) t	m-Xylene	13.409	399798	17.997 ng/ml
9) t	O-Xylene	14.139	402822	17.512 ng/ml
10) t	1,2,4-Trimethylbenzene	16.418	409165	17.355 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080919\
Data File : FB021970.D
Signal(s) : FID2B.CH
Acq On : 9 Aug 2019 12:41
Operator : DD/AJ
Sample : K4238-07MS
Misc : 5.03/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 10 01:45:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

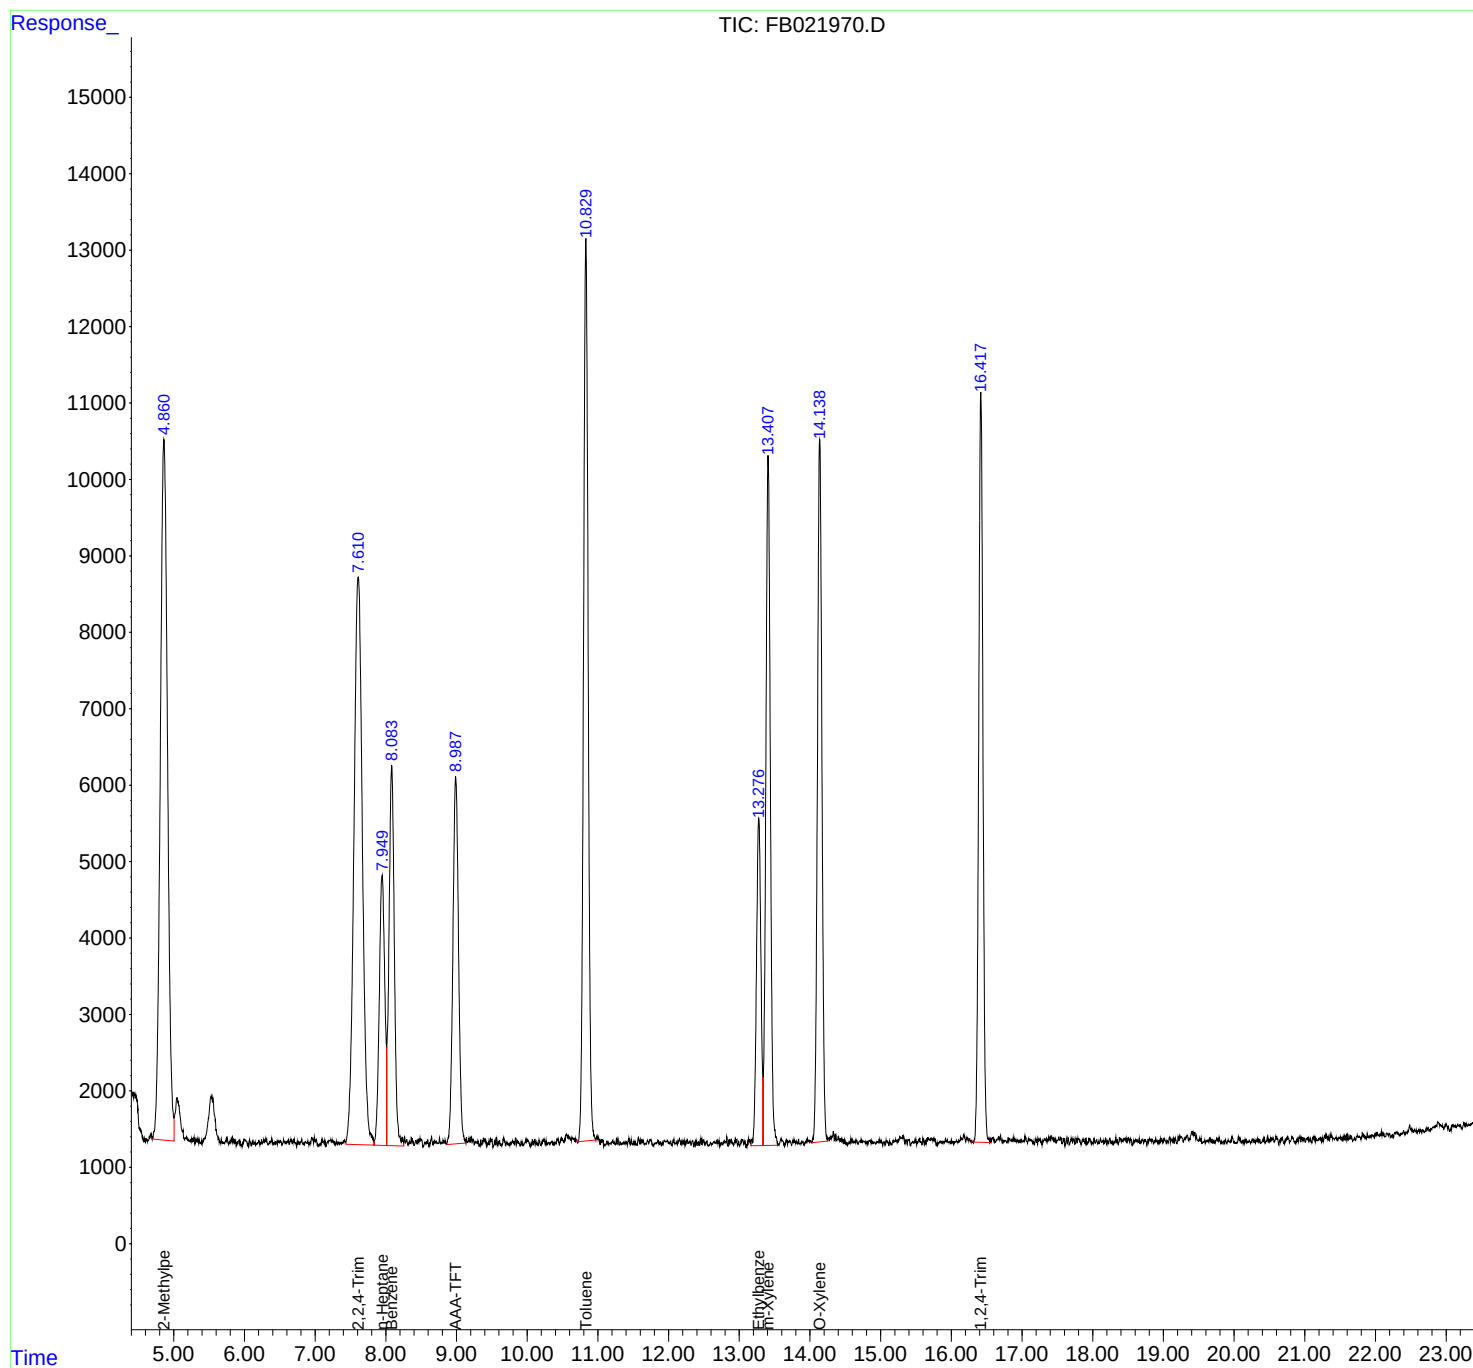

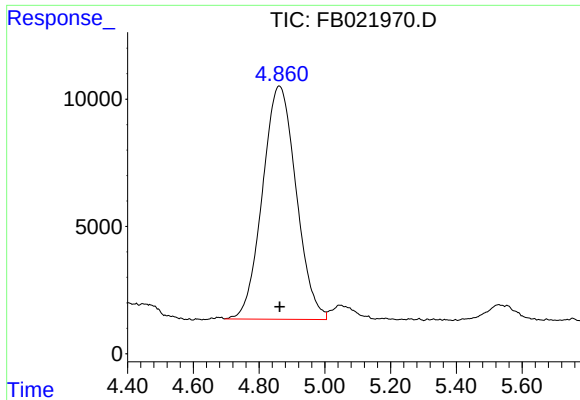


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 651233
Conc: 23.62 ng/ml

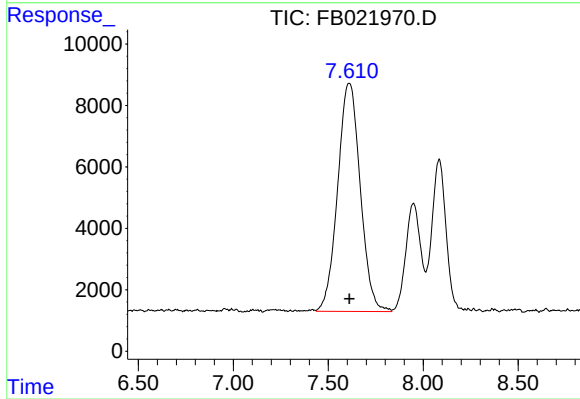


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.002 min
Response: 614728
Conc: 23.25 ng/ml

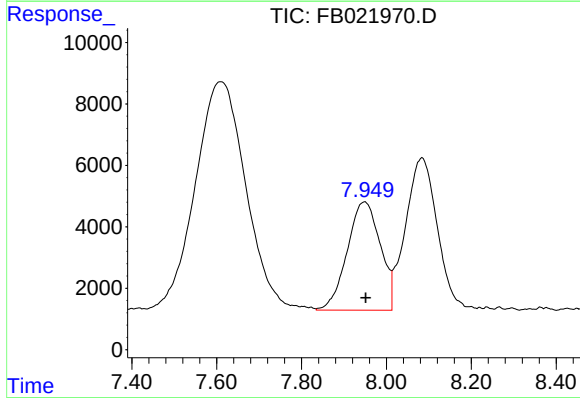


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.003 min
Response: 190807
Conc: 7.70 ng/ml

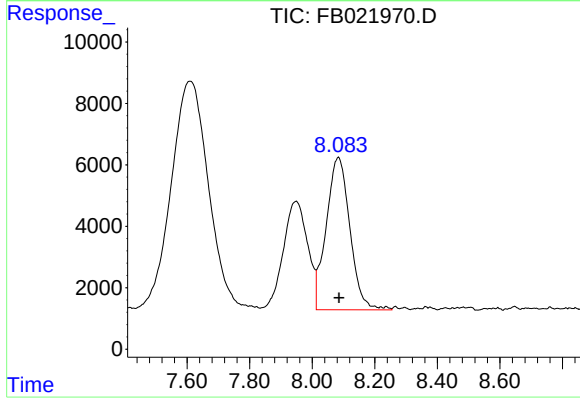


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 261371
Conc: 8.95 ng/ml

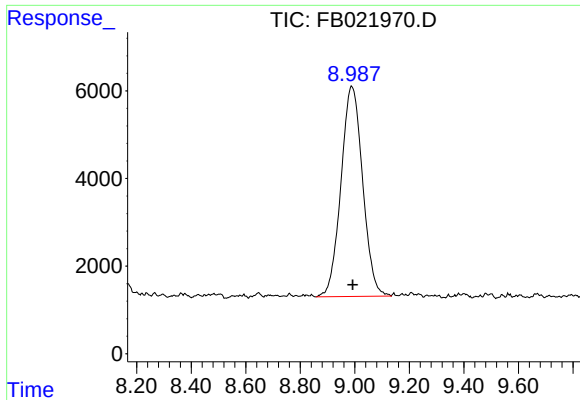


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.003 min
Response: 264732
Conc: 19.40 ng/ml

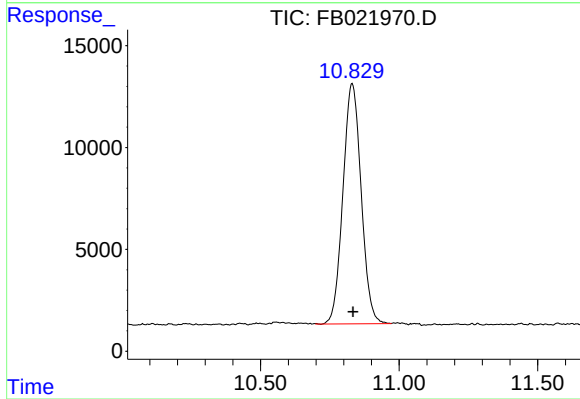


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 539092
Conc: 26.20 ng/ml

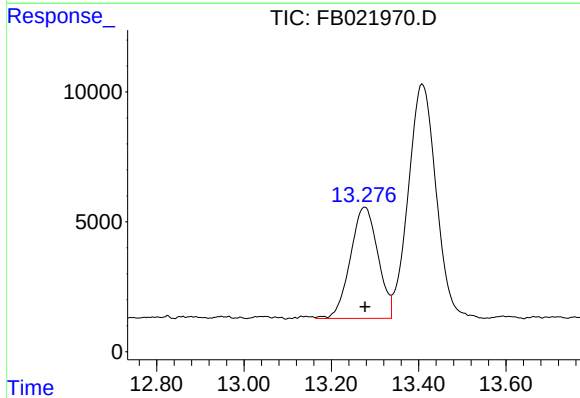


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.000 min
Response: 187777
Conc: 9.03 ng/ml

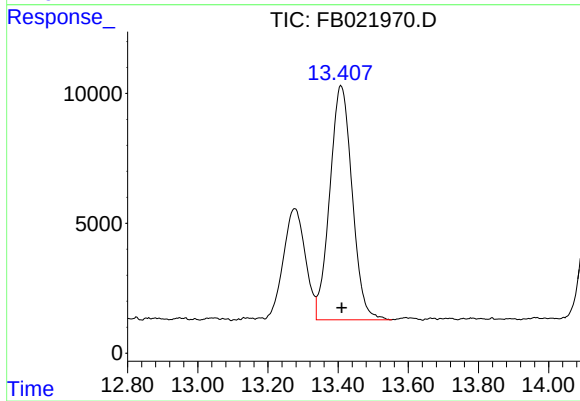


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 399798
Conc: 18.00 ng/ml

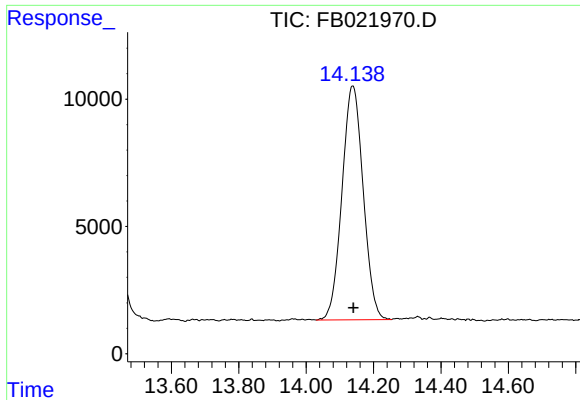

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.001 min
Response: 402822
Conc: 17.51 ng/ml

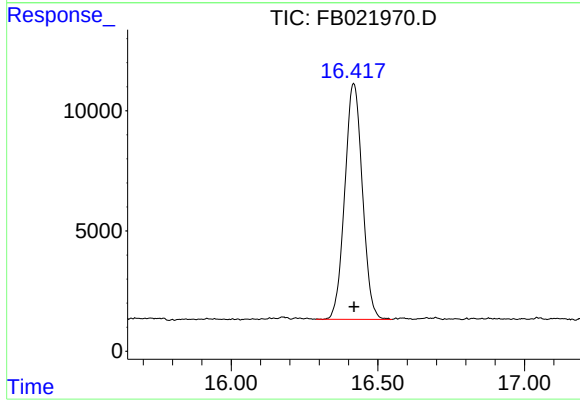

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.001 min
Response: 409165
Conc: 17.35 ng/ml