

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080919\
 Data File : FB021971.D
 Signal(s) : FID2B.CH
 Acq On : 9 Aug 2019 13:12
 Operator : DD/AJ
 Sample : K4238-07MSD
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 10 01:45:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	279333	20.469 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.863	713408	25.870 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	655591	24.801 ng/ml
3) t	n-Heptane	7.950	206926	8.346 ng/ml
4) t	Benzene	8.085	289410	9.906 ng/ml
6) t	Toluene	10.833	607222	29.511 ng/ml
7) t	Ethylbenzene	13.277	201437	9.682 ng/ml
8) t	m-Xylene	13.411	429398	19.329 ng/ml
9) t	O-Xylene	14.140	444169	19.309 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	449657	19.072 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB080919\
Data File : FB021971.D
Signal(s) : FID2B.CH
Acq On : 9 Aug 2019 13:12
Operator : DD/AJ
Sample : K4238-07MSD
Misc : 5.05/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 10 01:45:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

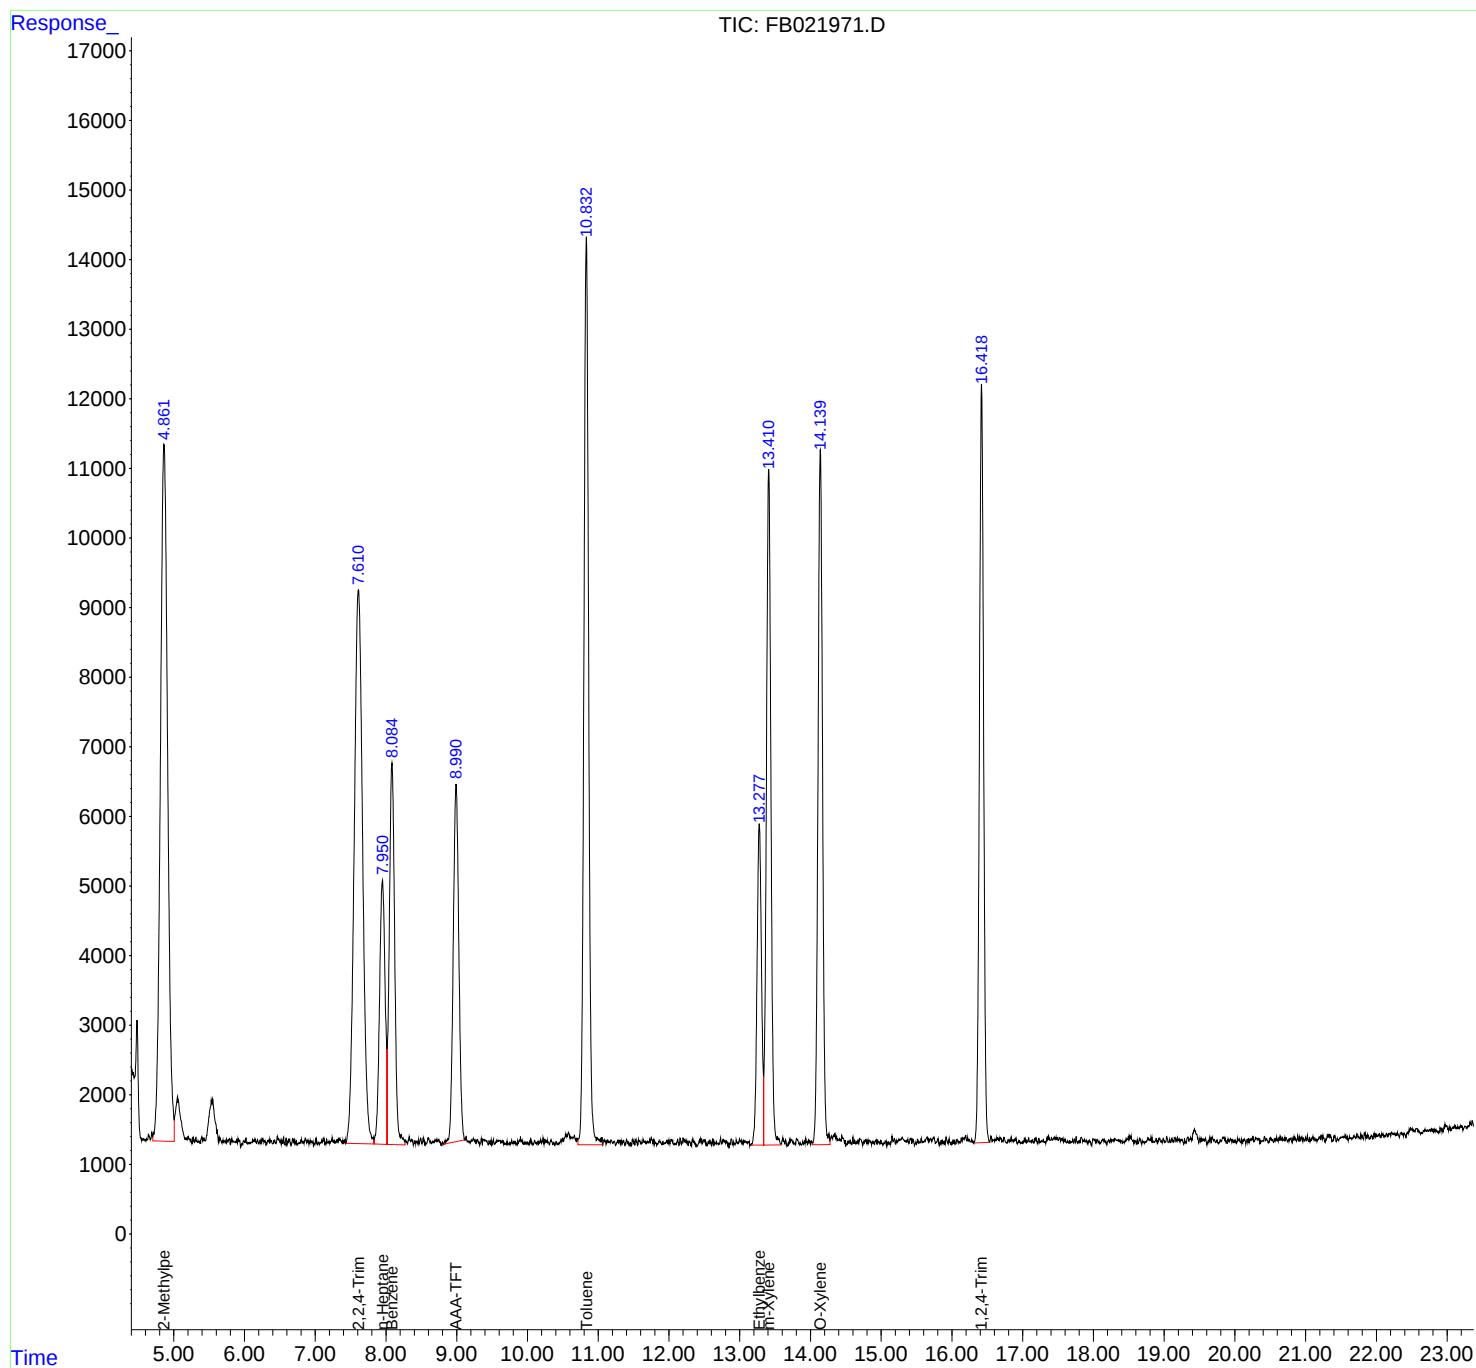

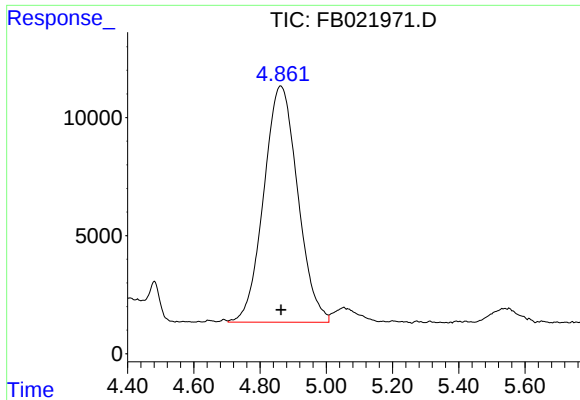


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 713408
Conc: 25.87 ng/ml

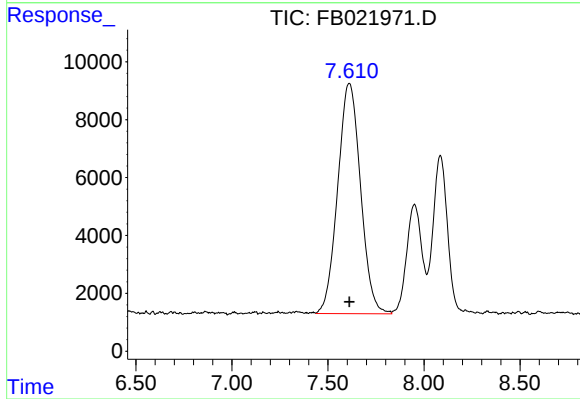


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 655591
Conc: 24.80 ng/ml

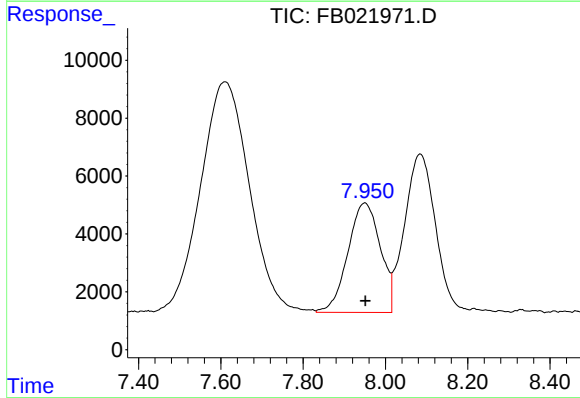


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 206926
Conc: 8.35 ng/ml

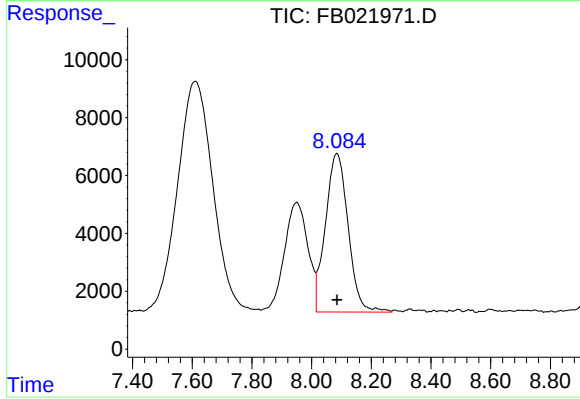


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 289410
Conc: 9.91 ng/ml

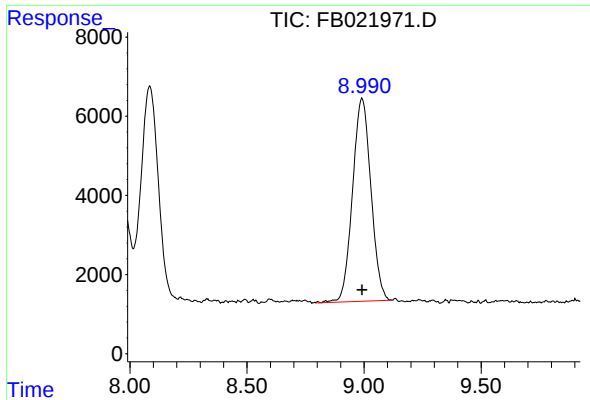


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 279333
Conc: 20.47 ng/ml

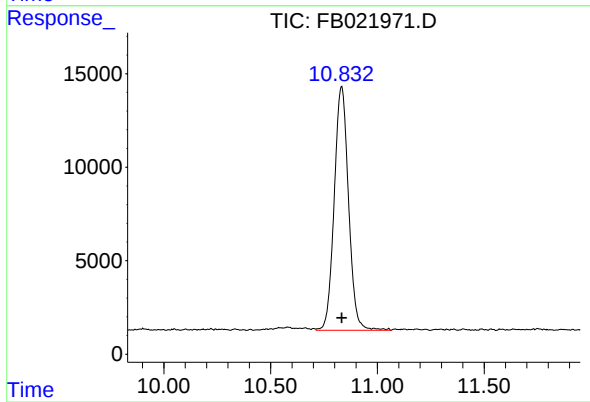


#6 Toluene

R.T.: 10.833 min
Delta R.T.: 0.000 min
Response: 607222
Conc: 29.51 ng/ml

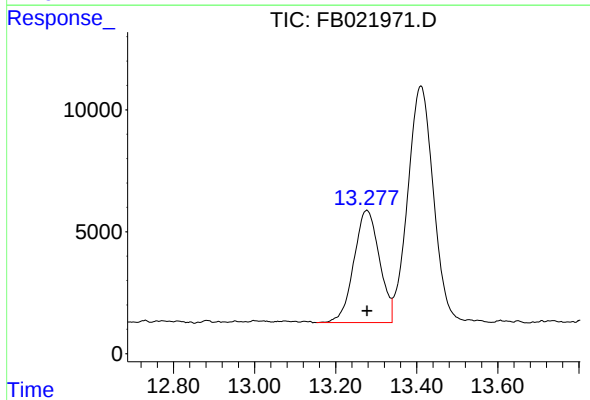


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.000 min
Response: 201437
Conc: 9.68 ng/ml

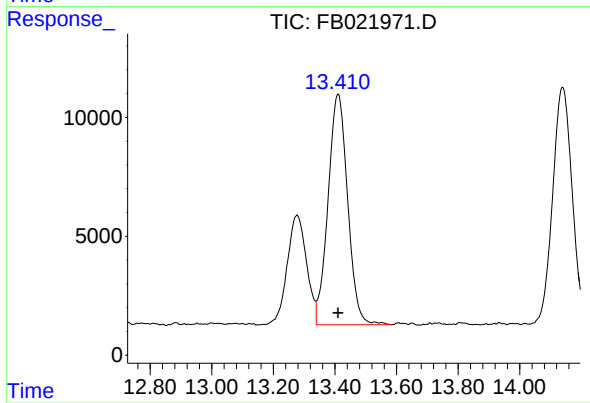


#8 m-Xylene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 429398
Conc: 19.33 ng/ml

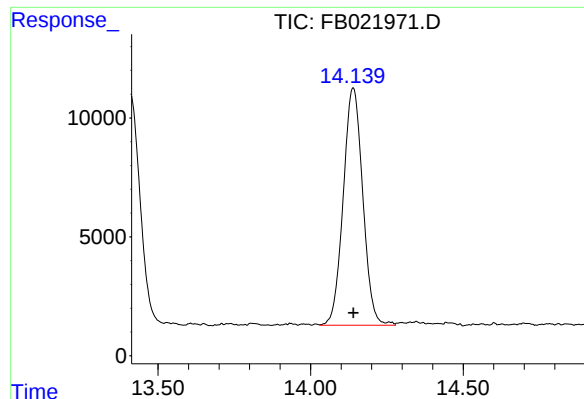

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.000 min
Response: 444169
Conc: 19.31 ng/ml

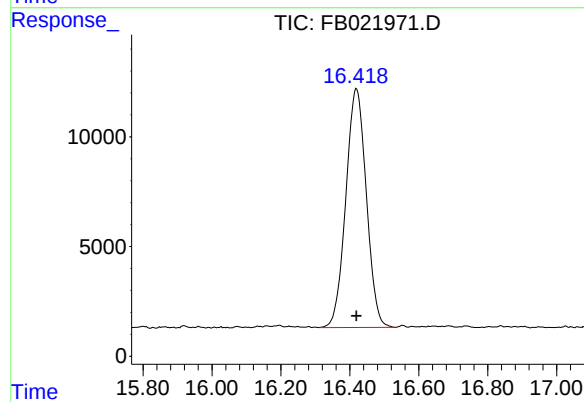

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.000 min
Response: 449657
Conc: 19.07 ng/ml