

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081020\
Data File : FB024736.D
Signal(s) : FID2B.CH
Acq On : 10 Aug 2020 13:57
Operator : DD/AJ
Sample : VBF0810S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 11 00:42:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	387031	18.743 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.398	1030	0.037 ng/ml
6) t	Toluene	10.637	5528	0.160 ng/ml
9) t	O-Xylene	13.919	1795	0.059 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	1898	0.077 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081020\
Data File : FB024736.D
Signal(s) : FID2B.CH
Acq On : 10 Aug 2020 13:57
Operator : DD/AJ
Sample : VBF0810S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 11 00:42:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

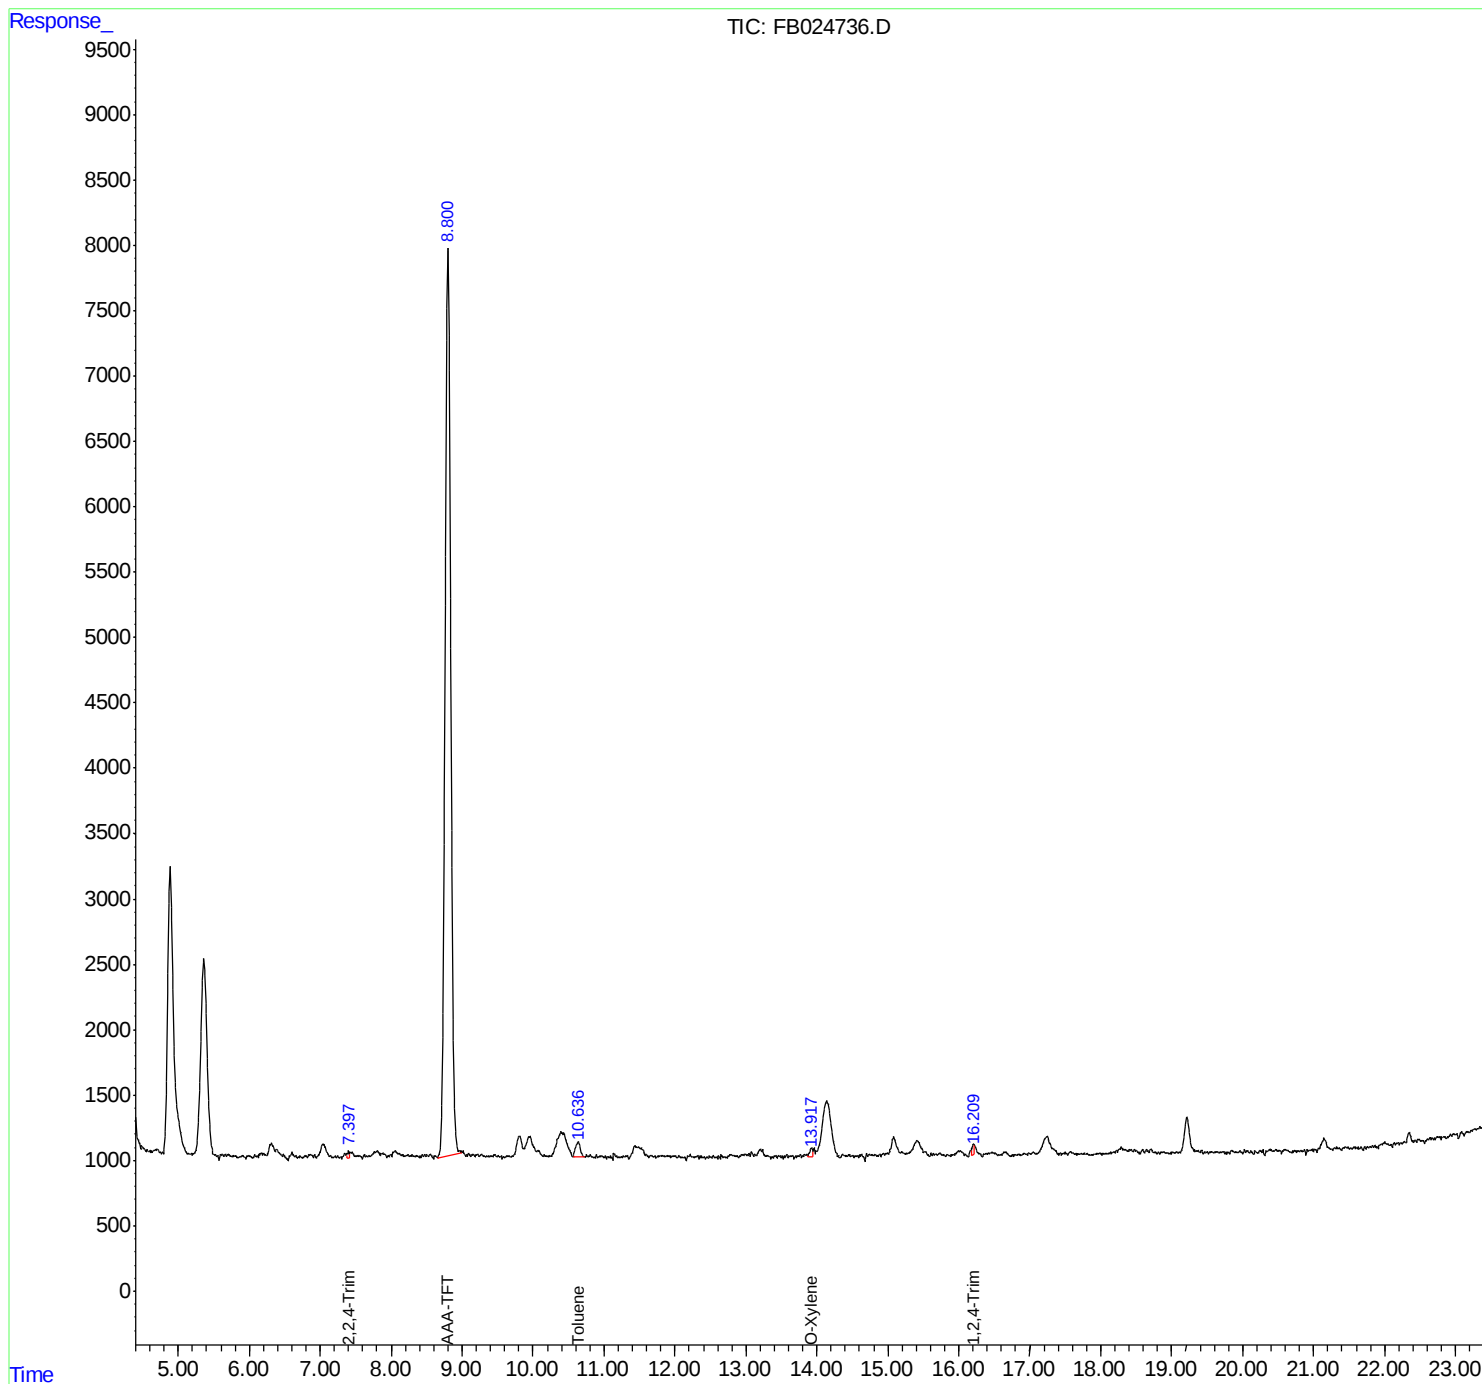

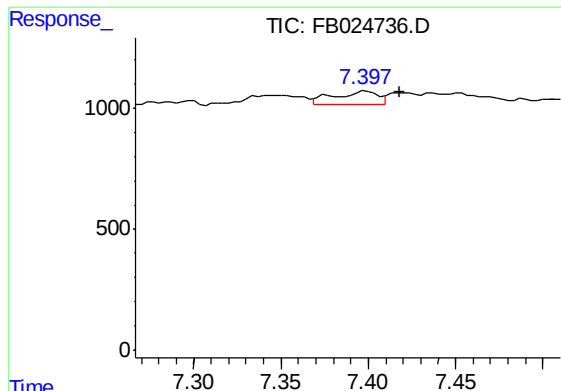


#2 2,2,4-Trimethylpentane

R.T.: 7.398 min
Delta R.T.: -0.019 min
Response: 1030
Conc: 0.04 ng/ml

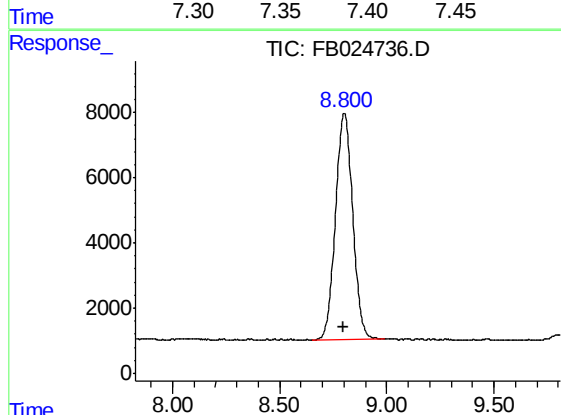


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 387031
Conc: 18.74 ng/ml

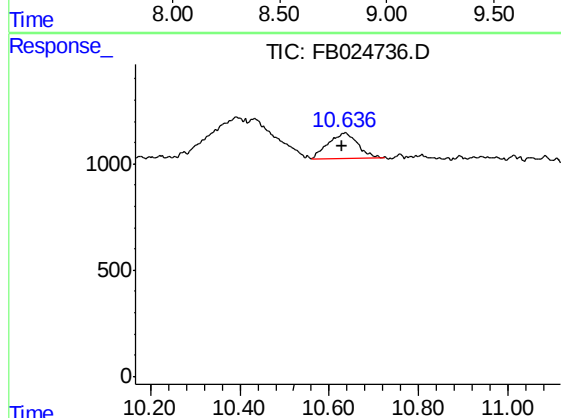

#6 Toluene

R.T.: 10.637 min
Delta R.T.: 0.007 min
Response: 5528
Conc: 0.16 ng/ml

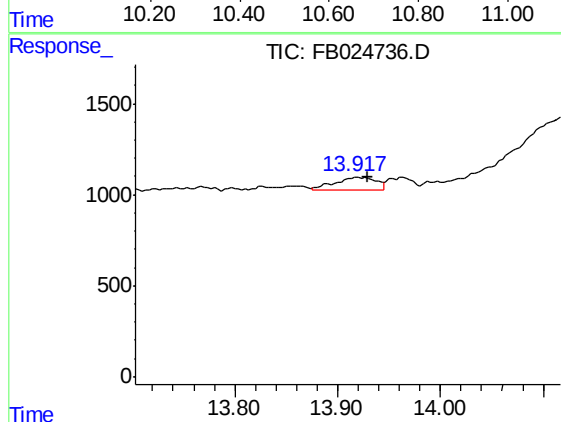

#9 O-Xylene


R.T.: 13.919 min
Delta R.T.: -0.011 min
Response: 1795
Conc: 0.06 ng/ml

Response_

TIC: FB024736.D

#10 1,2,4-Trimethylbenzene

Time

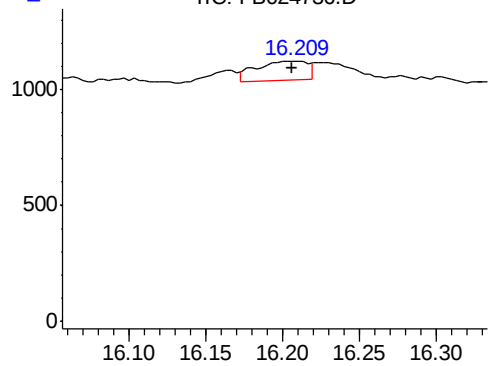

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 1898
Conc: 0.08 ng/ml