

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081121\
 Data File : FB026137.D
 Signal(s) : FID2B.CH
 Acq On : 11 Aug 2021 13:52
 Operator : AJ/MA
 Sample : BSF0811S2
 Misc : 4.99G\5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 12 01:10:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
 Quant Title :
 QLast Update : Tue Jul 27 12:01:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.845	452780	16.316 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.845	808018	24.618 ng/ml
2) t 2,2,4-Trimethylpentane	7.506	767208	23.568 ng/ml
3) t n-Heptane	7.820	357779	7.736 ng/ml
4) t Benzene	7.959	379435	7.809 ng/ml
6) t Toluene	10.654	1060522	23.299 ng/ml
7) t Ethylbenzene	13.073	293814	7.701 ng/ml
8) t m-Xylene	13.205	559085	15.507 ng/ml
9) t O-Xylene	13.930	483727	15.602 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	388517	15.146 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081121\
Data File : FB026137.D
Signal(s) : FID2B.CH
Acq On : 11 Aug 2021 13:52
Operator : AJ/MA
Sample : BSF0811S2
Misc : 4.99G\5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 12 01:10:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
Quant Title :
QLast Update : Tue Jul 27 12:01:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

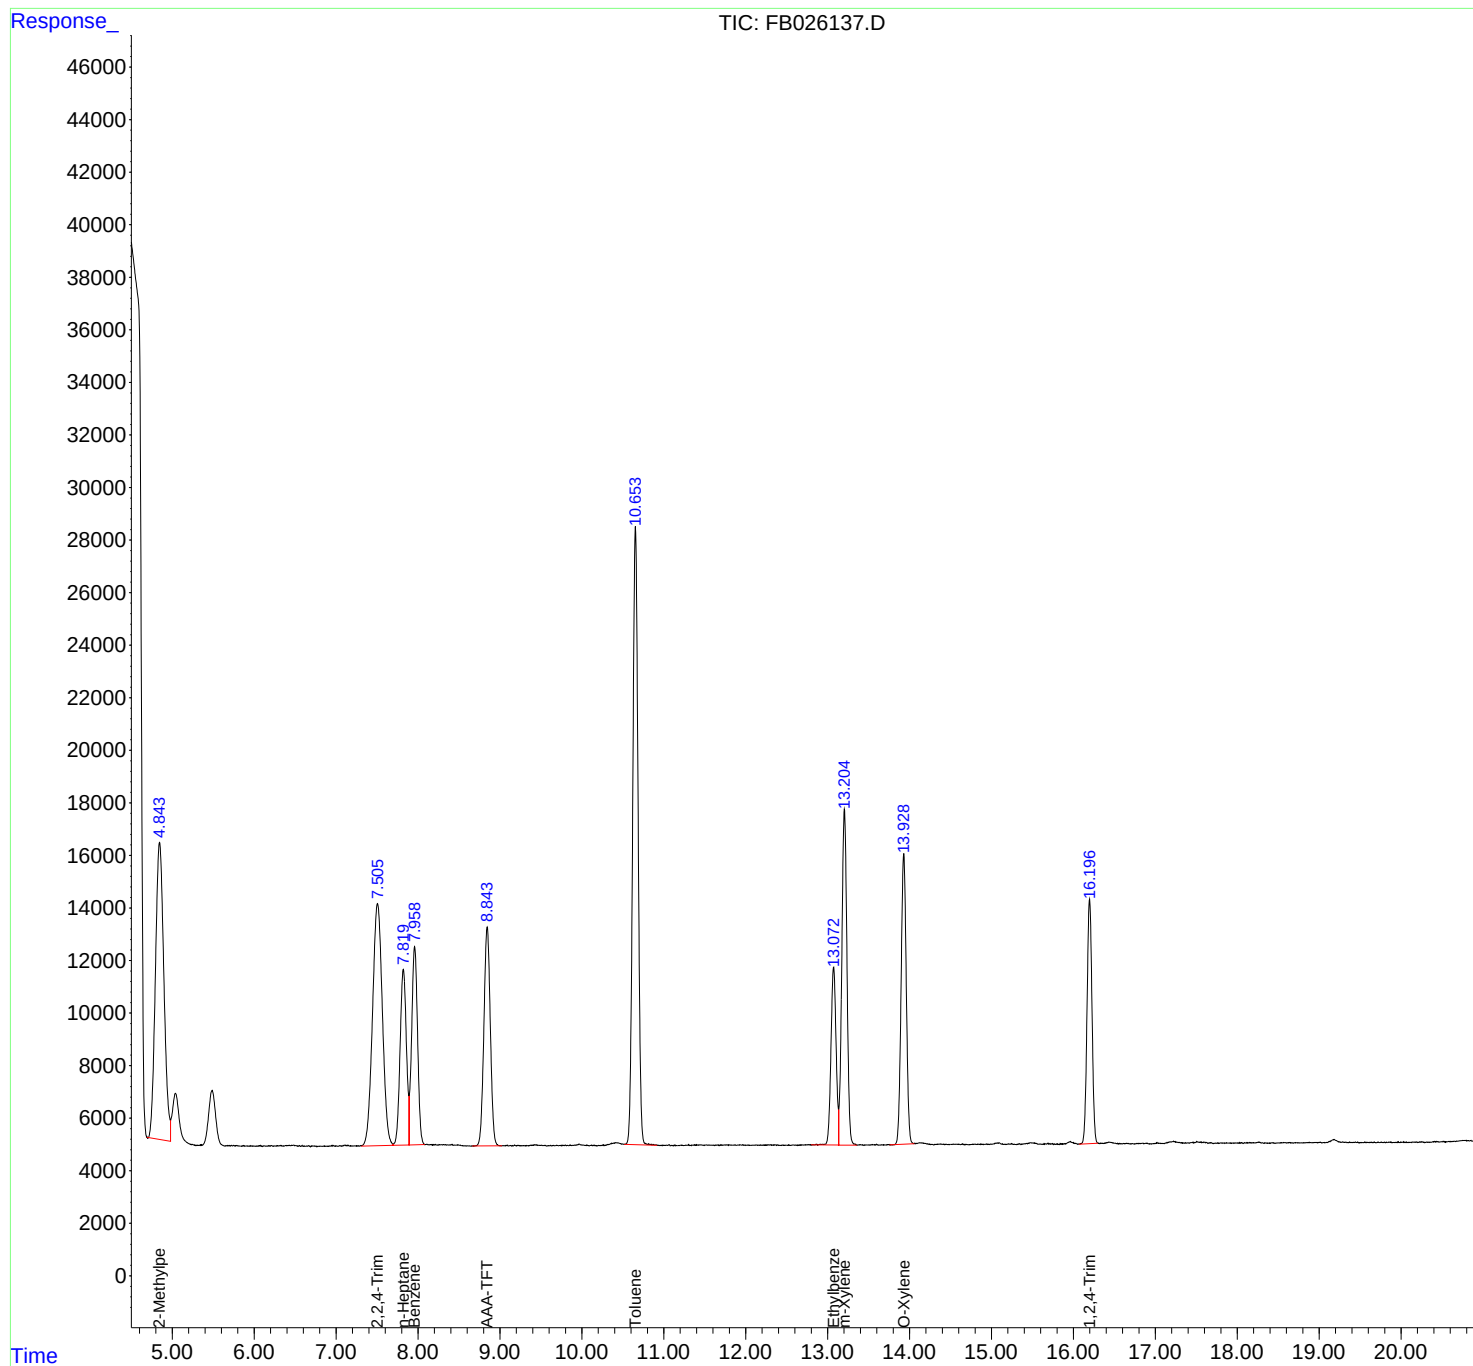


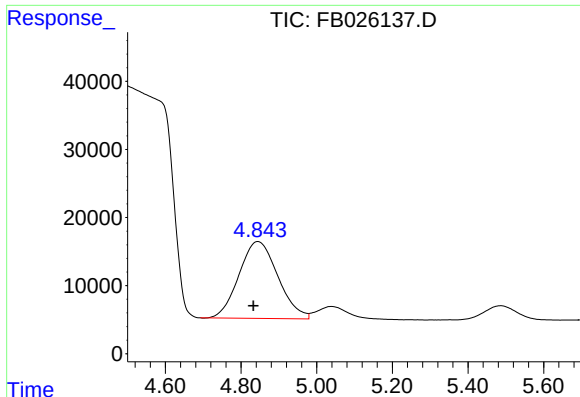

#1 2-Methylpentane


R.T.: 4.845 min
Delta R.T.: 0.012 min
Response: 808018
Conc: 24.62 ng/ml

Instrument :
FID_B
ClientSampleId :

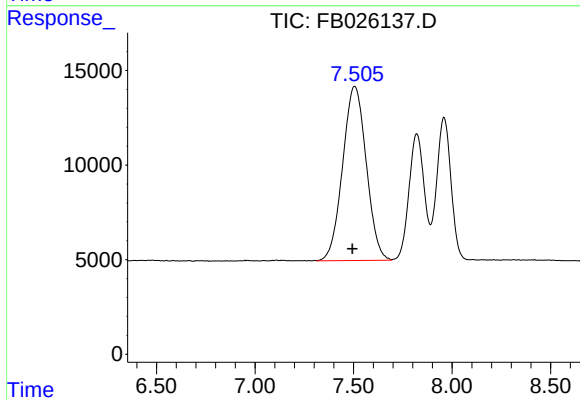


#2 2,2,4-Trimethylpentane

R.T.: 7.506 min
Delta R.T.: 0.012 min
Response: 767208
Conc: 23.57 ng/ml

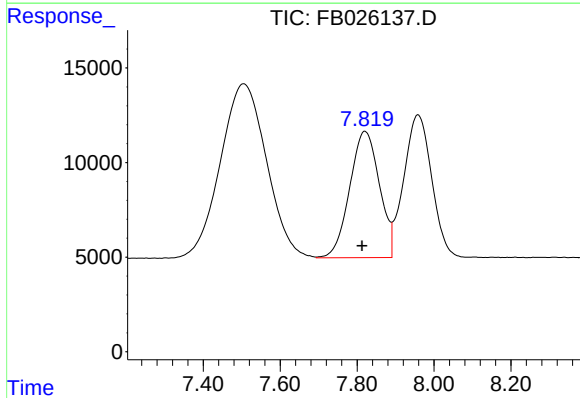


#3 n-Heptane

R.T.: 7.820 min
Delta R.T.: 0.008 min
Response: 357779
Conc: 7.74 ng/ml

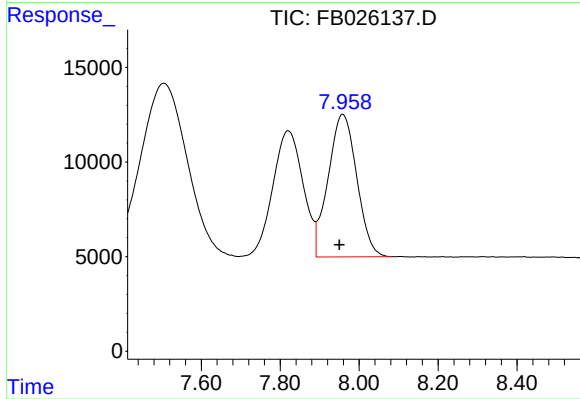

#4 Benzene


R.T.: 7.959 min
Delta R.T.: 0.009 min
Response: 379435
Conc: 7.81 ng/ml

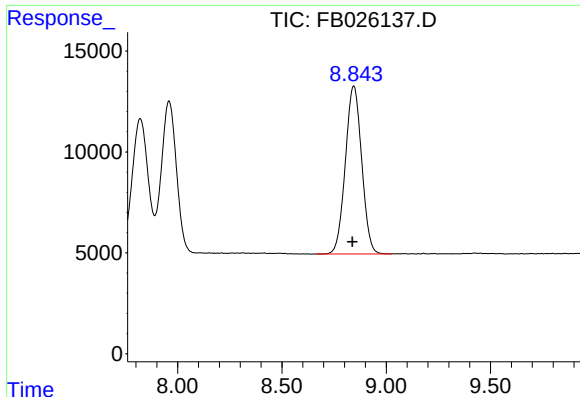

#5 AAA-TFT


R.T.: 8.845 min
Delta R.T.: 0.007 min
Response: 452780
Conc: 16.32 ng/ml

Instrument :
FID_B
ClientSampleId :

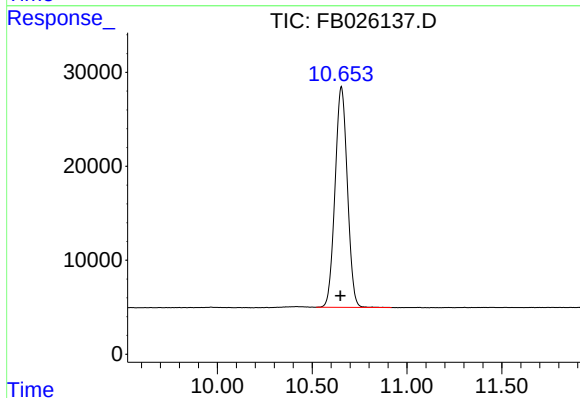


#6 Toluene

R.T.: 10.654 min
Delta R.T.: 0.006 min
Response: 1060522
Conc: 23.30 ng/ml

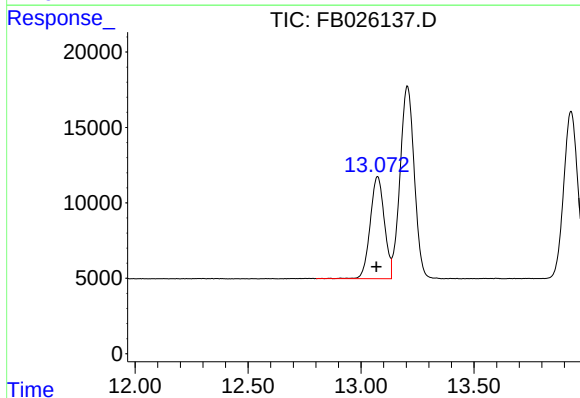


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.005 min
Response: 293814
Conc: 7.70 ng/ml

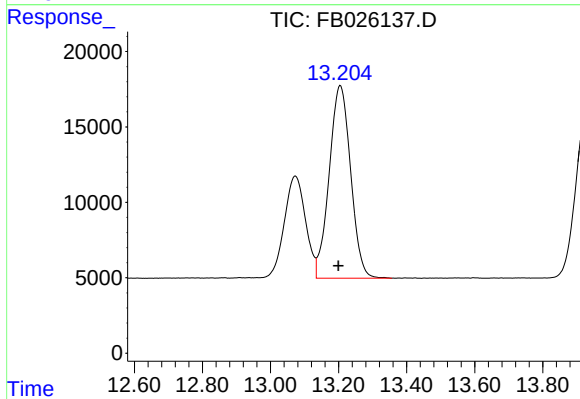

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.005 min
Response: 559085
Conc: 15.51 ng/ml

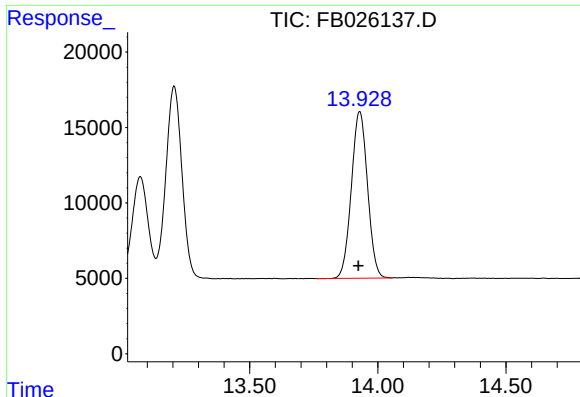

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.005 min
Response: 483727
Conc: 15.60 ng/ml

Instrument :
FID_B
ClientSampleId :

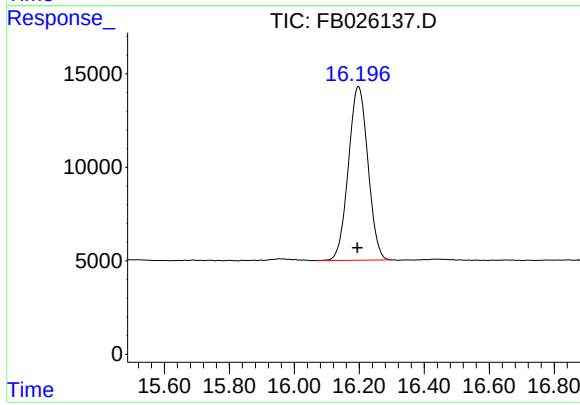

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.004 min
Response: 388517
Conc: 15.15 ng/ml