

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081121\
 Data File : FB026138.D
 Signal(s) : FID2B.CH
 Acq On : 11 Aug 2021 14:37
 Operator : AJ/MA
 Sample : M3326-01
 Misc : 6.70G\5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 12 01:10:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
 Quant Title :
 QLast Update : Tue Jul 27 12:01:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.871	1675892	60.392 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.853	946854	28.848 ng/ml
2) t 2,2,4-Trimethylpentane	7.518	5203407	159.845 ng/ml
3) t n-Heptane	7.821	870616	18.825 ng/ml
7) t Ethylbenzene	13.043	558519	14.639 ng/ml
8) t m-Xylene	13.184	205527	5.700 ng/ml
9) t O-Xylene	13.930	94994	3.064 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	56187	2.190 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081121\
Data File : FB026138.D
Signal(s) : FID2B.CH
Acq On : 11 Aug 2021 14:37
Operator : AJ/MA
Sample : M3326-01
Misc : 6.70G\5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 12 01:10:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072721.M
Quant Title :
QLast Update : Tue Jul 27 12:01:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

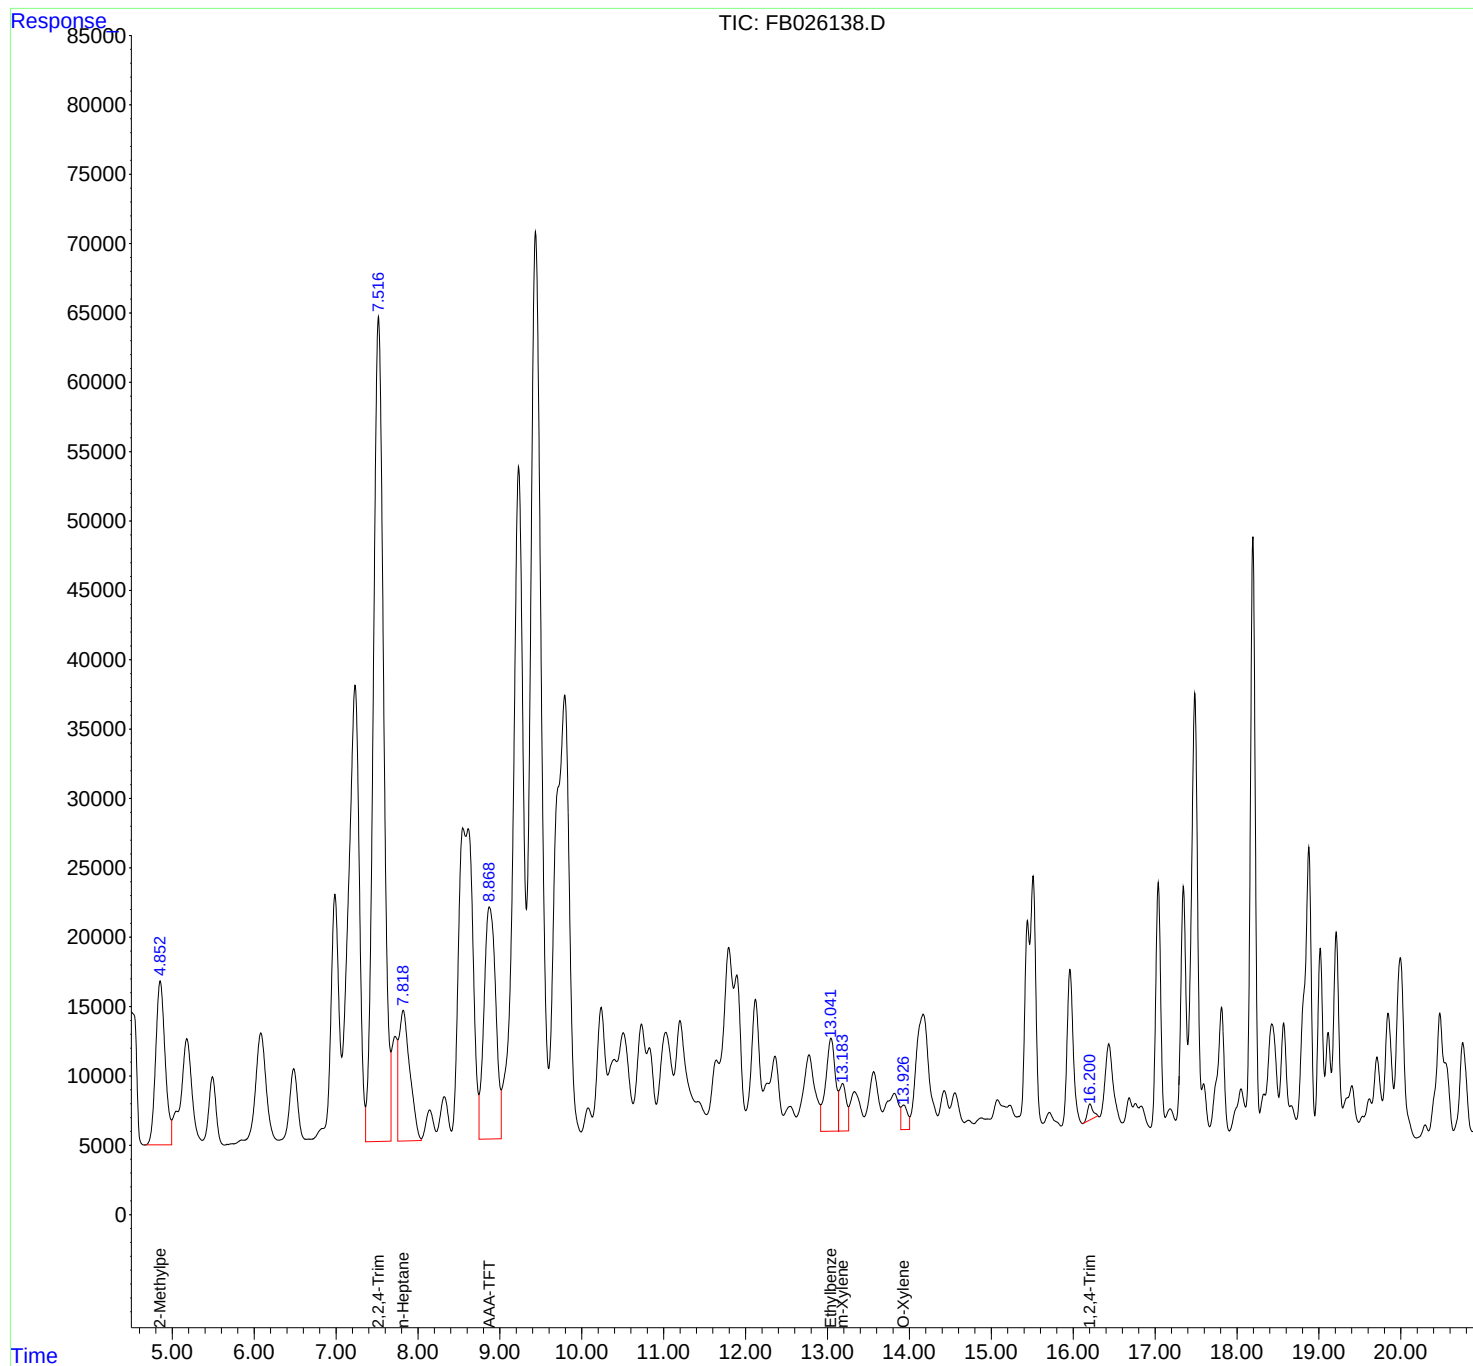


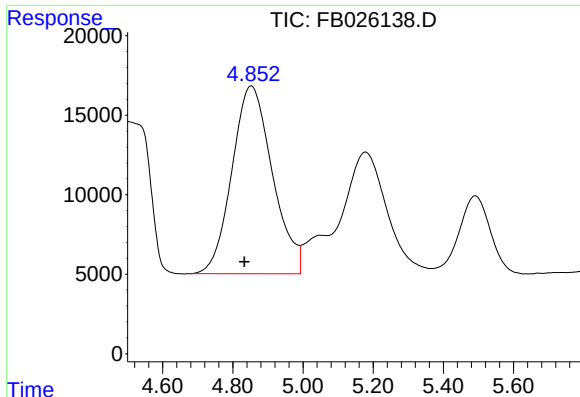

#1 2-Methylpentane


R.T.: 4.853 min
Delta R.T.: 0.020 min
Response: 946854
Conc: 28.85 ng/ml

Instrument :
FID_B
ClientSampleId :

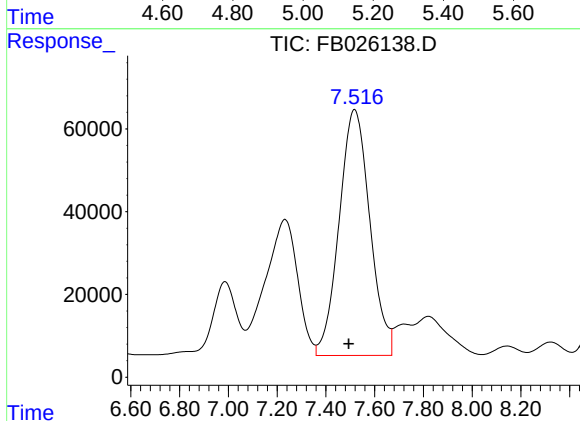


#2 2,2,4-Trimethylpentane

R.T.: 7.518 min
Delta R.T.: 0.024 min
Response: 5203407
Conc: 159.84 ng/ml

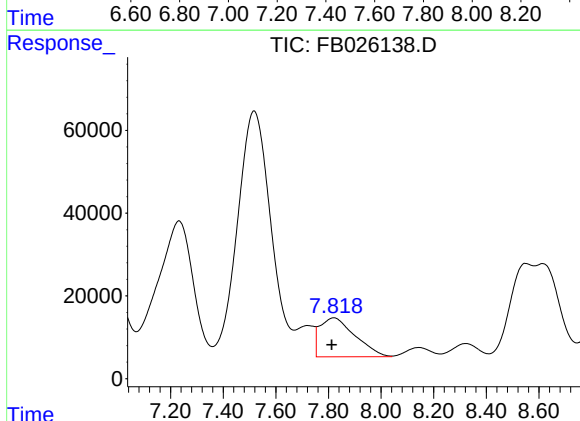


#3 n-Heptane

R.T.: 7.821 min
Delta R.T.: 0.008 min
Response: 870616
Conc: 18.82 ng/ml

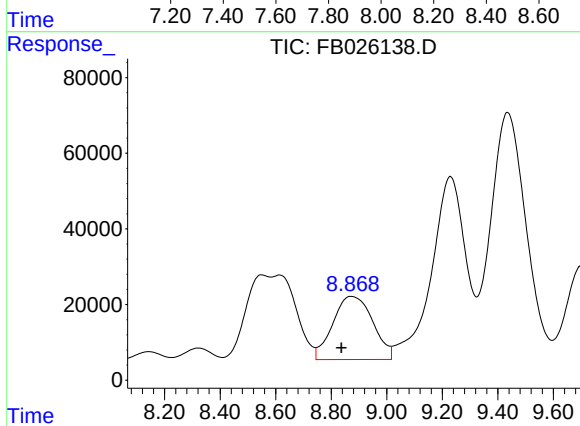

#5 AAA-TFT


R.T.: 8.871 min
Delta R.T.: 0.034 min
Response: 1675892
Conc: 60.39 ng/ml

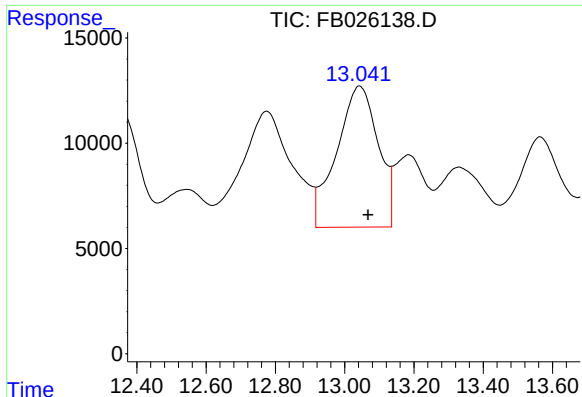

#7 Ethylbenzene


R.T.: 13.043 min
Delta R.T.: -0.025 min
Response: 558519
Conc: 14.64 ng/ml

Instrument :
FID_B
ClientSampleId :

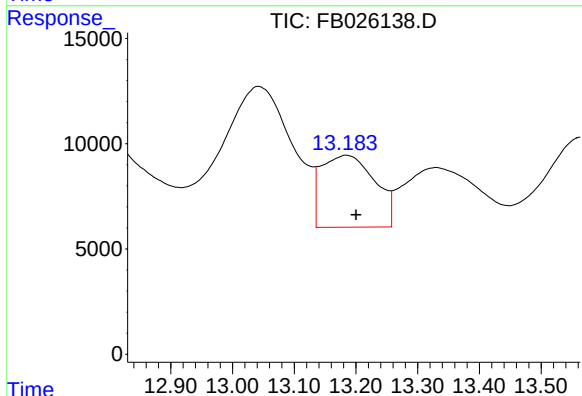


#8 m-Xylene

R.T.: 13.184 min
Delta R.T.: -0.016 min
Response: 205527
Conc: 5.70 ng/ml

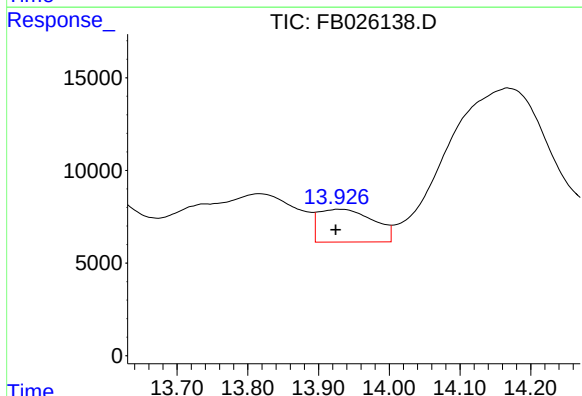

#9 o-Xylene

R.T.: 13.930 min
Delta R.T.: 0.005 min
Response: 94994
Conc: 3.06 ng/ml

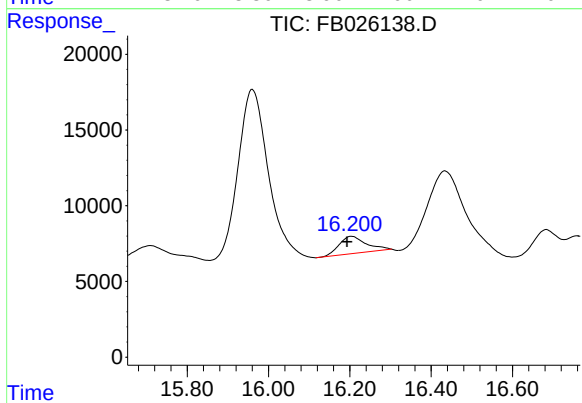

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.011 min
Response: 56187
Conc: 2.19 ng/ml